

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034639.D
 Acq On : 13 Apr 2022 02:33
 Operator : CG/JU
 Sample : N2319-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2J6

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 13 05:11:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.884	152	2570	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.688	136	7168	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.525	164	3942	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.267	188	7435	0.400	ng/ul	-0.02
17) Chrysene-d12	21.477	240	6282	0.400	ng/ul	# 0.00
23) Perylene-d12	23.815	264	3713m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	15841m	3.556	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.294	152	3865	0.407	ng/ul	-0.01
18) Fluoranthene-d10	19.294	212	9868	0.540	ng/ul	-0.01
Target Compounds						
2) 1,4-Dioxane	3.290	88	438m	0.099	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034639.D
Acq On : 13 Apr 2022 02:33
Operator : CG/JU
Sample : N2319-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2J6


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 13 05:11:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

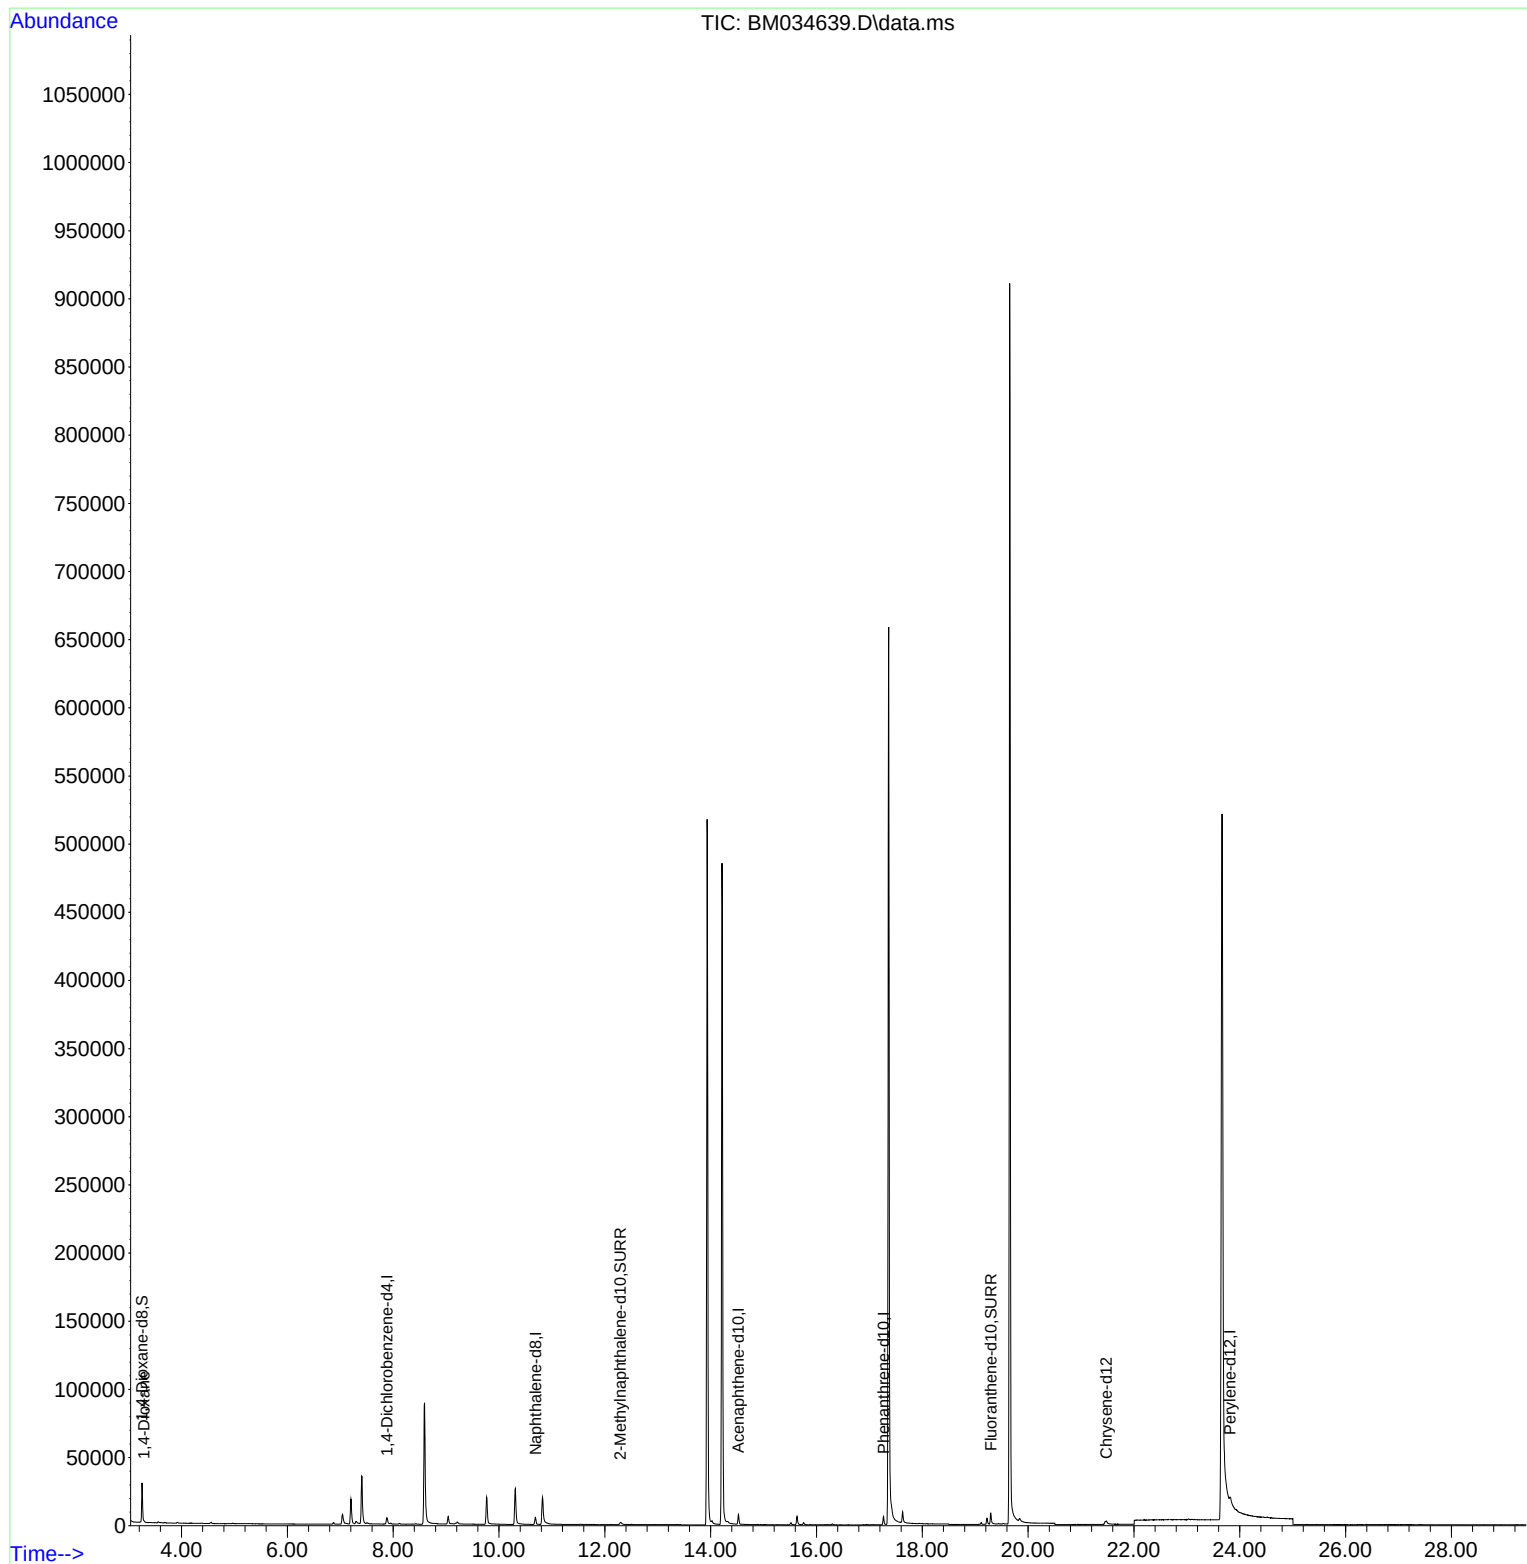


Abundance Scan 62 (3.294 min): BM034630.D\data.ms (-56)

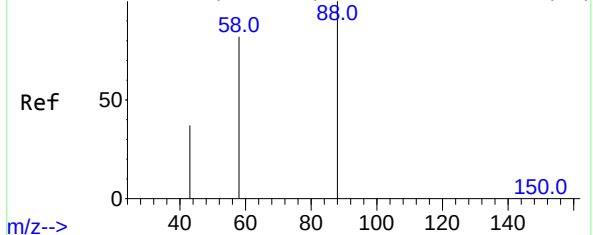


m/z-->

Abundance Scan 61 (3.290 min): BM034639.D\data.ms

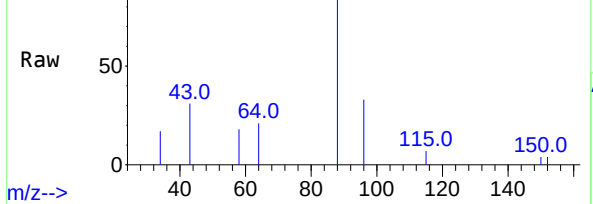

m/z-->


Abundance Scan 61 (3.290 min): BM034639.D\data.ms (-49)

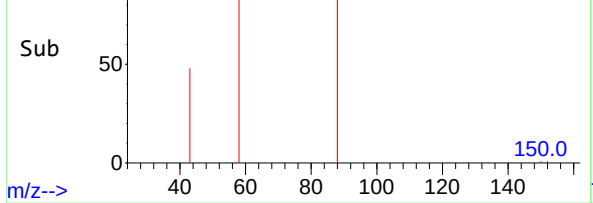

m/z-->

#2
1,4-Dioxane
Concen: 0.099 ng/ul m
RT: 3.290 min Scan# 61
Delta R.T. -0.000 min
Lab File: BM034639.D
Acq: 13 Apr 2022 02:33

Tgt Ion: 88	Resp: 438
Ion Ratio	Lower Upper
88	100
43	30.8 49.7 74.5
58	17.9 52.5 78.7

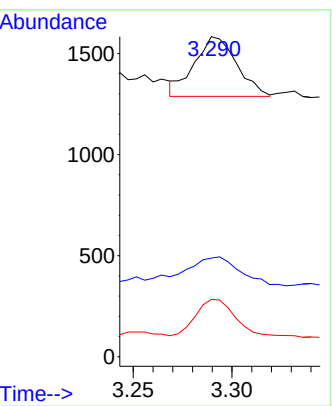

Instrument :
BNA_M
ClientSampleId :
YB2J6

Manual Integrations
APPROVED
Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022