

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034644.D
 Acq On : 13 Apr 2022 05:34
 Operator : CG/JU
 Sample : N2319-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
 Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 13 07:11:37 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	2291	0.400	ng/u1	-0.03
4) Naphthalene-d8	10.683	136	6393	0.400	ng/u1	#-0.02
9) Acenaphthene-d10	14.525	164	3502	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.267	188	6651m	0.400	ng/u1	-0.02
17) Chrysene-d12	21.480	240	5291	0.400	ng/u1	# 0.01
23) Perylene-d12	23.812	264	2328m	0.400	ng/u1	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	13971	3.518	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.305	152	3371	0.398	ng/u1	0.00
18) Fluoranthene-d10	19.294	212	8339	0.542	ng/u1	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.290	88	519m	0.132	ng/u1	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034644.D
Acq On : 13 Apr 2022 05:34
Operator : CG/JU
Sample : N2319-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YB2H2


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 13 07:11:37 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

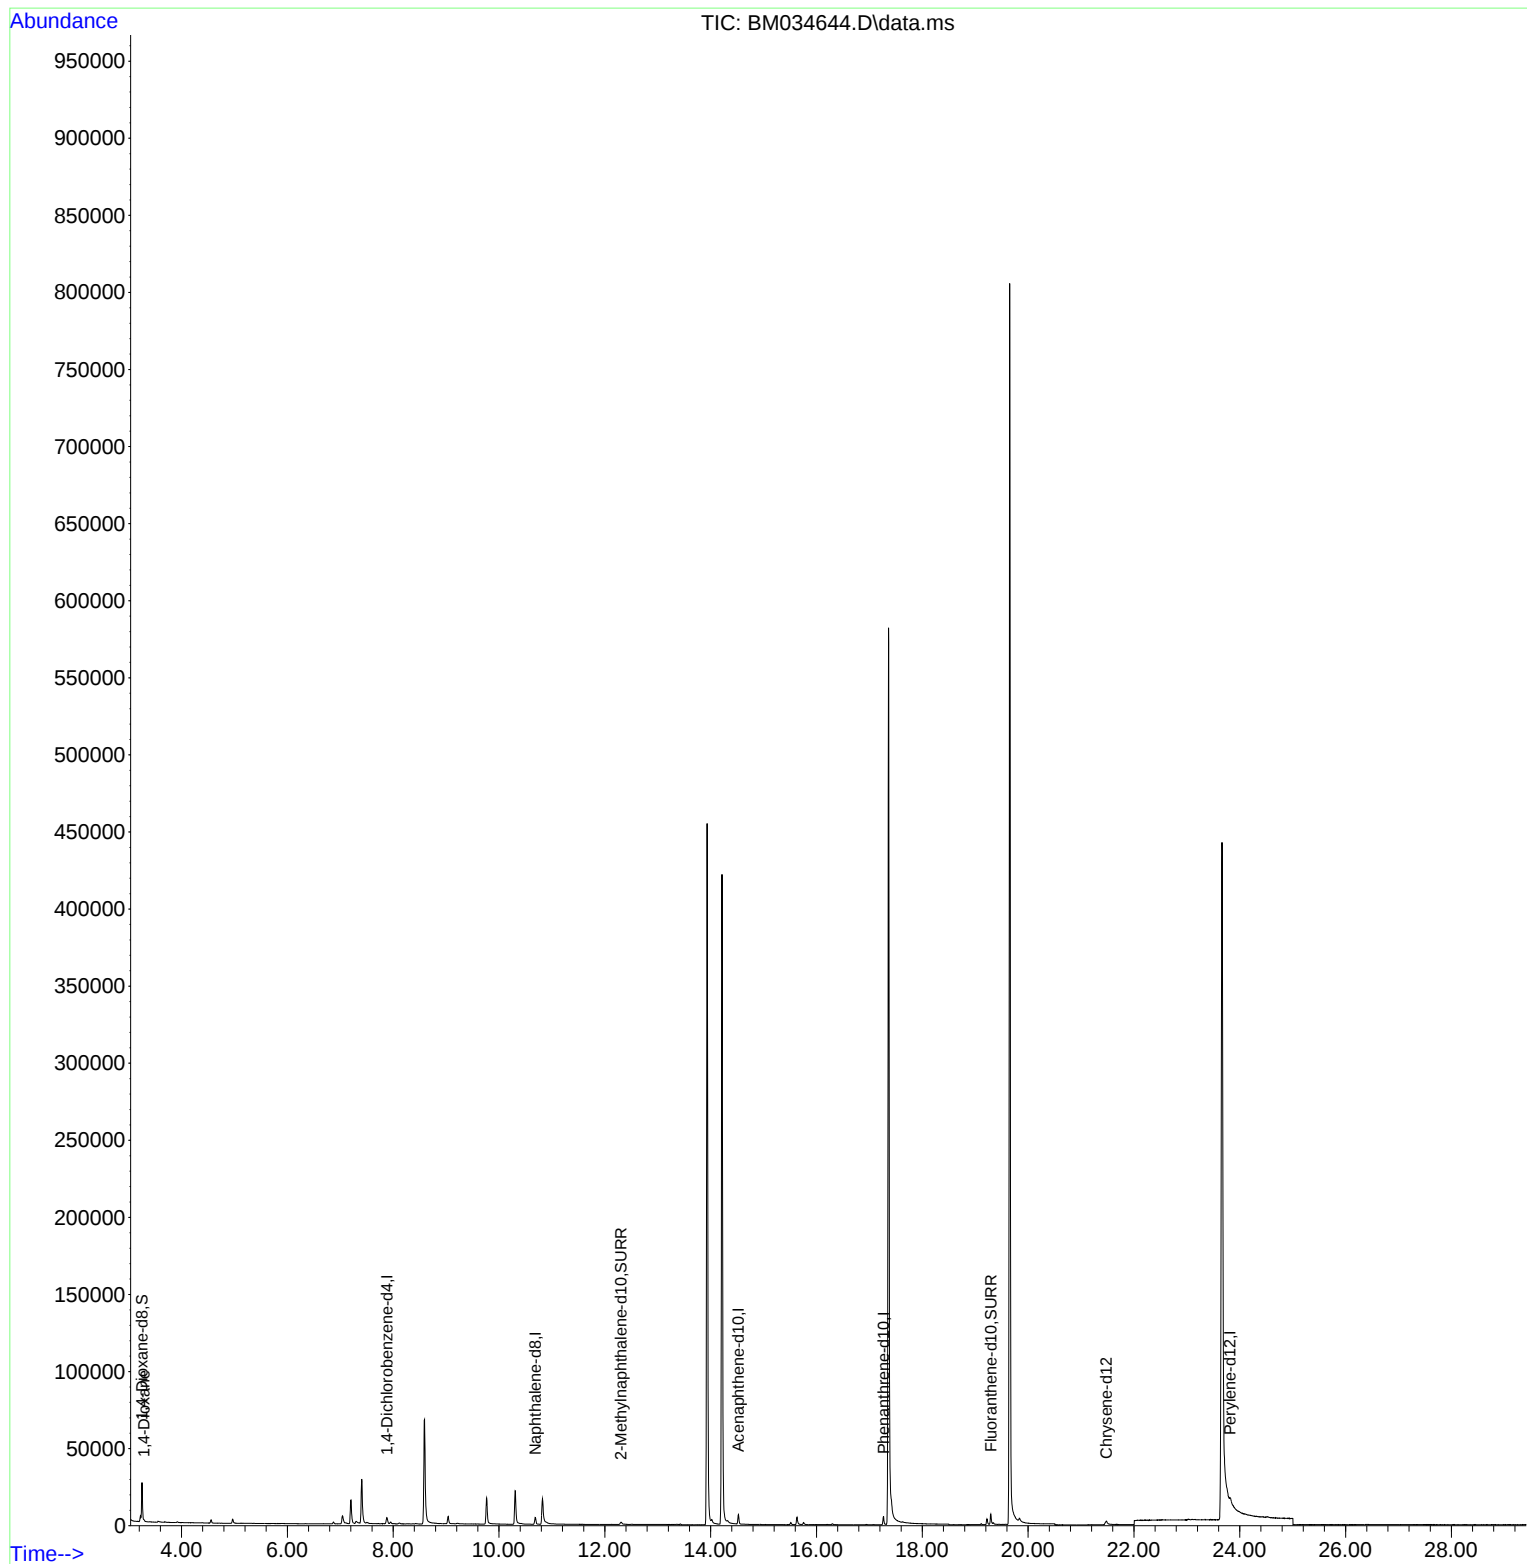


Abundance Scan 62 (3.294 min): BM034630.D\data.ms (-56)

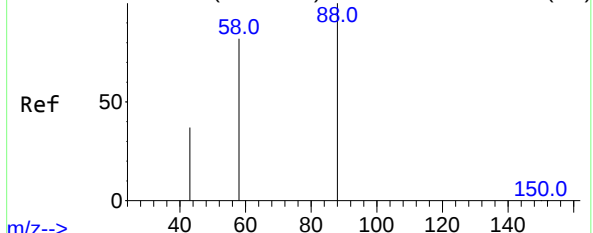


m/z-->

Abundance Scan 61 (3.290 min): BM034644.D\data.ms

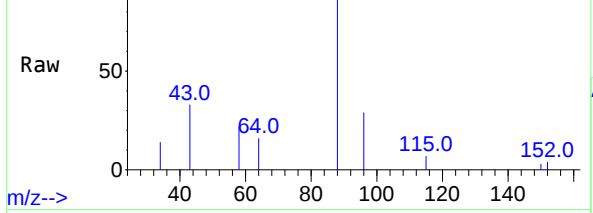

m/z-->

Abundance Scan 61 (3.290 min): BM034644.D\data.ms (-49)

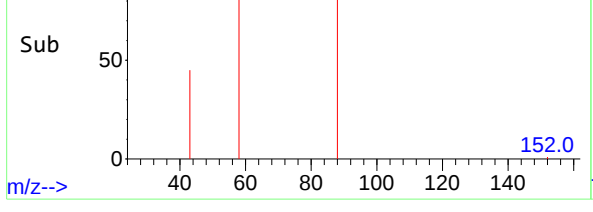

m/z-->

#2
1,4-Dioxane
Concen: 0.132 ng/ul m
RT: 3.290 min Scan# 61
Delta R.T. -0.000 min
Lab File: BM034644.D
Acq: 13 Apr 2022 05:34

Tgt Ion: 88	Resp: 519
Ion Ratio	Lower Upper
88	100
43	33.0 49.7 74.5
58	21.9 52.5 78.7

Instrument :
BNA_M
ClientSampleId :
YB2H2

Manual Integrations
APPROVED
Reviewed By :Jagrut Upadhyay 04/13/2022
Supervised By :Yogesh Patel 04/14/2022

