

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034650.D
 Acq On : 13 Apr 2022 09:47
 Operator : CG/JU
 Sample : N2319-02
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2G9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/14/2022
 Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 14 04:14:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	1949	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.683	136	5708	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.525	164	3163	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.263	188	6051m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.478	240	4551	0.400	ng/ul	# 0.01
23) Perylene-d12	23.808	264	2351m	0.400	ng/ul	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	13284	3.932	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152	3080	0.407	ng/ul	0.00
18) Fluoranthene-d10	19.294	212	7409	0.560	ng/ul	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.290	88	1125m	0.336	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034650.D
Acq On : 13 Apr 2022 09:47
Operator : CG/JU
Sample : N2319-02
Misc :
ALS Vial : 37 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
YB2G9

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/14/2022
Supervised By :Yogesh Patel 04/14/2022


Quant Time: Apr 14 04:14:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

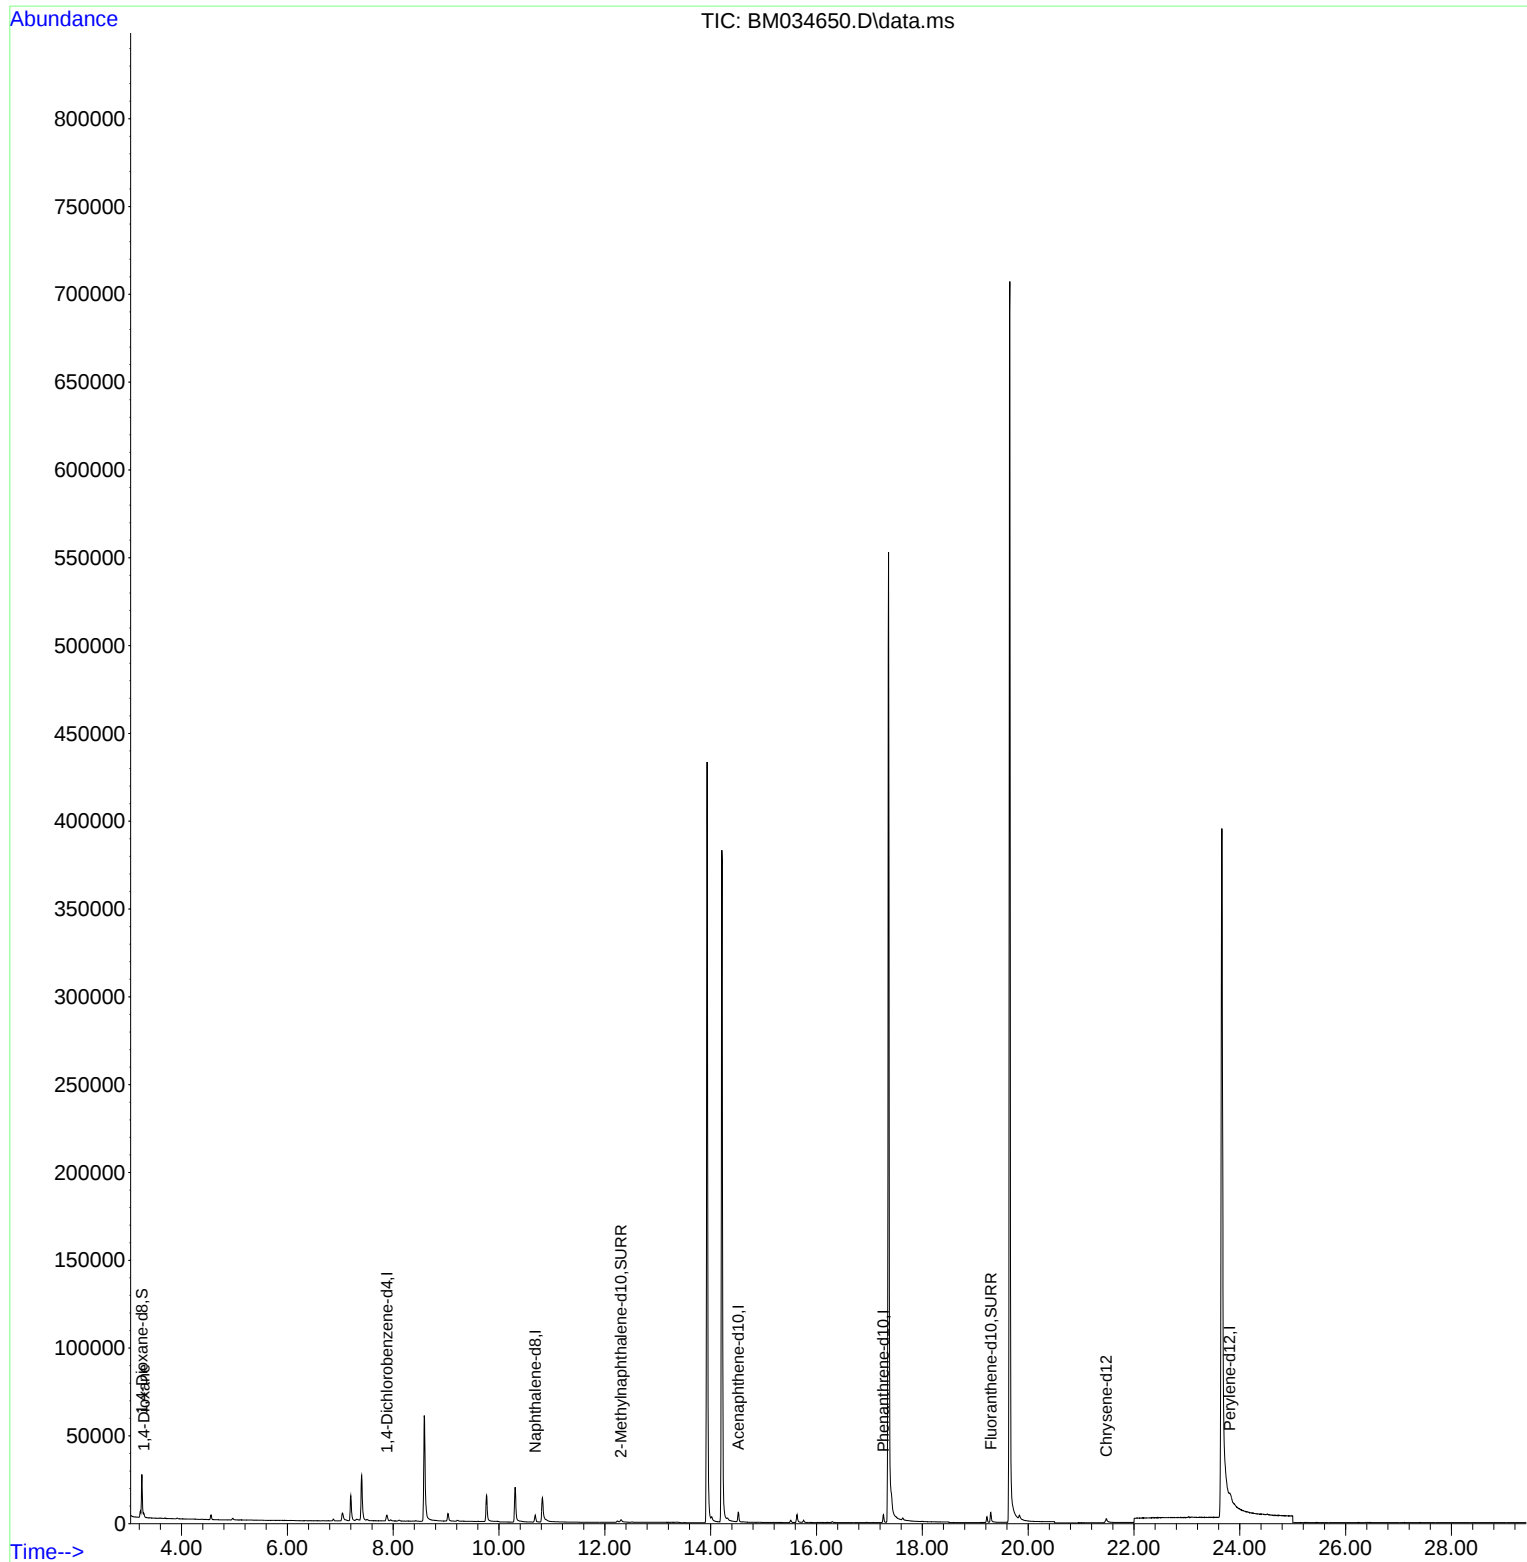

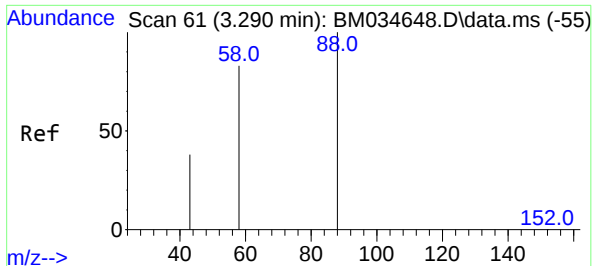

#2
 1,4-Dioxane
 Concen: 0.336 ng/ul m
 RT: 3.290 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BM034650.D
 Acq: 13 Apr 2022 09:47

Instrument :
 BNA_M
 ClientSampleId :
 YB2G9

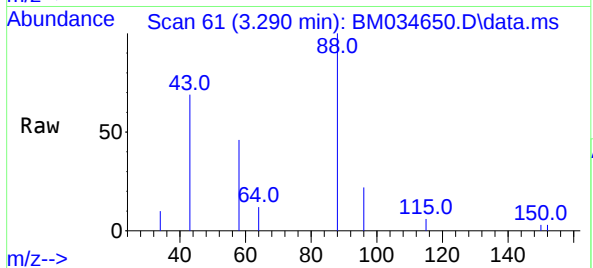

Tgt Ion: 88 Resp: 1125

Ion	Ratio	Lower	Upper
88	100		
43	69.1	49.7	74.5
58	46.1	52.5	78.7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/14/2022
 Supervised By :Yogesh Patel 04/14/2022

