

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
 Data File : BM034651.D
 Acq On : 13 Apr 2022 10:23
 Operator : CG/JU
 Sample : N2319-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YB2H0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/14/2022
 Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 14 04:14:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 12 15:46:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.880	152	2189	0.400	ng/u1	-0.03
4) Naphthalene-d8	10.683	136	6125	0.400	ng/u1	#-0.02
9) Acenaphthene-d10	14.520	164	3391	0.400	ng/u1	#-0.01
13) Phenanthrene-d10	17.263	188	6225	0.400	ng/u1	-0.02
17) Chrysene-d12	21.480	240	4527	0.400	ng/u1	# 0.01
23) Perylene-d12	23.804	264	1872m	0.400	ng/u1	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	13088	3.449	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.311	152	3038	0.374	ng/u1	0.00
18) Fluoranthene-d10	19.290	212	7292	0.554	ng/u1	-0.02
Target Compounds						
2) 1,4-Dioxane	3.285	88	1109m	0.295	ng/u1	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041222\
Data File : BM034651.D
Acq On : 13 Apr 2022 10:23
Operator : CG/JU
Sample : N2319-03
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
YB2H0

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/14/2022
Supervised By :Yogesh Patel 04/14/2022


Quant Time: Apr 14 04:14:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM041222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 12 15:46:33 2022
Response via : Initial Calibration

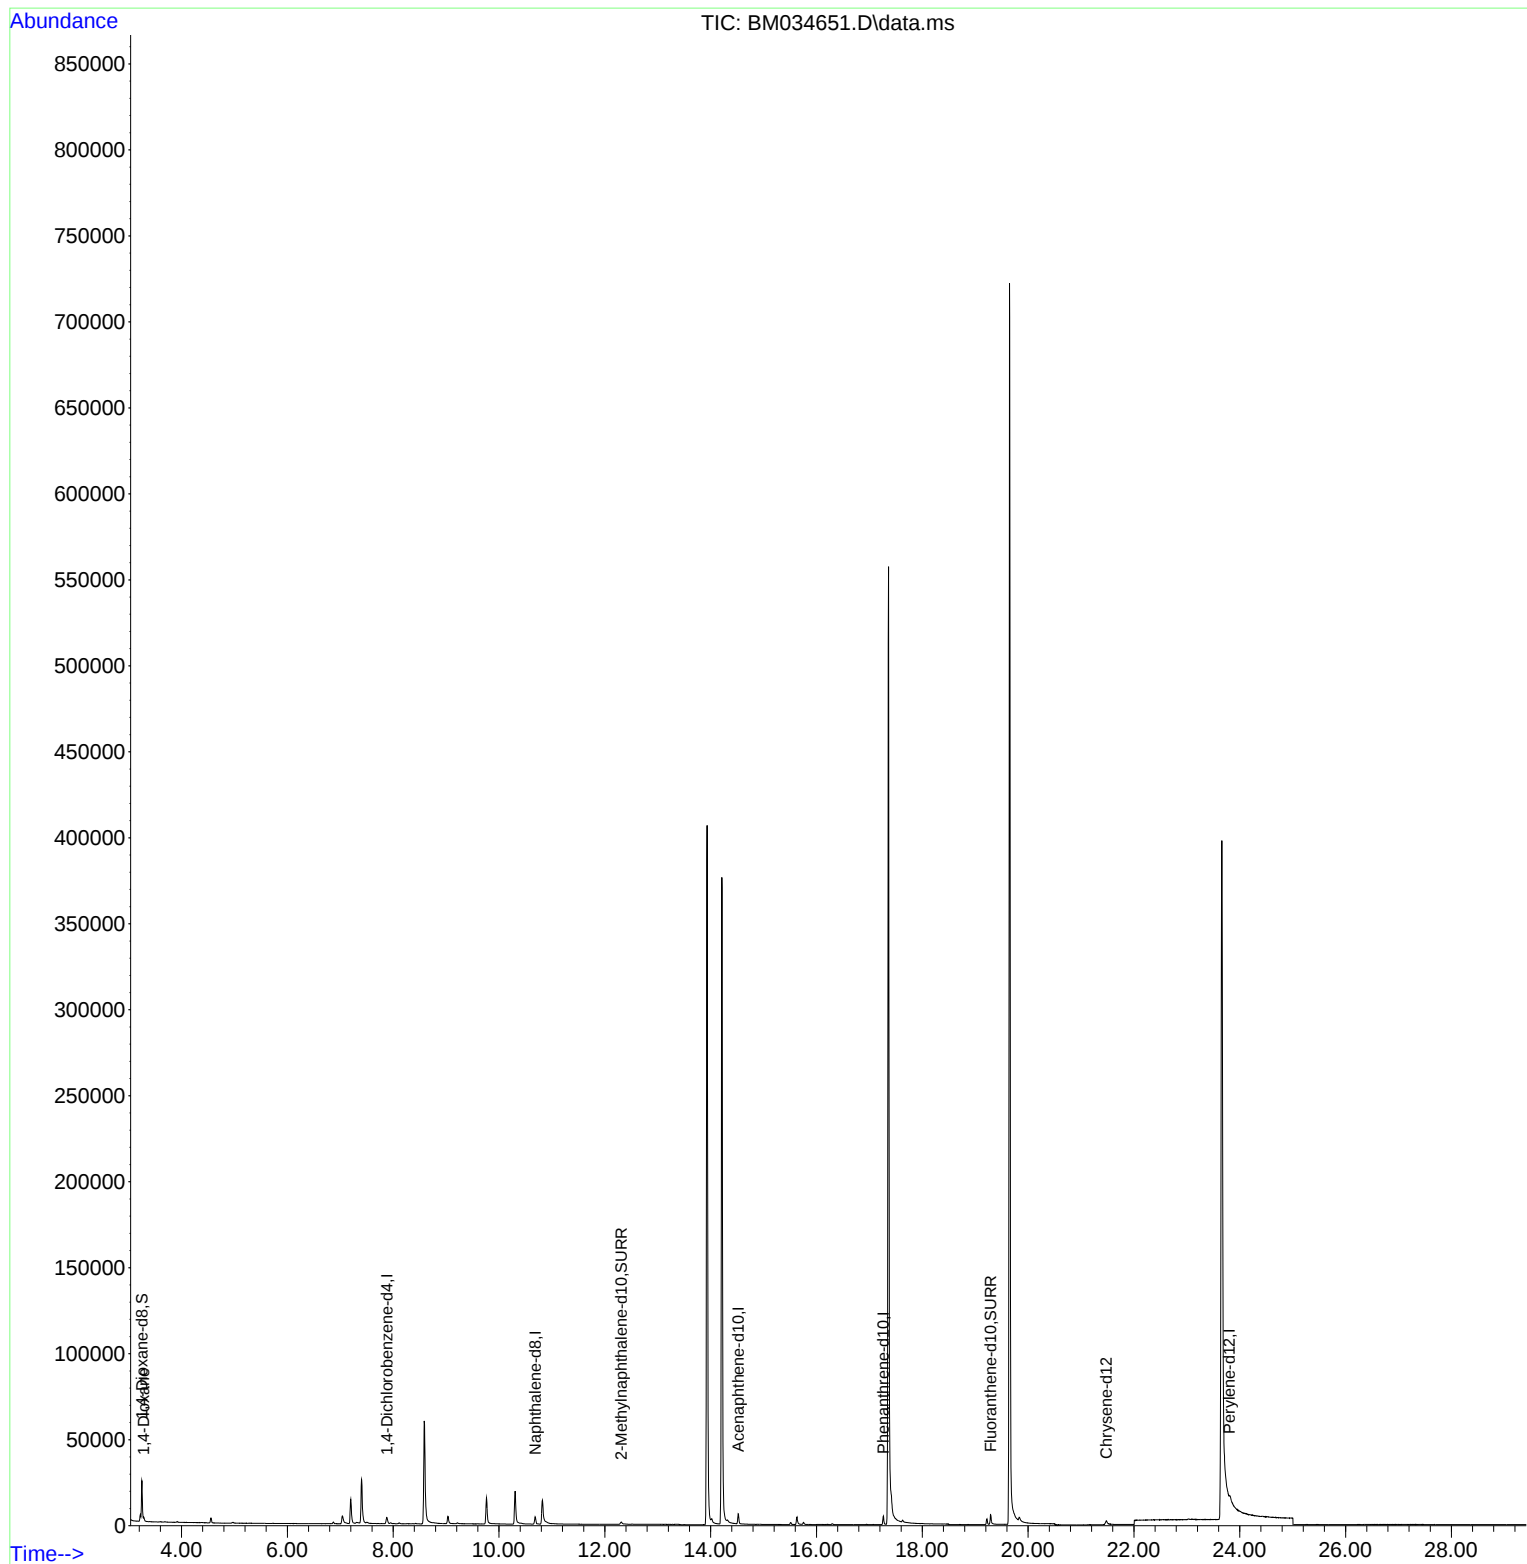

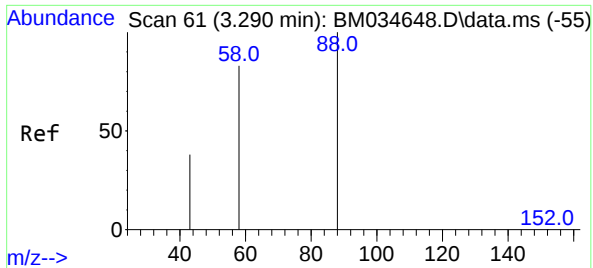

#2
 1,4-Dioxane
 Concen: 0.295 ng/ul m
 RT: 3.285 min Scan# 60
 Delta R.T. -0.005 min
 Lab File: BM034651.D
 Acq: 13 Apr 2022 10:23

Instrument :
 BNA_M
 ClientSampleId :
 YB2H0

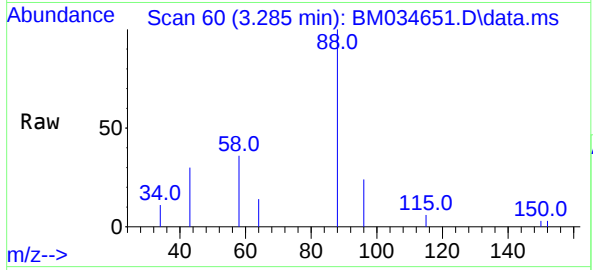

Tgt Ion: 88 Resp: 1109

Ion	Ratio	Lower	Upper
88	100		
43	29.9	49.7	74.5
58	35.5	52.5	78.7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/14/2022
 Supervised By :Yogesh Patel 04/14/2022

