
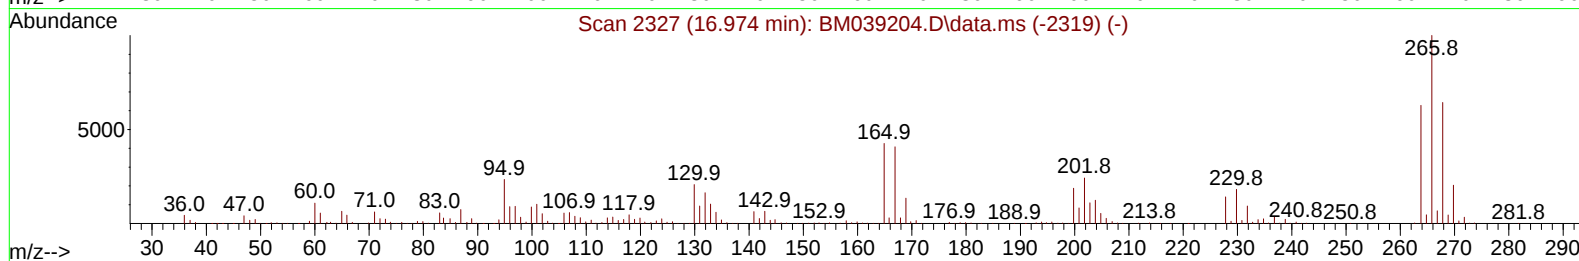
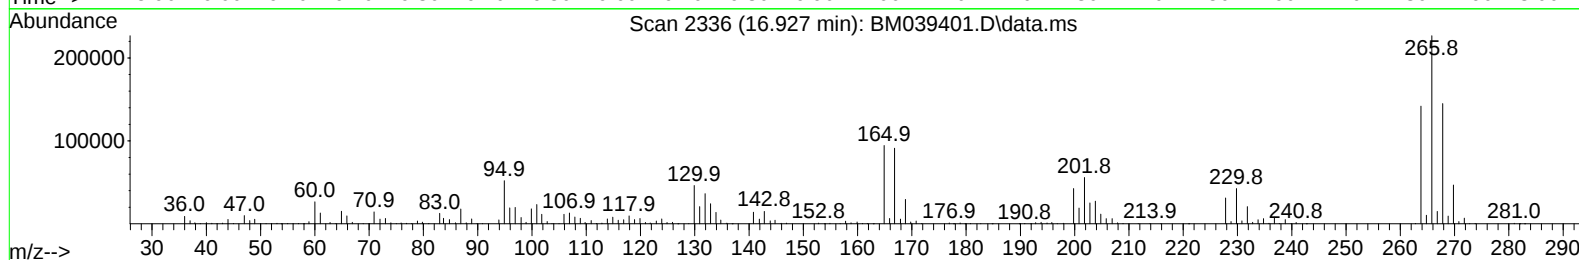


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041223\
Data File : BM039401.D
Acq On : 12 Apr 2023 12:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 03:45:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 11 16:05:42 2023
Response via : Initial Calibration

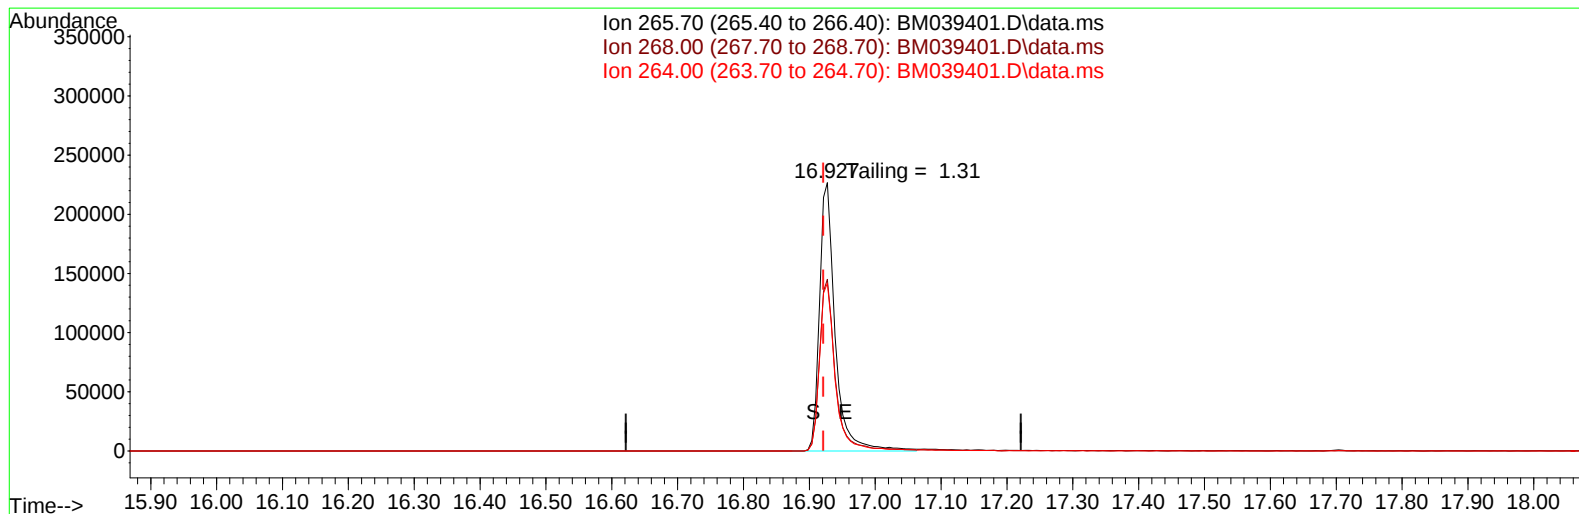

TIC: BM039401.D\data.ms

(70) Pentachlorophenol (C)




16.927min (+ 0.006) 0.00 ng

response 375732

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.99
264.00	62.80	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041223\
Data File : BM039401.D
Acq On : 12 Apr 2023 12:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 03:45:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 11 16:05:42 2023
Response via : Initial Calibration

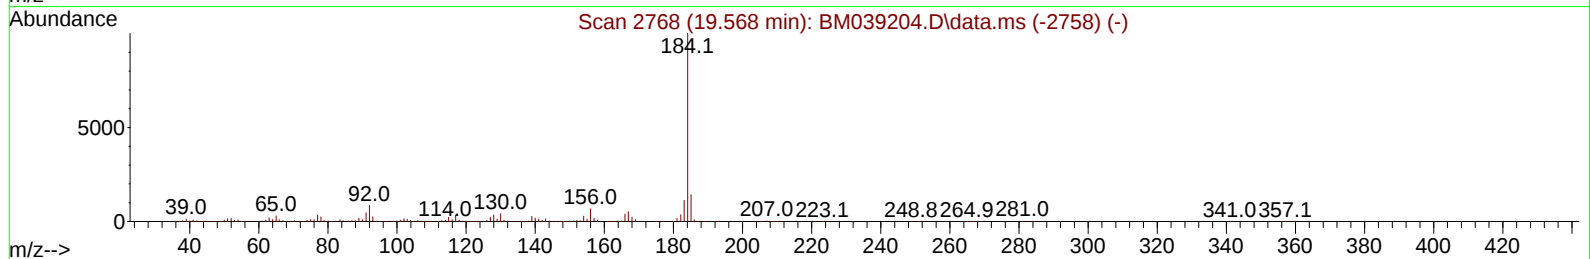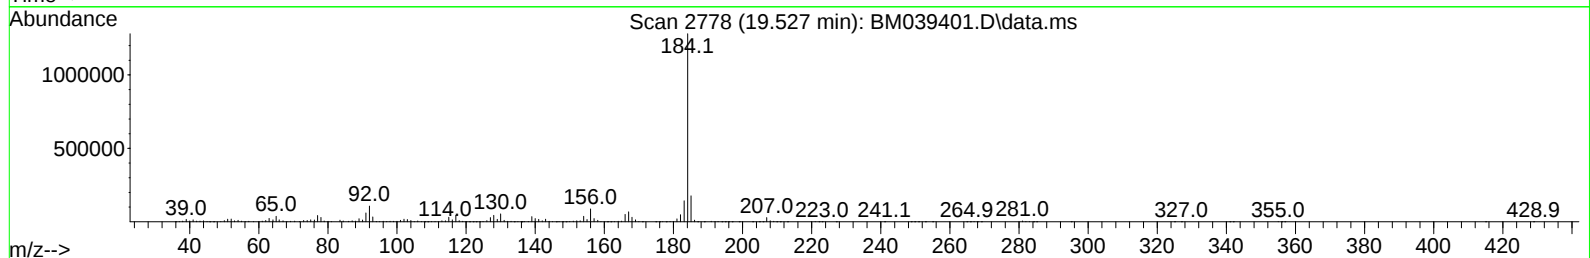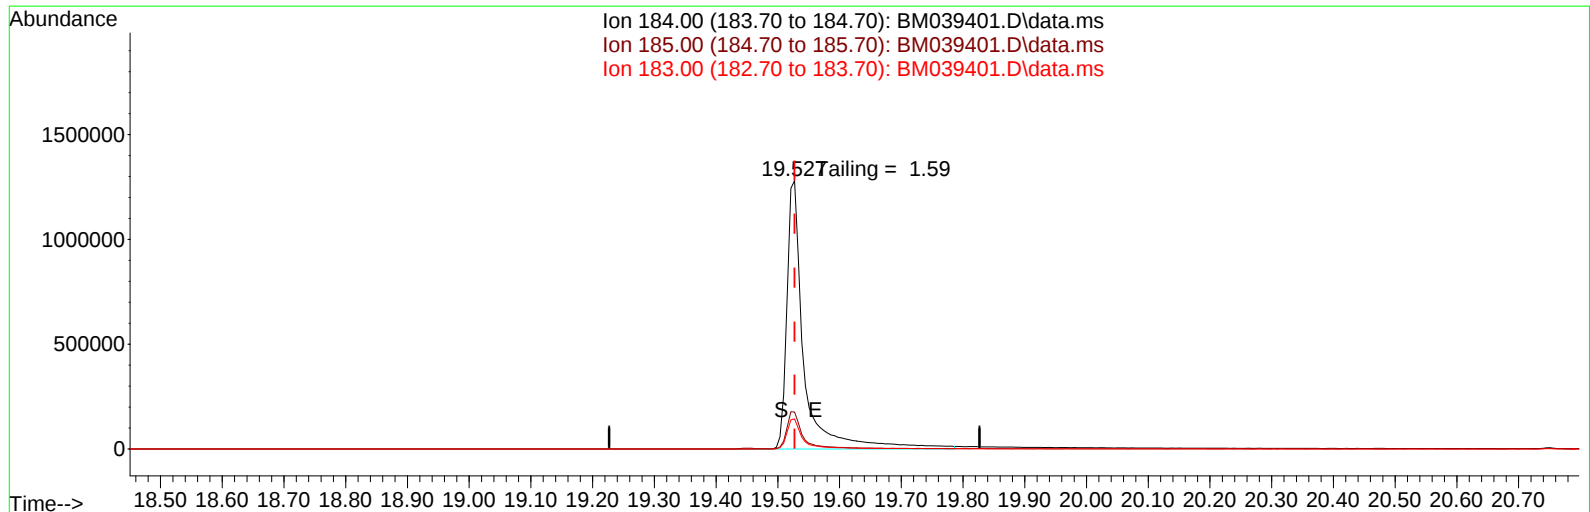

TIC: BM039401.D\data.ms

(77) Benzidine**19.527min (+ 0.000) 31117.69 ng****response 2502537**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.81
183.00	11.20	11.21
0.00	0.00	0.00