
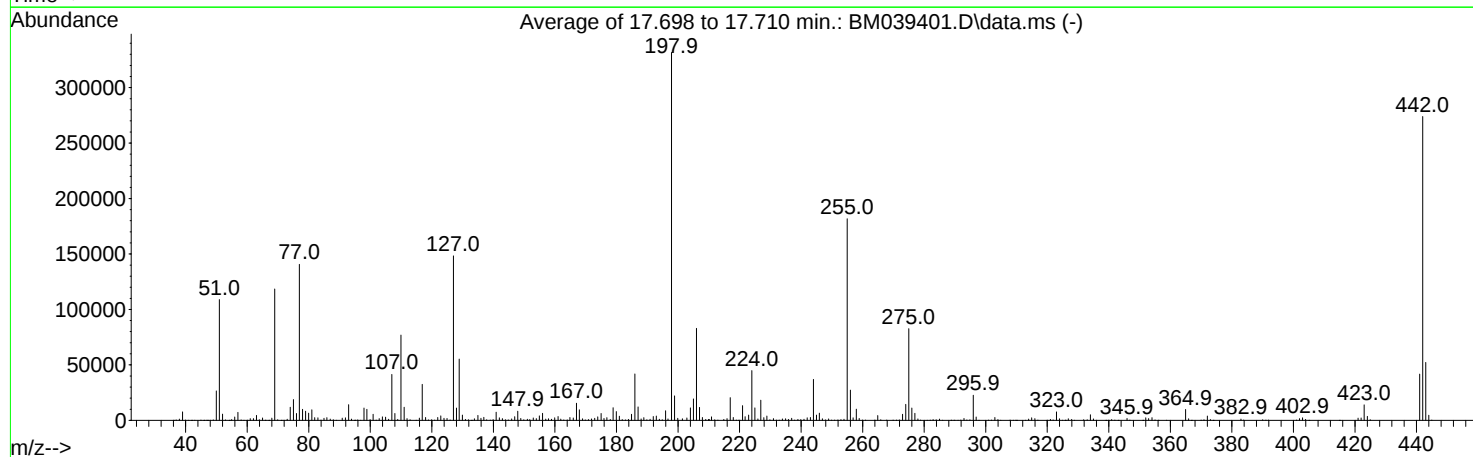


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041223\
Data File : BM039401.D
Acq On : 12 Apr 2023 12:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 11 16:05:42 2023

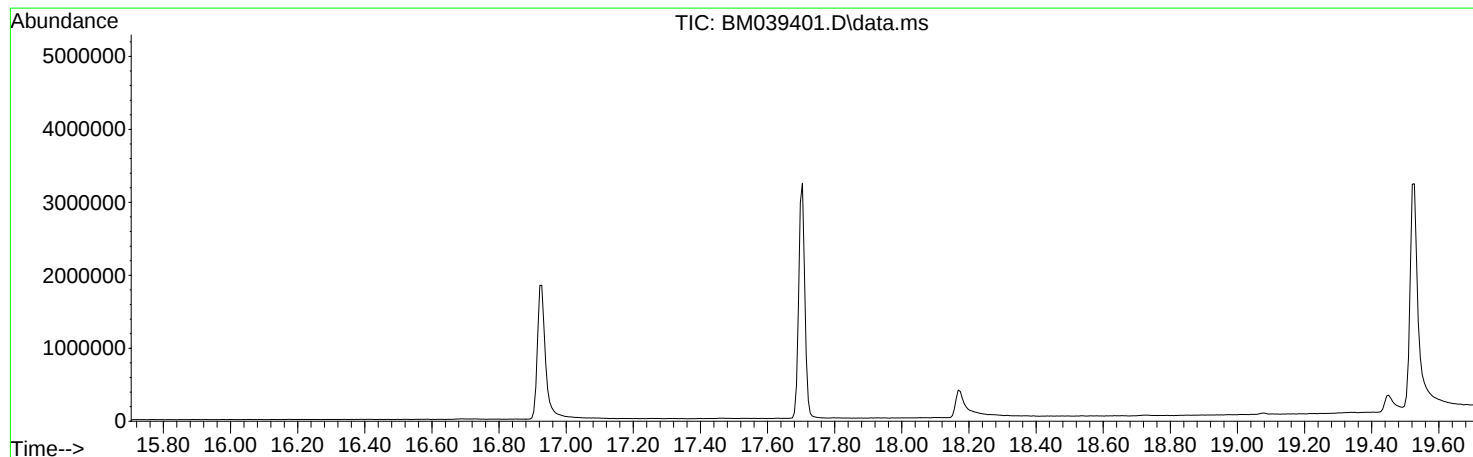




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	108867	PASS
68	69	0.00	2	1.7	2023	PASS
69	198	0.00	100	35.7	118405	PASS
70	69	0.00	2	0.5	561	PASS
127	198	10	80	44.7	148267	PASS
197	198	0.00	2	0.4	1340	PASS
198	198	100	100	100.0	331669	PASS
199	198	5	9	6.6	22030	PASS
275	198	10	60	24.9	82661	PASS
365	198	1	100	2.9	9761	PASS
441	198	0.01	100	12.6	41701	PASS
442	442	50	100	100.0	273963	PASS
443	442	15	24	19.1	52275	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041223\
Data File : BM039401.D
Acq On : 12 Apr 2023 12:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 13 03:45:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 11 16:05:42 2023
Response via : Initial Calibration

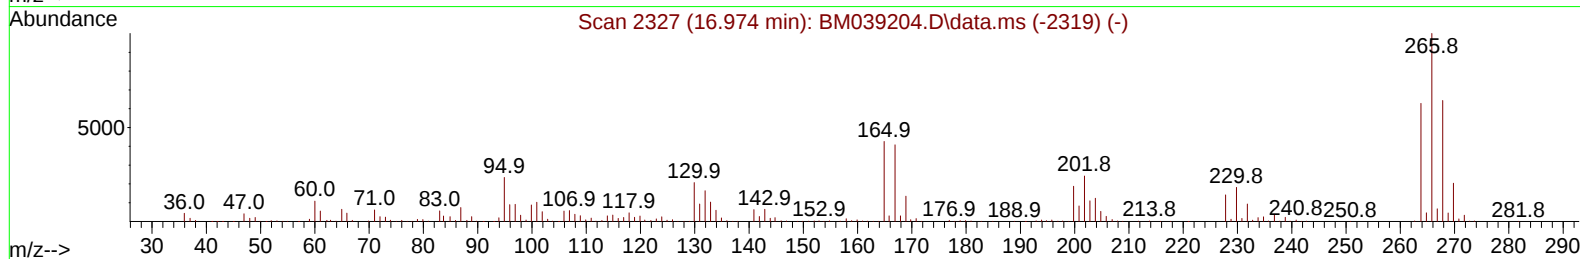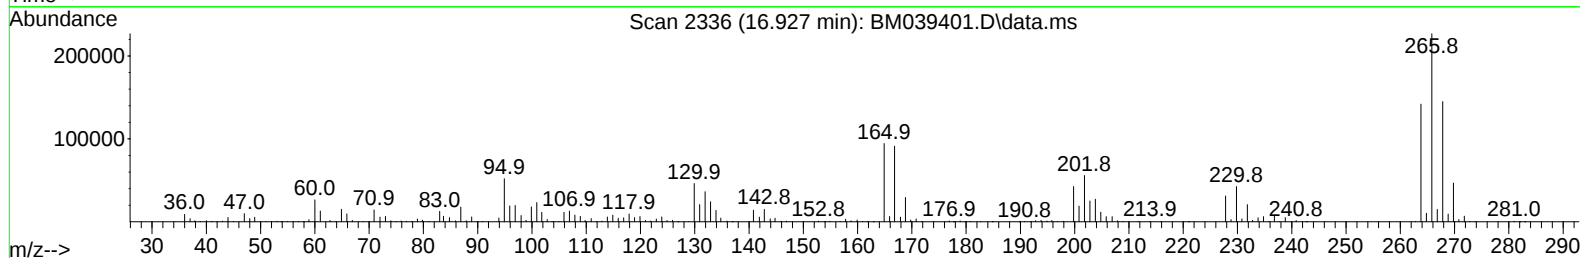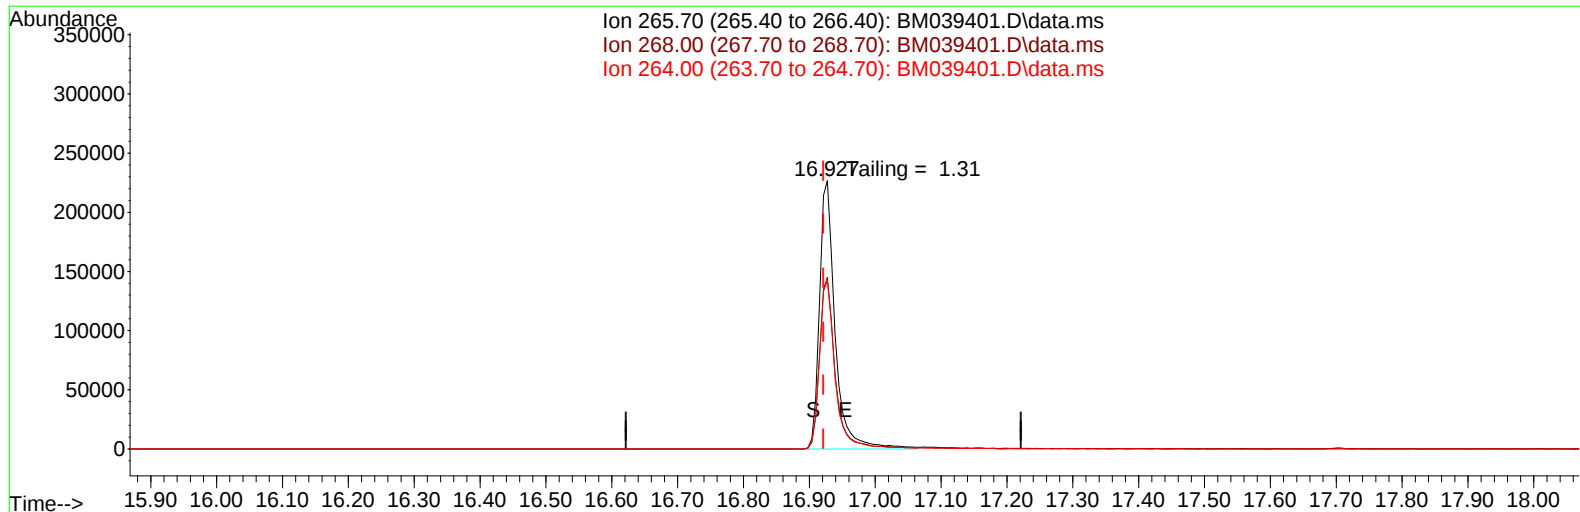

TIC: BM039401.D\data.ms

(70) Pentachlorophenol (C)

16.927min (+ 0.006) 0.00 ng




response 375732

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.99
264.00	62.80	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041223\
Data File : BM039401.D
Acq On : 12 Apr 2023 12:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 13 03:45:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 11 16:05:42 2023
Response via : Initial Calibration

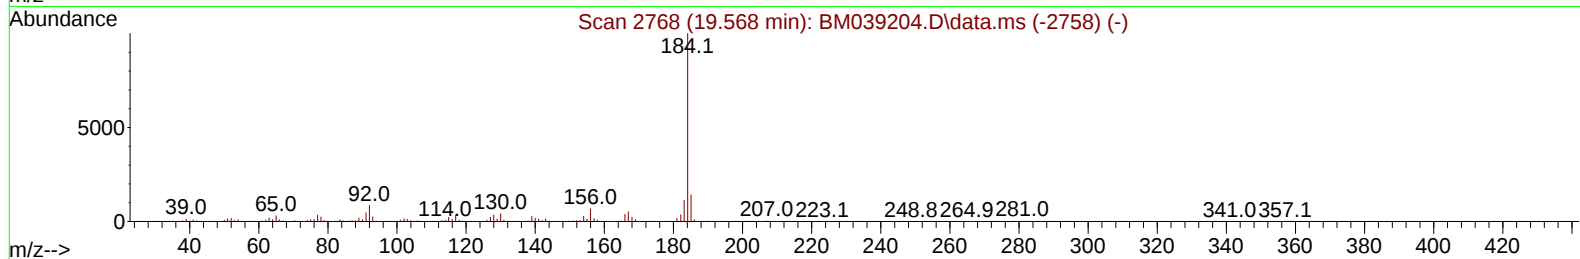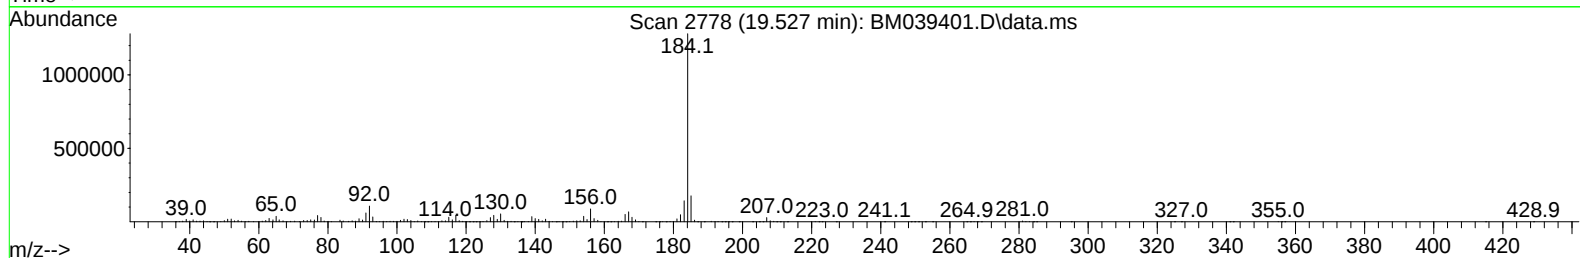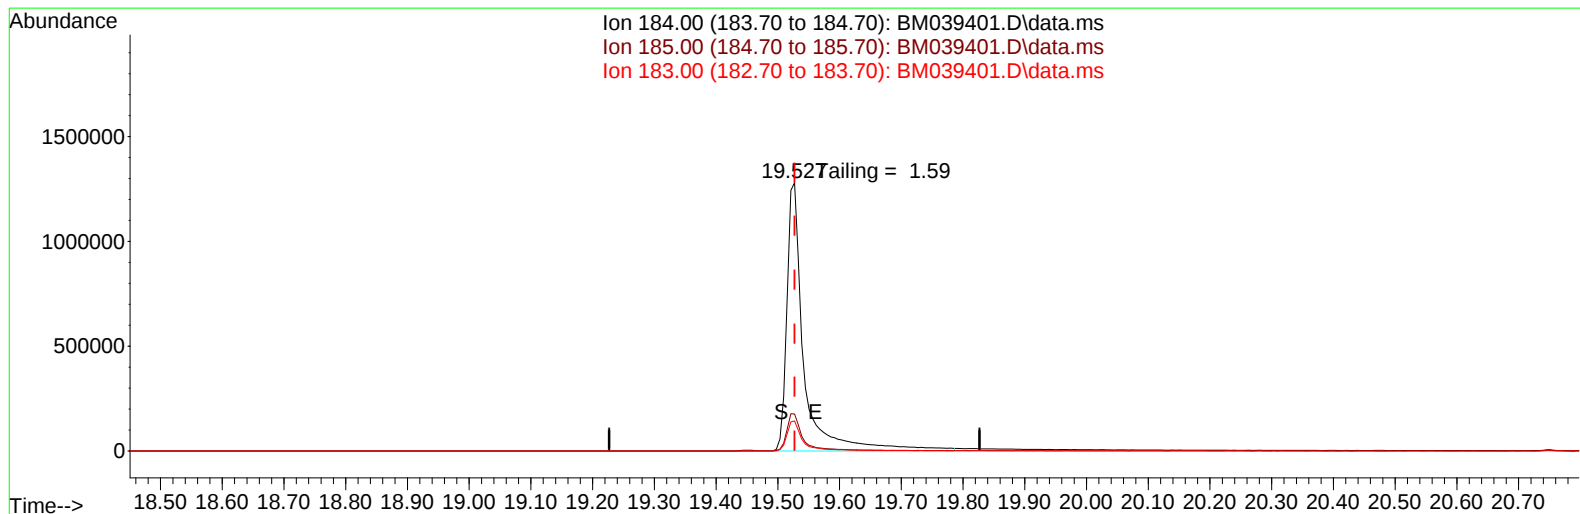

TIC: BM039401.D\data.ms

(77) Benzidine

19.527min (+ 0.000) 31117.69 ng

response 2502537

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.81
183.00	11.20	11.21
0.00	0.00	0.00

Date	Instrument Name	DFTPP Data File
4/12/2023	BNA_M	<u>BM039401.D</u>
Compound Name	Response	Retention Time
DDT	1156735	20.751
DDD	20442	20.356
DDE	959	19.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21401	1178136	1.82

Instrument :
 BNA_M
 ClientSampled :
 DFTPP