


Data Path : Z:\HPCHEM1\BNA_M\Data\BM041315\
 Data File : BM000951.D
 Acq On : 13 Apr 2015 12:35
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 10 16:15:17 2015

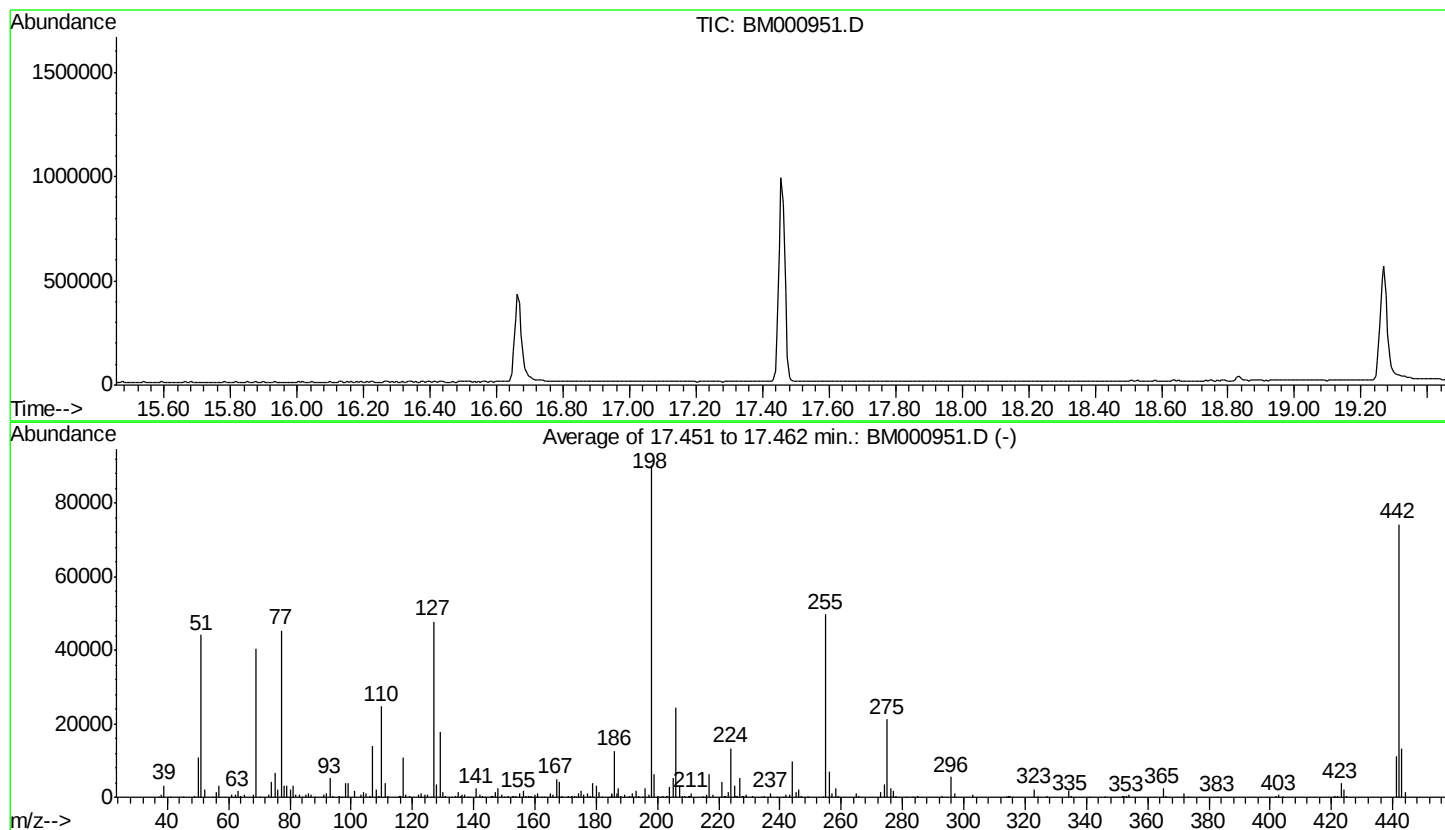

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.0	44149	PASS
68	69	0.00	2	1.7	672	PASS
69	198	0.00	100	45.0	40517	PASS
70	69	0.00	2	0.3	134	PASS
127	198	10	80	53.0	47773	PASS
197	198	0.00	2	0.8	729	PASS
198	198	100	100	100.0	90130	PASS
199	198	5	9	7.0	6316	PASS
275	198	10	60	23.5	21202	PASS
365	198	1	100	2.6	2310	PASS
441	442	0.01	24	15.1	11206	PASS
442	198	50	100	82.3	74146	PASS
443	442	15	24	18.0	13355	PASS