

Data Path : Z:\HPCHEM1\BNA M\DATA\BM041318\
 Data File : BM014710.D
 Acq On : 13 Apr 2018 21:33
 Operator : SJ/JU
 Sample : J2313-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 14 01:14:35 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032818MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 14 01:12:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.57	152	440539	20.00	ng/ul	0.00
18) Naphthalene-d8	11.42	136	1800664	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.17	164	930816	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.88	188	1912693	20.00	ng/ul	0.00
77) Chrysene-d12	21.96	240	1804909	20.00	ng/ul	0.00
85) Perylene-d12	24.48	264	1790581	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.69	96	56656	6.19	ng/uL	0.00
5) Phenol-d5	7.69	99	234185	6.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.87	67	764161	34.58	ng/ul	0.00
9) 2-Chlorophenol-d4	8.09	132	807905	27.87	ng/ul	0.00
13) 4-Methylphenol-d8	9.27	113	468179	16.31	ng/ul	0.00
19) Nitrobenzene-d5	9.75	128	488638	42.20	ng/ul	0.00
22) 2-Nitrophenol-d4	10.48	143	516742	49.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	11.02	165	859785	32.33	ng/ul	0.00
29) 4-Chloroaniline-d4	11.53	131	988	0.03	ng/ul	-0.01
43) Dimethylphthalate-d6	14.56	166	2643367	35.94	ng/ul	0.00
46) Acenaphthylene-d8	14.87	160	3449064	36.92	ng/ul	0.00
51) 4-Nitrophenol-d4	15.32	143	71084	5.96	ng/ul	0.00
57) Fluorene-d10	16.15	176	2266335	35.83	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.24	200	314219	38.48	ng/ul	0.00
70) Anthracene-d10	17.98	188	3307672	36.71	ng/ul	0.00
78) Pyrene-d10	20.21	212	3385652	36.96	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.32	264	3134252	35.65	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
33) 4-Chloro-3-methylphenol	12.64	107	27872	1.050	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM041318\
Data File : BM014710.D
Acq On : 13 Apr 2018 21:33
Operator : SJ/JU
Sample : J2313-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Apr 14 01:14:35 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM032818MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 14 01:12:03 2018
Response via : Initial Calibration

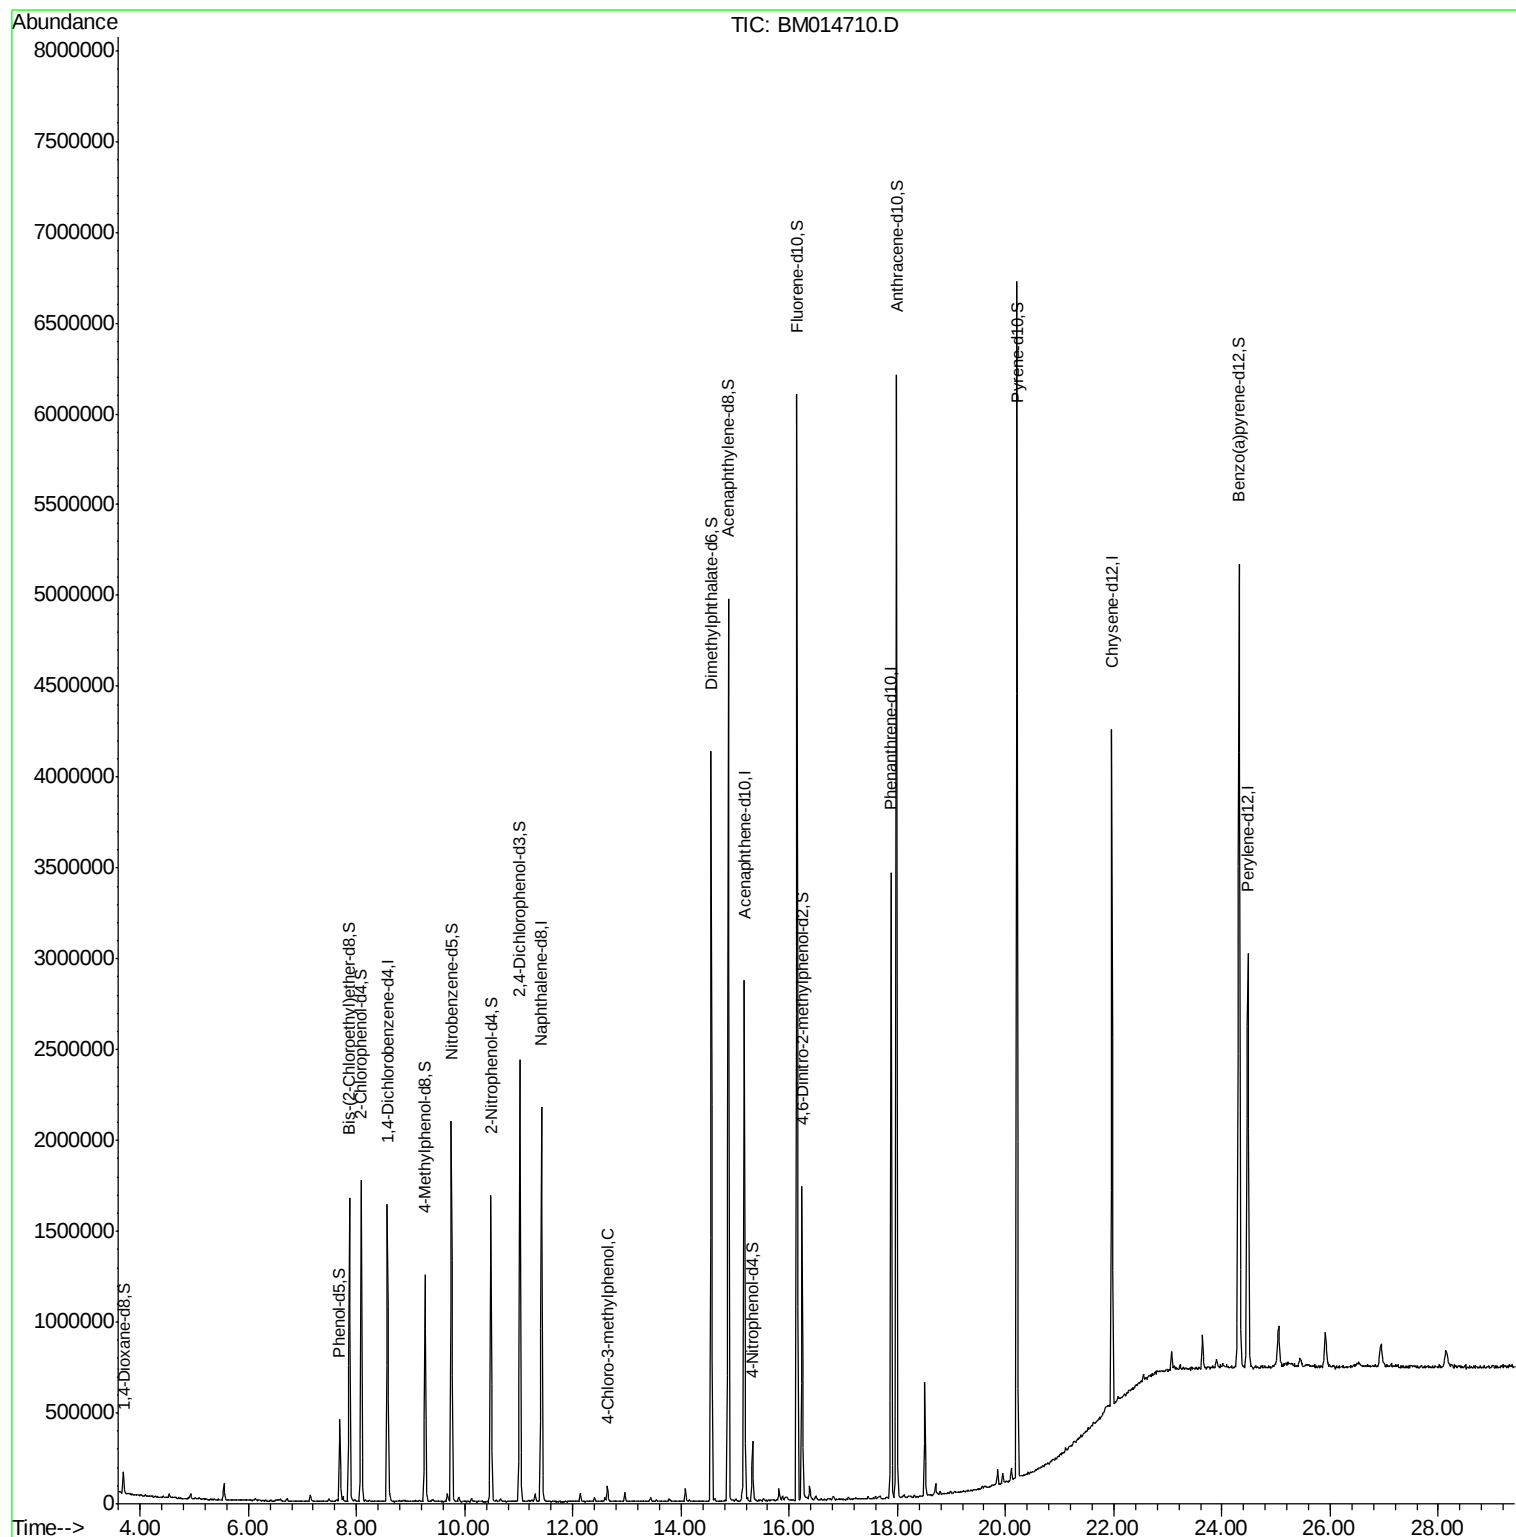

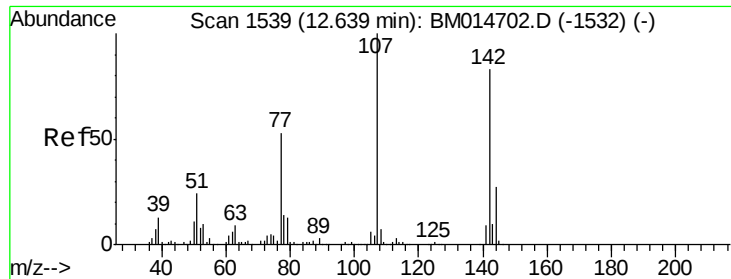

#33
 4-Chloro-3-methylphenol
 Concen: 1.050 ng/ul
 RT: 12.64 min Scan# 1539
 Delta R.T. 0.00 min
 Lab File: BM014710.D
 Acq: 13 Apr 2018 21:33

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
107	100		
144	27.9	20.4	30.6
142	76.6	62.5	93.7

