
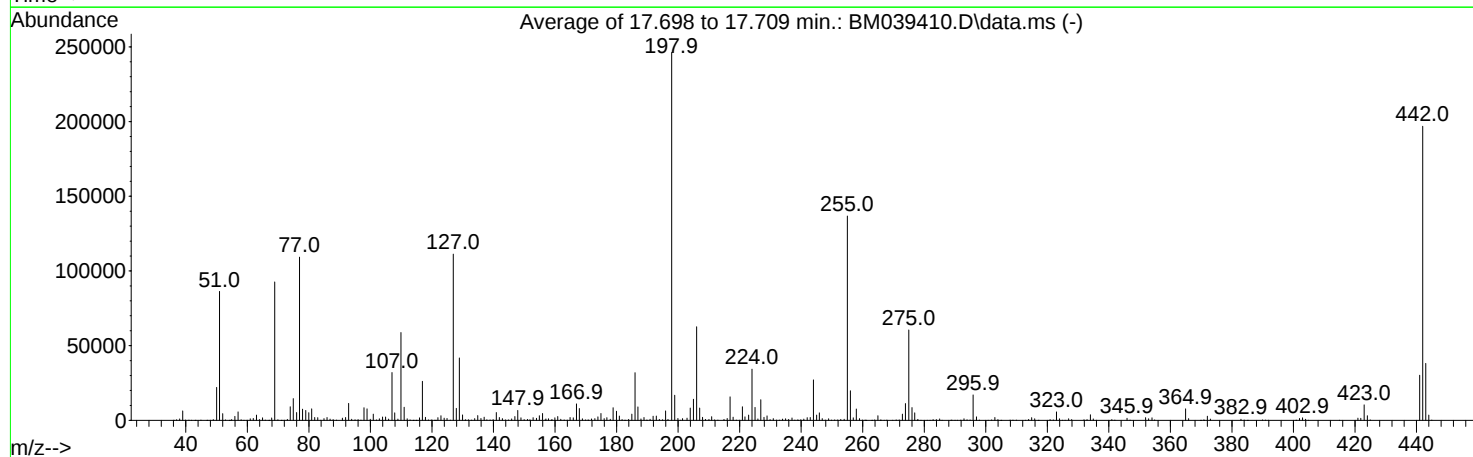


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041323\
Data File : BM039410.D
Acq On : 13 Apr 2023 14:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 14 14:49:28 2023

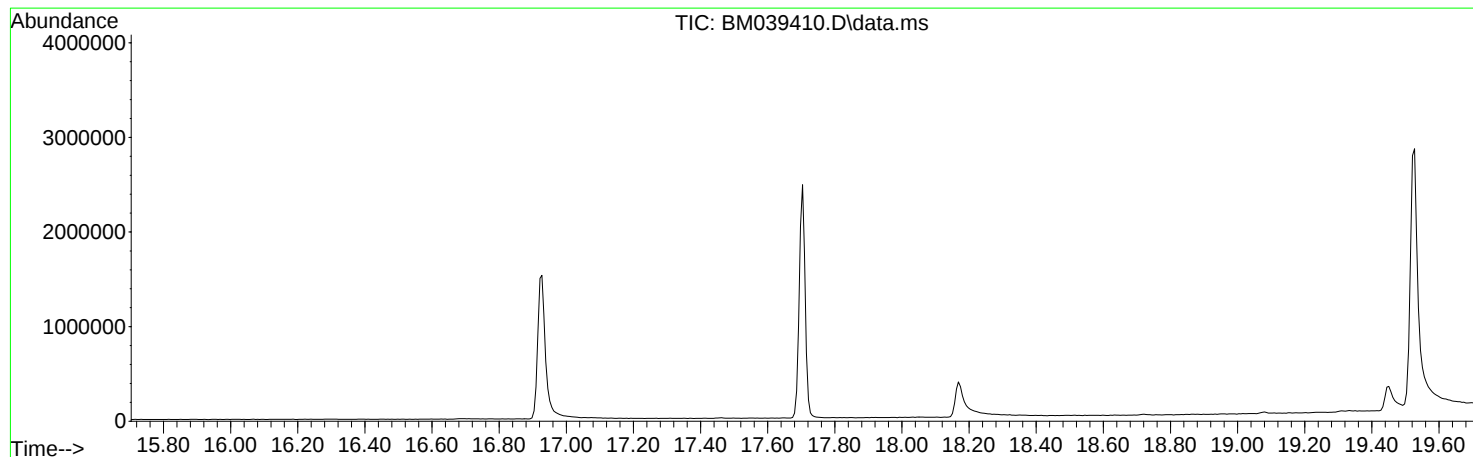




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	86314	PASS
68	69	0.00	2	1.7	1582	PASS
69	198	0.00	100	37.6	92639	PASS
70	69	0.00	2	0.5	431	PASS
127	198	10	80	45.2	111331	PASS
197	198	0.00	2	0.3	651	PASS
198	198	100	100	100.0	246229	PASS
199	198	5	9	6.8	16776	PASS
275	198	10	60	24.6	60544	PASS
365	198	1	100	3.1	7745	PASS
441	198	0.01	100	12.3	30219	PASS
442	442	50	100	100.0	196800	PASS
443	442	15	24	19.4	38109	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041323\
Data File : BM039410.D
Acq On : 13 Apr 2023 14:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 14 08:29:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 11 16:05:42 2023
Response via : Initial Calibration

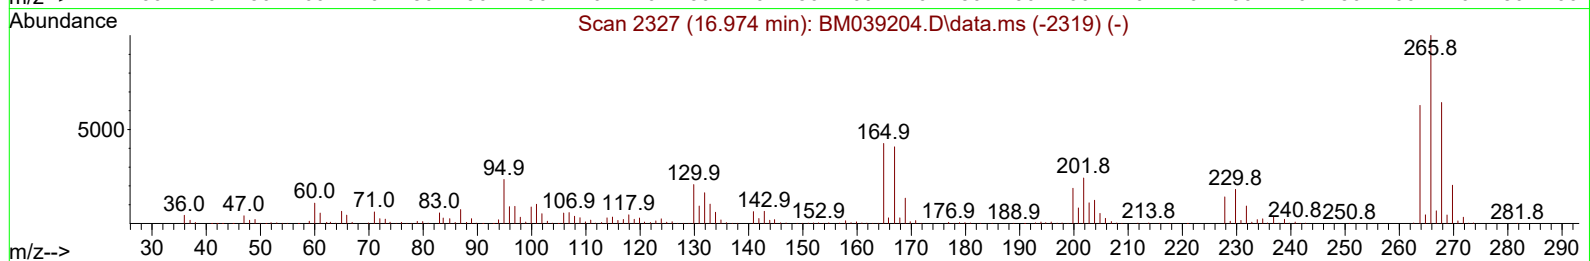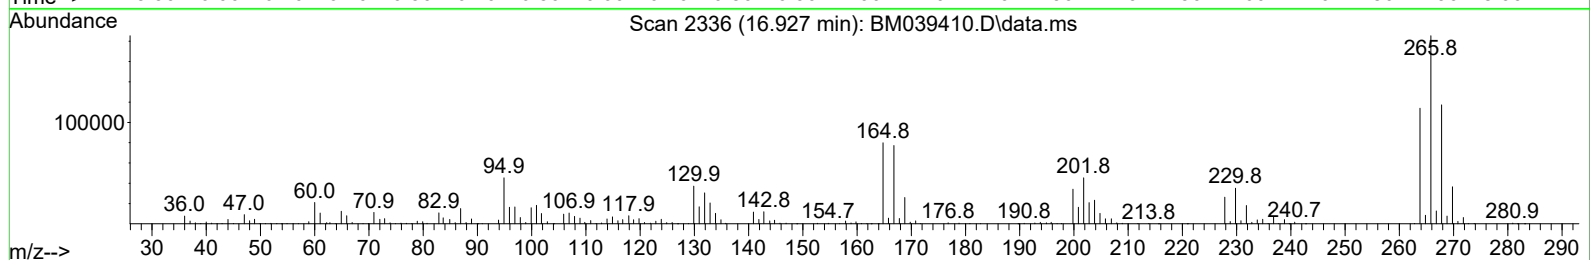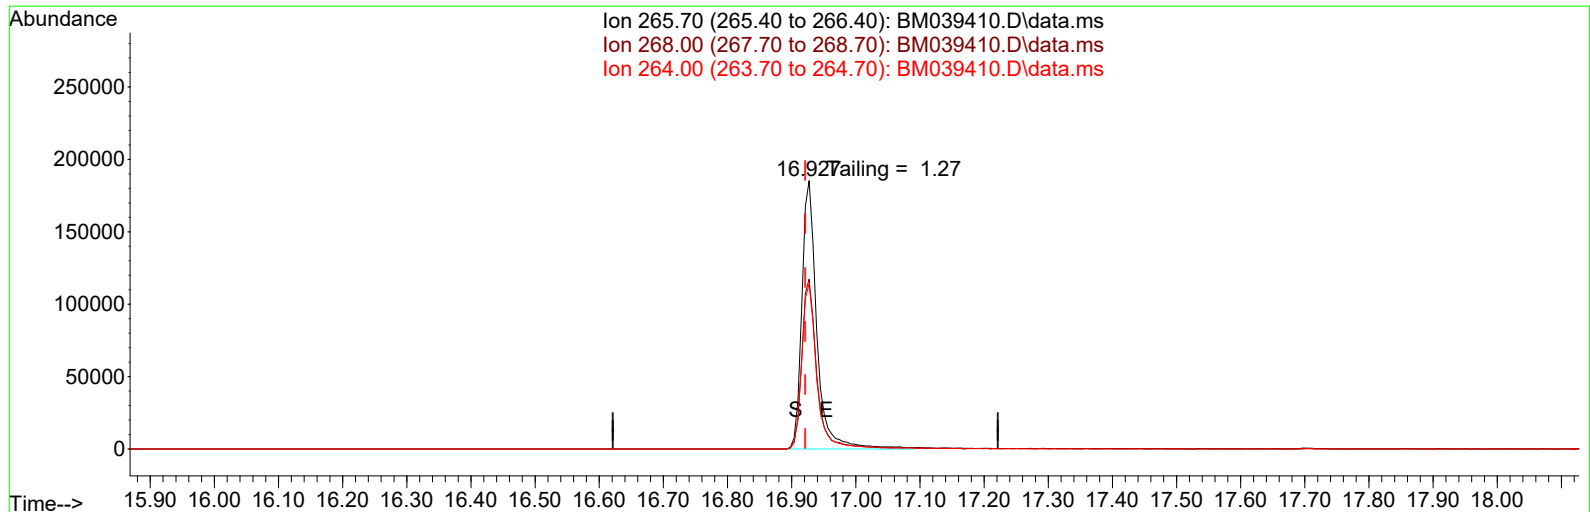

TIC: BM039410.D\data.ms

(70) Pentachlorophenol (C)

16.927min (+ 0.006) 0.00 ng




response 305279

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.24
264.00	62.80	61.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041323\
 Data File : BM039410.D
 Acq On : 13 Apr 2023 14:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 14 08:29:08 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 11 16:05:42 2023
 Response via : Initial Calibration

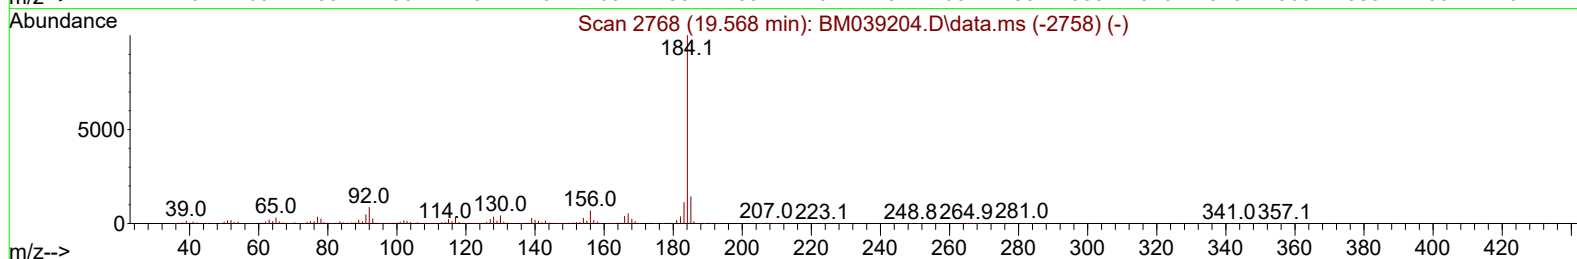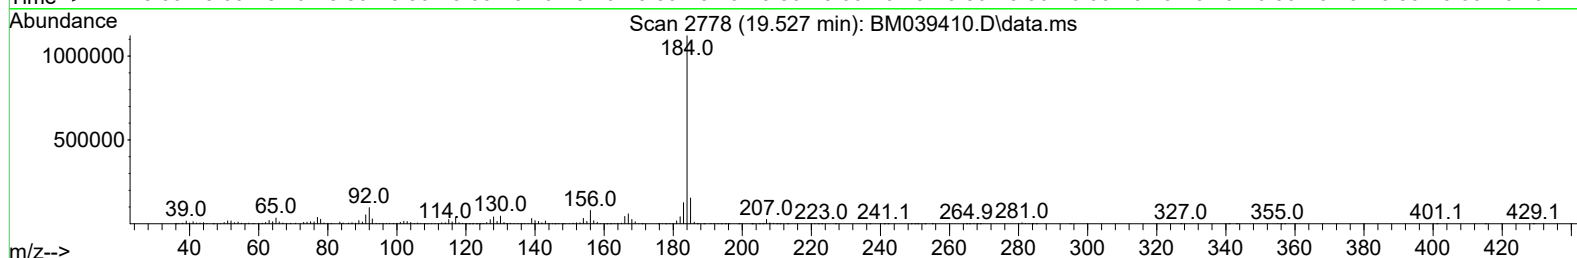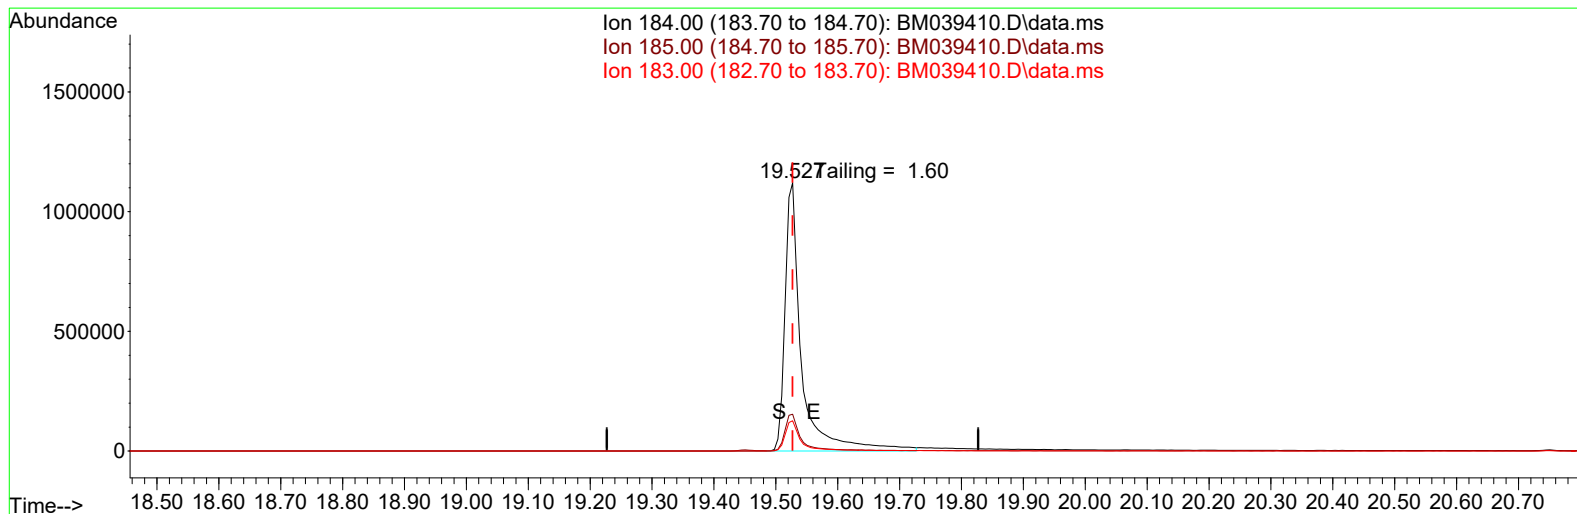

TIC: BM039410.D\data.ms

(77) Benzidine

19.527min (+ 0.000) 30431.77 ng

response 2143961

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.72
183.00	11.20	11.27
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/13/2023	BNA_M	<u>BM039410.D</u>
Compound Name	Response	Retention Time
DDT	855896	20.75
DDD	15405	20.362
DDE	909	19.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16314	872210	1.87

Instrument :
BNA_M
ClientSampleId :
DFTPP