

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
 Data File : BM045208.D
 Acq On : 13 Apr 2024 17:05
 Operator : MA/JU
 Sample : P2014-16
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0ME1

Quant Time: Apr 15 00:35:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 00:32:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.606	152	1670	0.400	ng/ul	0.00
4) Naphthalene-d8	10.375	136	5130	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.251	164	2769	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.111	188	500559	0.400	ng/ul	# 0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.24
23) Perylene-d12	23.444	264	9414	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	7890	3.597	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.997	152	2272	0.327	ng/ul	0.00
18) Fluoranthene-d10	19.057	212	5223	0.000	ng/ul	-0.01
Target Compounds						
					Qvalue	
5) Naphthalene	10.424	128	298	0.022	ng/ul#	38
26) Benzo(a)pyrene	23.294	252	2761	0.085	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045208.D
Acq On : 13 Apr 2024 17:05
Operator : MA/JU
Sample : P2014-16
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME1


Quant Time: Apr 15 00:35:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration

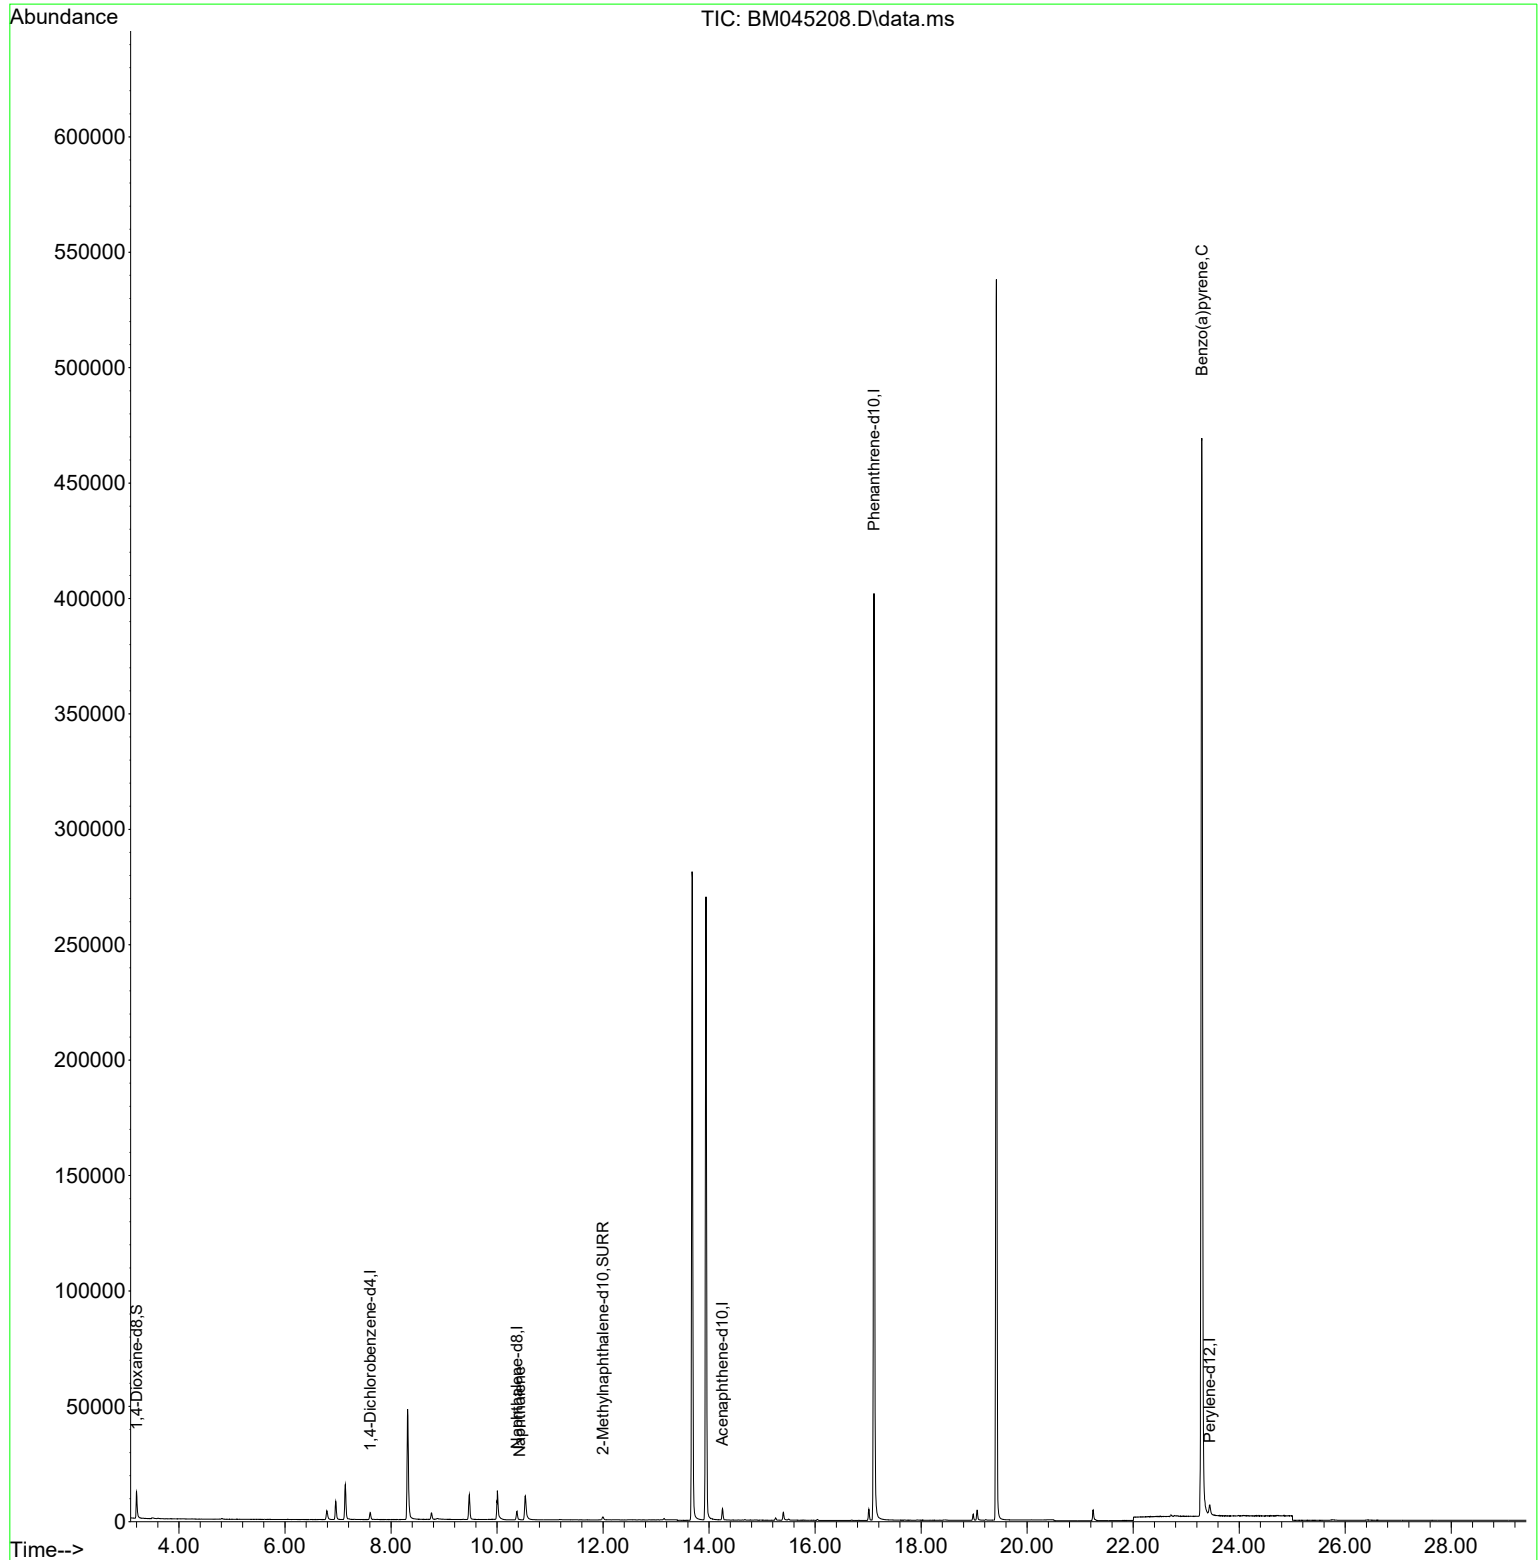



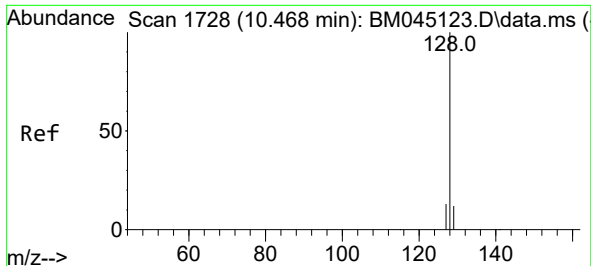


#5
Naphthalene
Concen: 0.022 ng/ul
RT: 10.424 min Scan# 1
Delta R.T. -0.016 min
Lab File: BM045208.D
Acq: 13 Apr 2024 17:05

Instrument :
BNA_M
ClientSampleId :
E0ME1

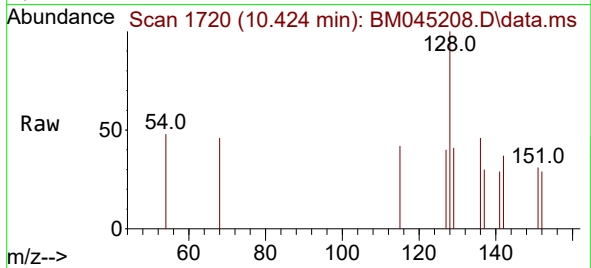

Tgt Ion:128 Resp: 298
Ion Ratio Lower Upper
128 100
129 40.6 11.3 16.9#
127 39.6 11.9 17.9#

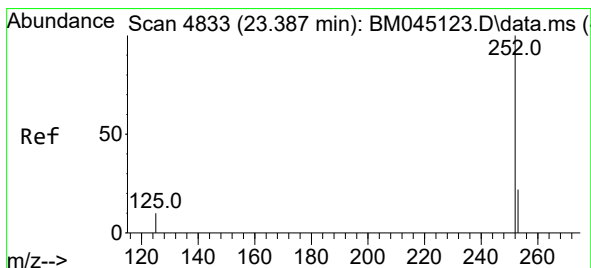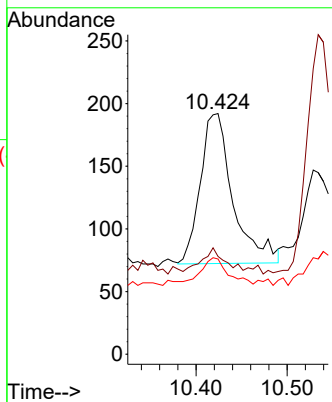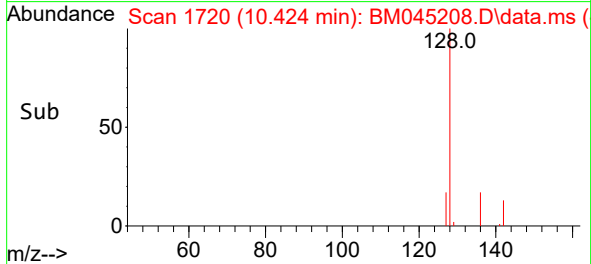

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.294 min Scan# 4801
Delta R.T. -0.069 min
Lab File: BM045208.D
Acq: 13 Apr 2024 17:05

Tgt Ion:252 Resp: 2761
Ion Ratio Lower Upper
252 100
253 55.2 24.6 37.0#
125 36.4 18.2 27.4#

