

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
 Data File : BM045210.D
 Acq On : 13 Apr 2024 18:17
 Operator : MA/JU
 Sample : P2014-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0ME3

Quant Time: Apr 15 00:36:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 00:32:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.606	152	1454	0.400	ng/ul	0.00
4) Naphthalene-d8	10.375	136	4484	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.251	164	2433	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.111	188	476234	0.400	ng/ul	# 0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.24
23) Perylene-d12	23.438	264	8648	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	6626	3.469	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.991	152	2201	0.362	ng/ul	0.00
18) Fluoranthene-d10	19.057	212	5434	0.000	ng/ul	-0.01
Target Compounds						Qvalue
5) Naphthalene	10.419	128	253	0.021	ng/ul#	40
24) Benzo(b)fluoranthene	22.783	252	704	0.023	ng/ul#	1
26) Benzo(a)pyrene	23.292	252	2801	0.094	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045210.D
Acq On : 13 Apr 2024 18:17
Operator : MA/JU
Sample : P2014-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME3


Quant Time: Apr 15 00:36:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration

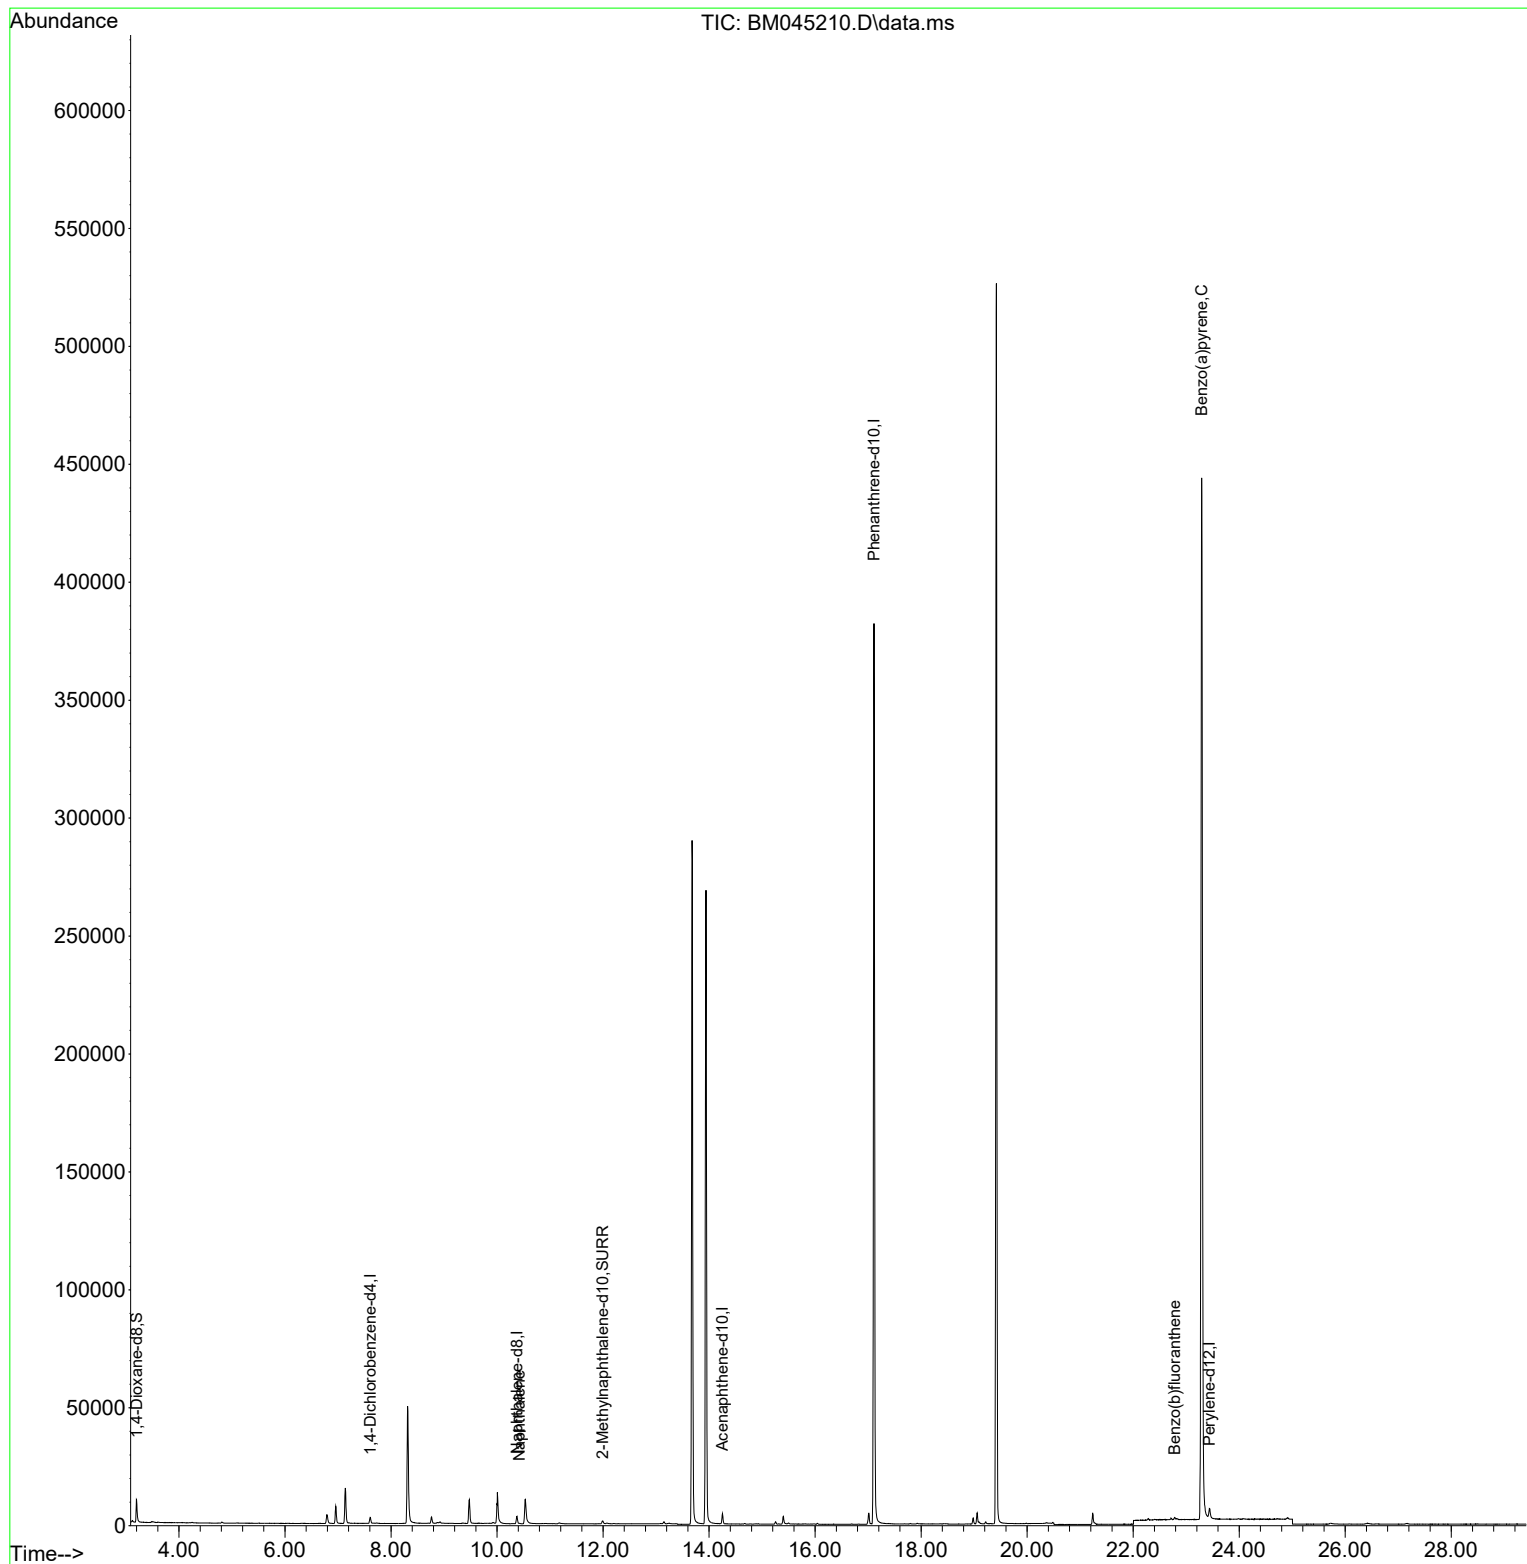



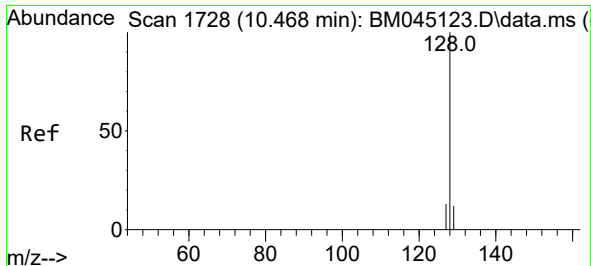


#5
Naphthalene
Concen: 0.021 ng/ul
RT: 10.419 min Scan# 1719
Delta R.T. -0.022 min
Lab File: BM045210.D
Acq: 13 Apr 2024 18:17

Instrument :
BNA_M
ClientSampleId :
EOME3



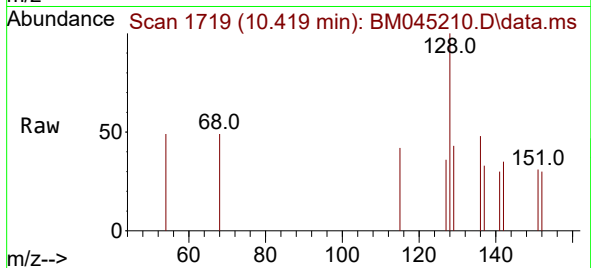



Tgt Ion:128 Resp: 253
Ion Ratio Lower Upper
128 100
129 42.7 11.3 16.9#
127 35.9 11.9 17.9#

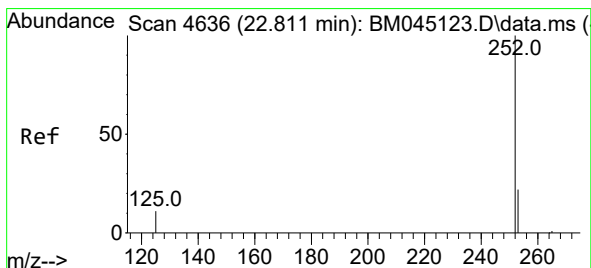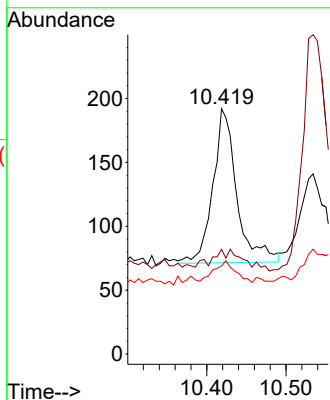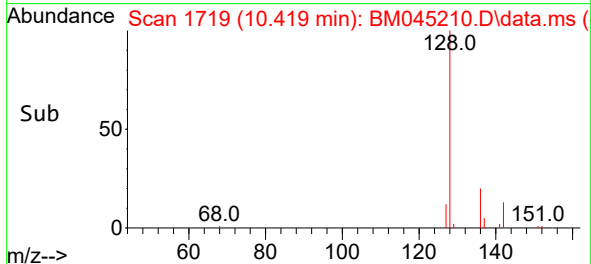

#24
Benzo(b)fluoranthene
Concen: 0.023 ng/ul
RT: 22.783 min Scan# 4626
Delta R.T. -0.011 min
Lab File: BM045210.D
Acq: 13 Apr 2024 18:17


Tgt Ion:252 Resp: 704
Ion Ratio Lower Upper
252 100
253 96.1 0.0 56.4#
125 134.4 0.0 33.4#

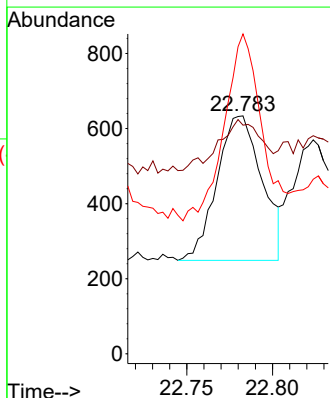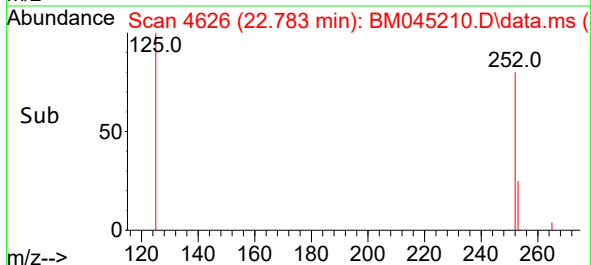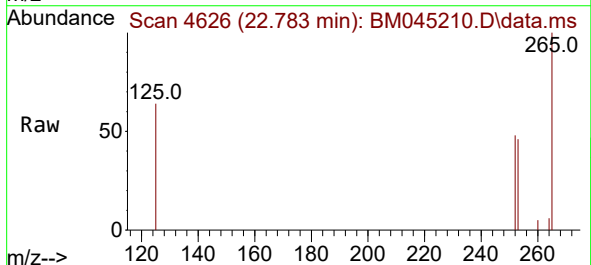

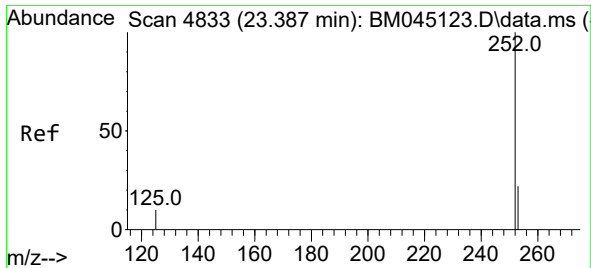

#26
Benzo(a)pyrene
Concen: 0.094 ng/ul
RT: 23.292 min Scan# 41
Delta R.T. -0.072 min
Lab File: BM045210.D
Acq: 13 Apr 2024 18:17

Instrument :
BNA_M
ClientSampleId :
E0ME3

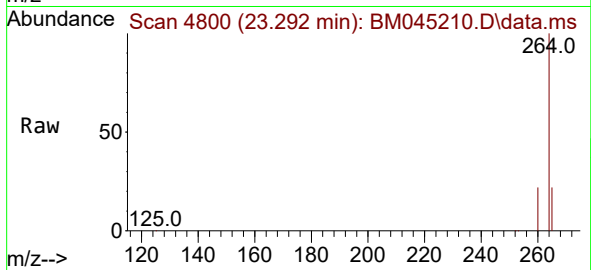

Tgt Ion:252 Resp: 2801
Ion Ratio Lower Upper
252 100
253 58.0 24.6 37.0#
125 41.4 18.2 27.4#

