

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
 Data File : BM045216.D
 Acq On : 13 Apr 2024 21:53
 Operator : MA/JU
 Sample : P2014-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MD6

Quant Time: Apr 15 00:36:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 00:32:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.606	152	1607	0.400	ng/ul	0.00
4) Naphthalene-d8	10.375	136	4670	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.251	164	2451	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.111	188	436060	0.400	ng/ul	# 0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.24
23) Perylene-d12	23.441	264	8428	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	6350	3.008	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.002	152	1801	0.285	ng/ul	0.00
18) Fluoranthene-d10	19.052	212	4335	0.000	ng/ul	-0.01
Target Compounds						
26) Benzo(a)pyrene	23.289	252	2349	0.081	ng/ul#	Qvalue 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045216.D
Acq On : 13 Apr 2024 21:53
Operator : MA/JU
Sample : P2014-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD6


Quant Time: Apr 15 00:36:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration

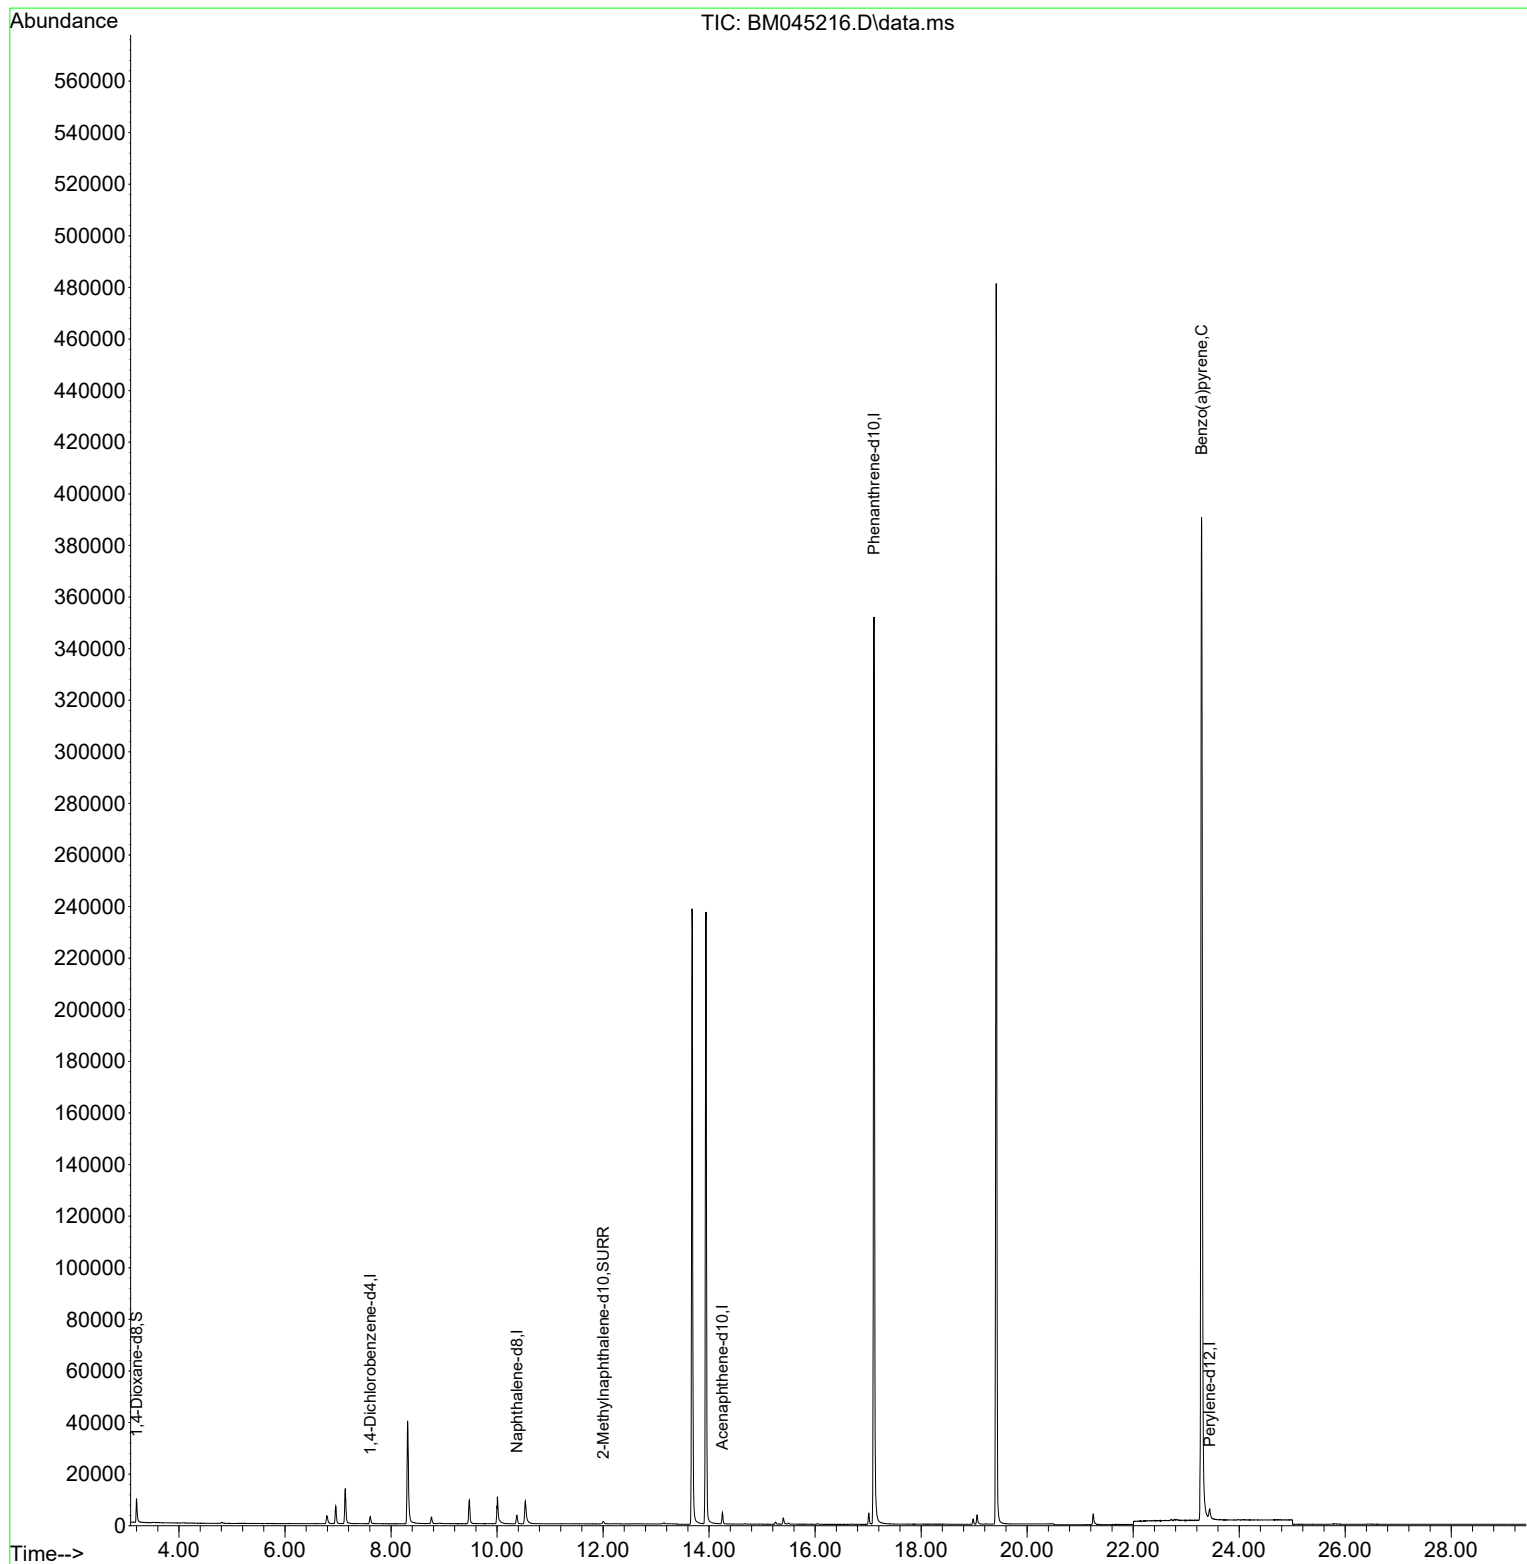

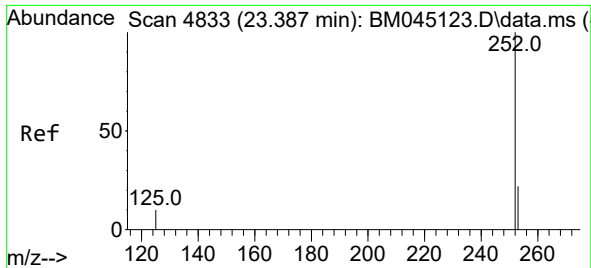

#26
Benzo(a)pyrene
Concen: 0.081 ng/ul
RT: 23.289 min Scan# 41
Delta R.T. -0.075 min
Lab File: BM045216.D
Acq: 13 Apr 2024 21:53

Instrument :
BNA_M
ClientSampleId :
E0MD6

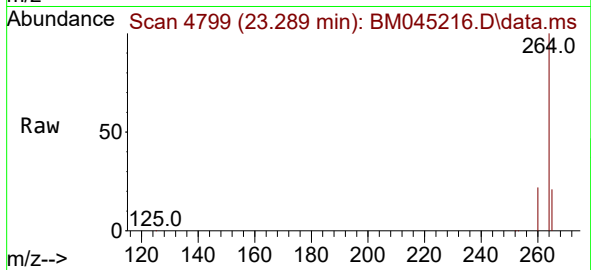

Tgt Ion:252 Resp: 2349
Ion Ratio Lower Upper
252 100
253 55.3 24.6 37.0#
125 36.4 18.2 27.4#

