

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
 Data File : BM045217.D
 Acq On : 13 Apr 2024 22:29
 Operator : MA/JU
 Sample : P2014-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MD7

Quant Time: Apr 15 00:37:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 00:32:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.606	152	1478	0.400	ng/ul	0.00
4) Naphthalene-d8	10.375	136	4260	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.251	164	2229	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.111	188	417927	0.400	ng/ul	# 0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.24
23) Perylene-d12	23.438	264	7390	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	6162	3.174	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.991	152	1761	0.305	ng/ul	0.00
18) Fluoranthene-d10	19.052	212	4563	0.000	ng/ul	-0.01
Target Compounds						
26) Benzo(a)pyrene	23.289	252	2204	0.086	ng/ul#	Qvalue 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045217.D
Acq On : 13 Apr 2024 22:29
Operator : MA/JU
Sample : P2014-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MD7


Quant Time: Apr 15 00:37:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration

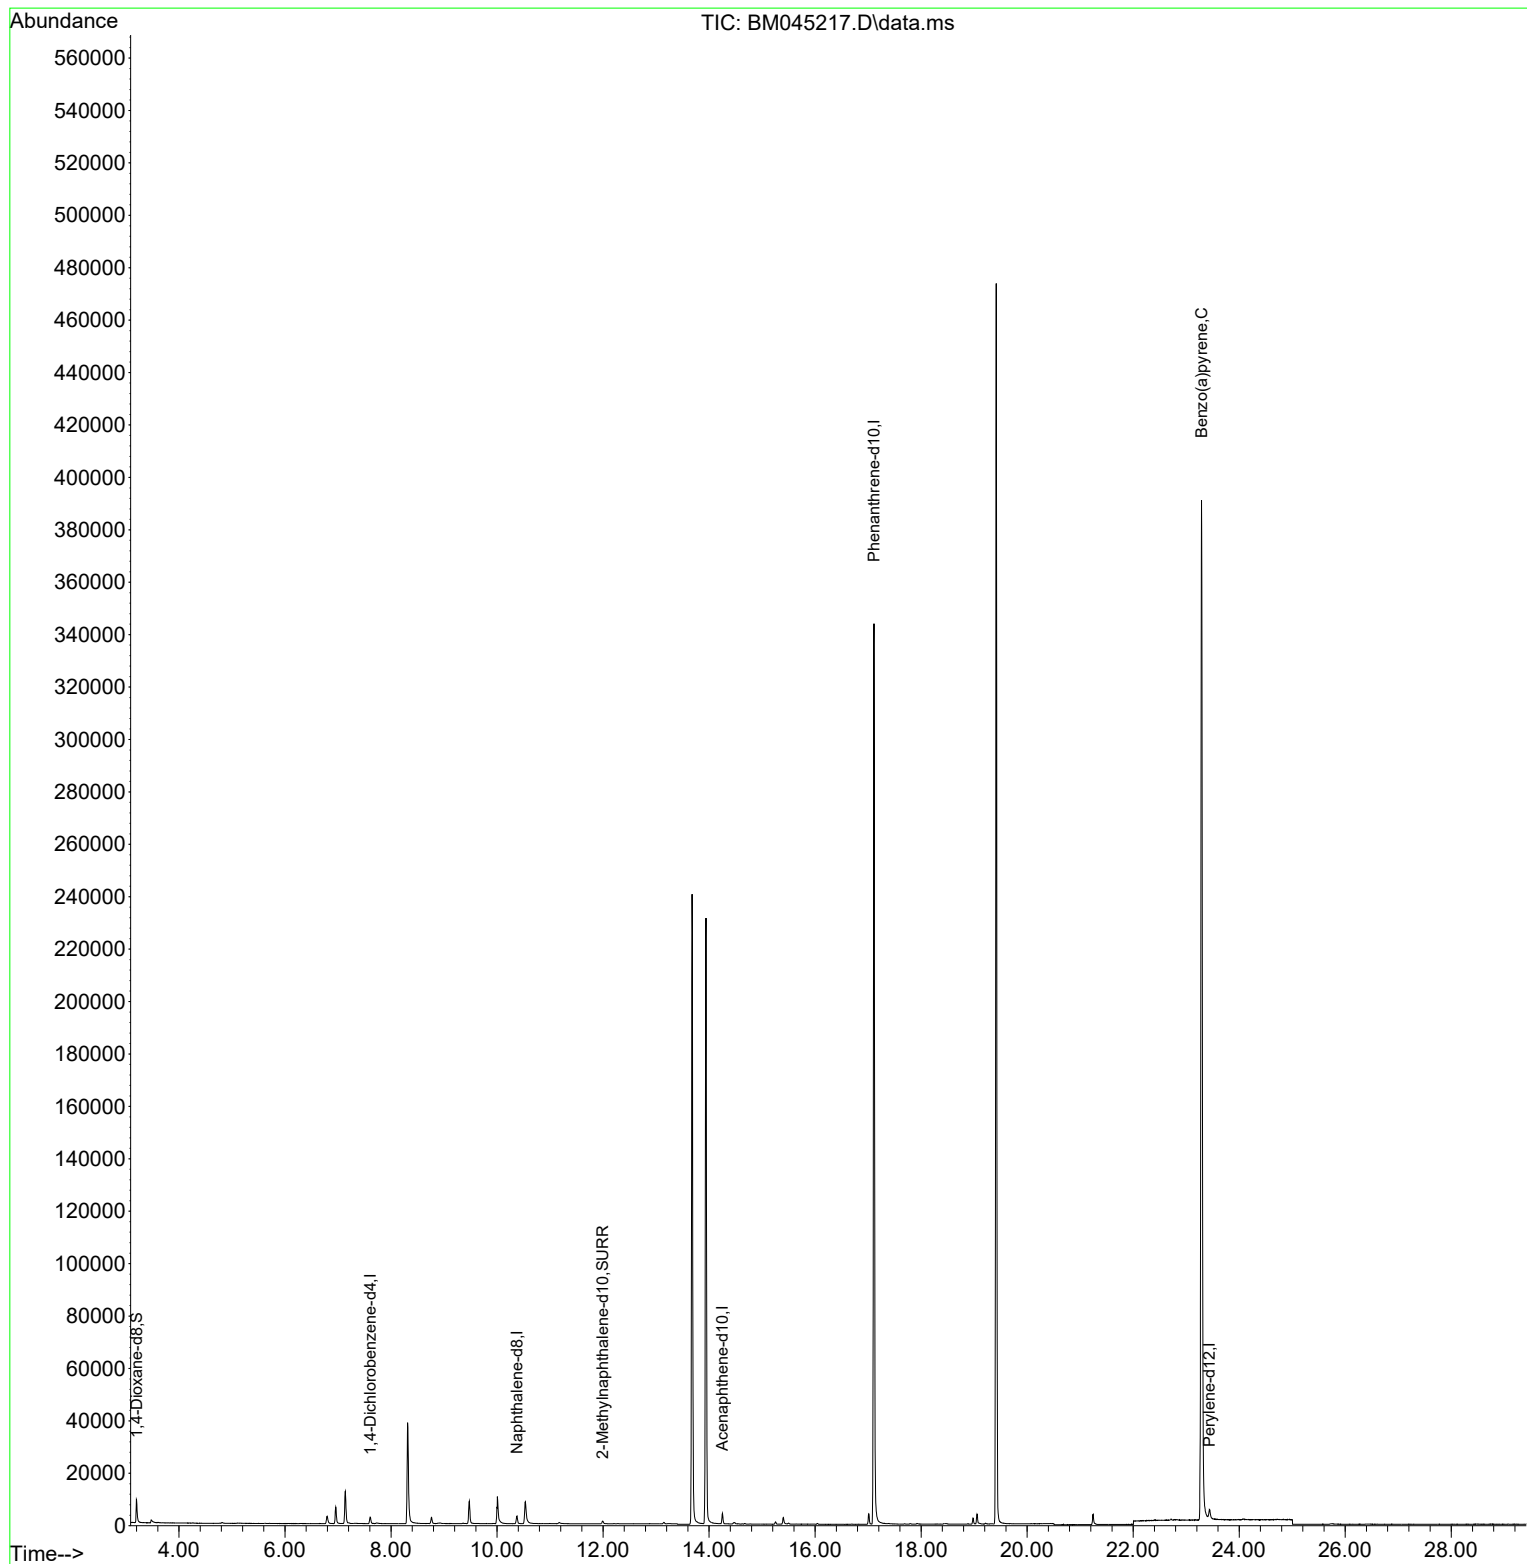

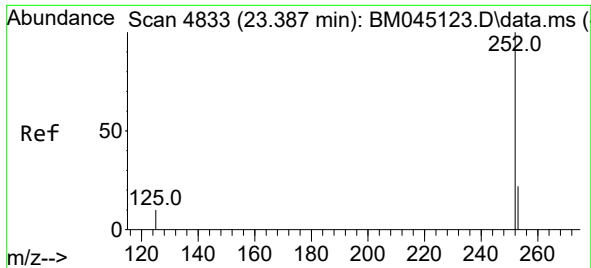

#26
Benzo(a)pyrene
Concen: 0.086 ng/ul
RT: 23.289 min Scan# 41
Delta R.T. -0.075 min
Lab File: BM045217.D
Acq: 13 Apr 2024 22:29

Instrument :
BNA_M
ClientSampleId :
E0MD7

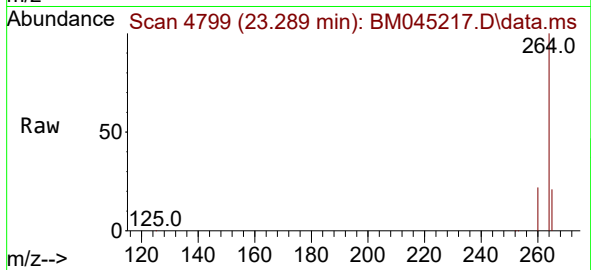

Tgt Ion:252 Resp: 2204
Ion Ratio Lower Upper
252 100
253 56.9 24.6 37.0#
125 39.0 18.2 27.4#

