

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
 Data File : BM045225.D
 Acq On : 14 Apr 2024 03:53
 Operator : MA/JU
 Sample : P2014-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0ME0

Quant Time: Apr 15 00:38:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 00:32:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.606	152	1298	0.400	ng/ul	0.00
4) Naphthalene-d8	10.369	136	3921	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.251	164	2438	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.106	188	472401	0.400	ng/ul	0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.24
23) Perylene-d12	23.437	264	7651	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.197	96	6947	4.074	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.991	152	1952	0.367	ng/ul	0.00
18) Fluoranthene-d10	19.052	212	4965	0.000	ng/ul	-0.02
Target Compounds						
26) Benzo(a)pyrene	23.288	252	2367	0.090	ng/ul#	Qvalue 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045225.D
Acq On : 14 Apr 2024 03:53
Operator : MA/JU
Sample : P2014-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME0


Quant Time: Apr 15 00:38:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration

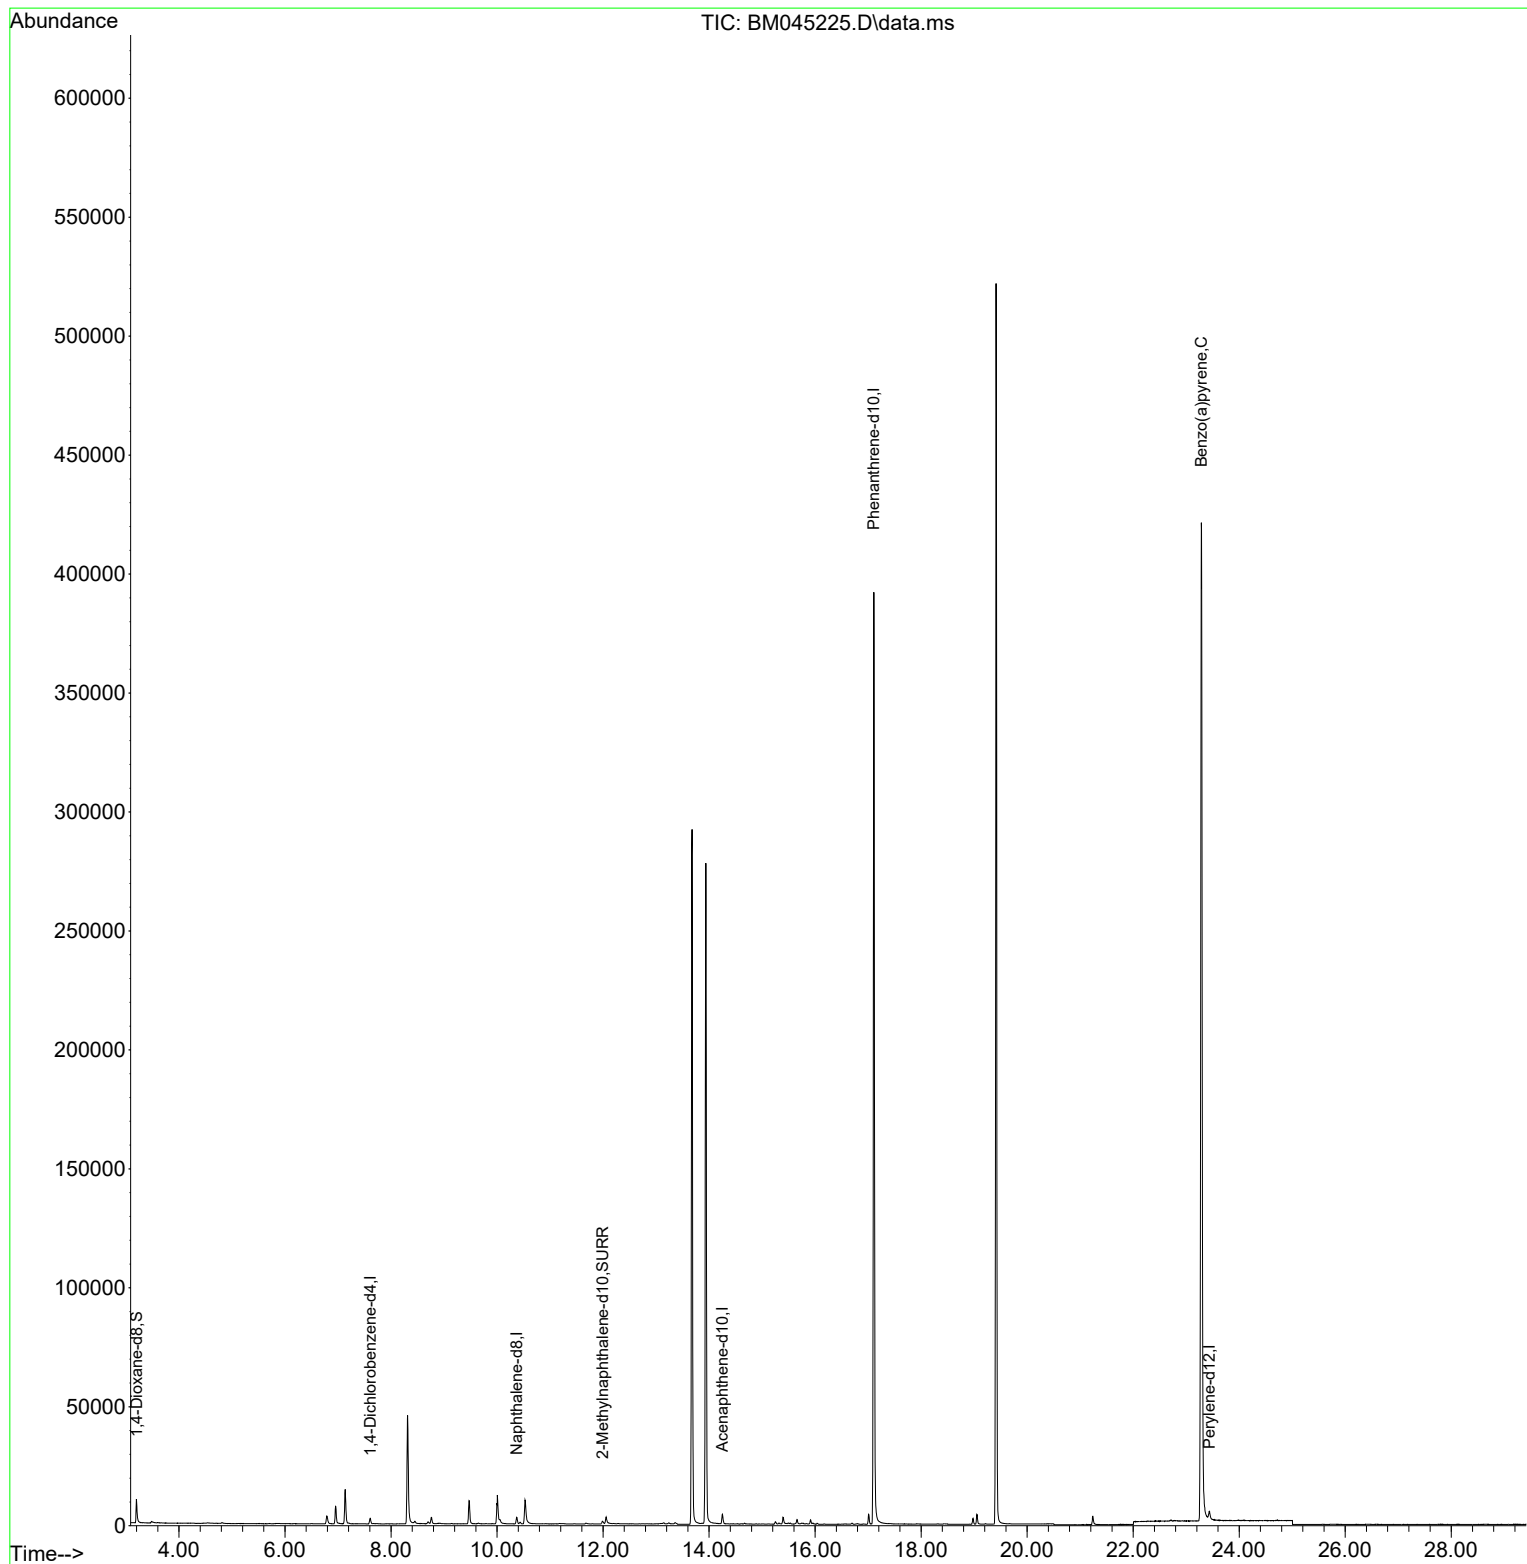

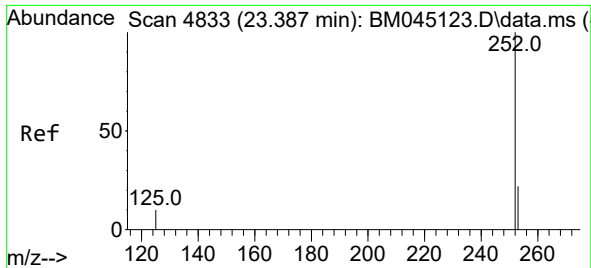

#26
 Benzo(a)pyrene
 Concen: 0.090 ng/ul
 RT: 23.288 min Scan# 41
 Delta R.T. -0.075 min
 Lab File: BM045225.D
 Acq: 14 Apr 2024 03:53

Instrument :
 BNA_M
 ClientSampleId :
 E0ME0

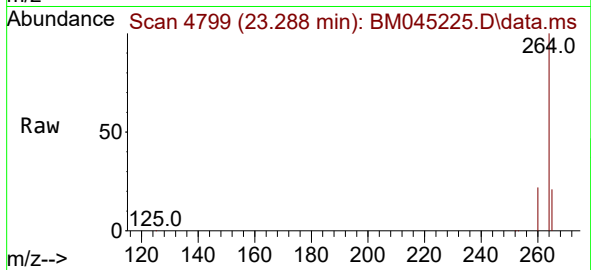

Tgt Ion:252 Resp: 2367
 Ion Ratio Lower Upper
 252 100
 253 54.3 24.6 37.0#
 125 38.5 18.2 27.4#

