

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
 Data File : BM045227.D
 Acq On : 14 Apr 2024 05:05
 Operator : MA/JU
 Sample : P2032-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0ME8

Quant Time: Apr 15 00:38:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 00:32:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.606	152	1281	0.400	ng/ul	0.00
4) Naphthalene-d8	10.373	136	3752	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.250	164	2020	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.109	188	454686	0.400	ng/ul	# 0.08
17) Chrysene-d12	21.250	240	2641	0.400	ng/ul	0.01
23) Perylene-d12	23.436	264	7733	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.196	96	6383	3.793	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.995	152	1965	0.386	ng/ul	0.00
18) Fluoranthene-d10	19.055	212	4669	0.700	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.413	202	987	0.099	ng/ul#	1
26) Benzo(a)pyrene	23.287	252	2328	0.087	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045227.D
Acq On : 14 Apr 2024 05:05
Operator : MA/JU
Sample : P2032-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOME8

Quant Time: Apr 15 00:38:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration




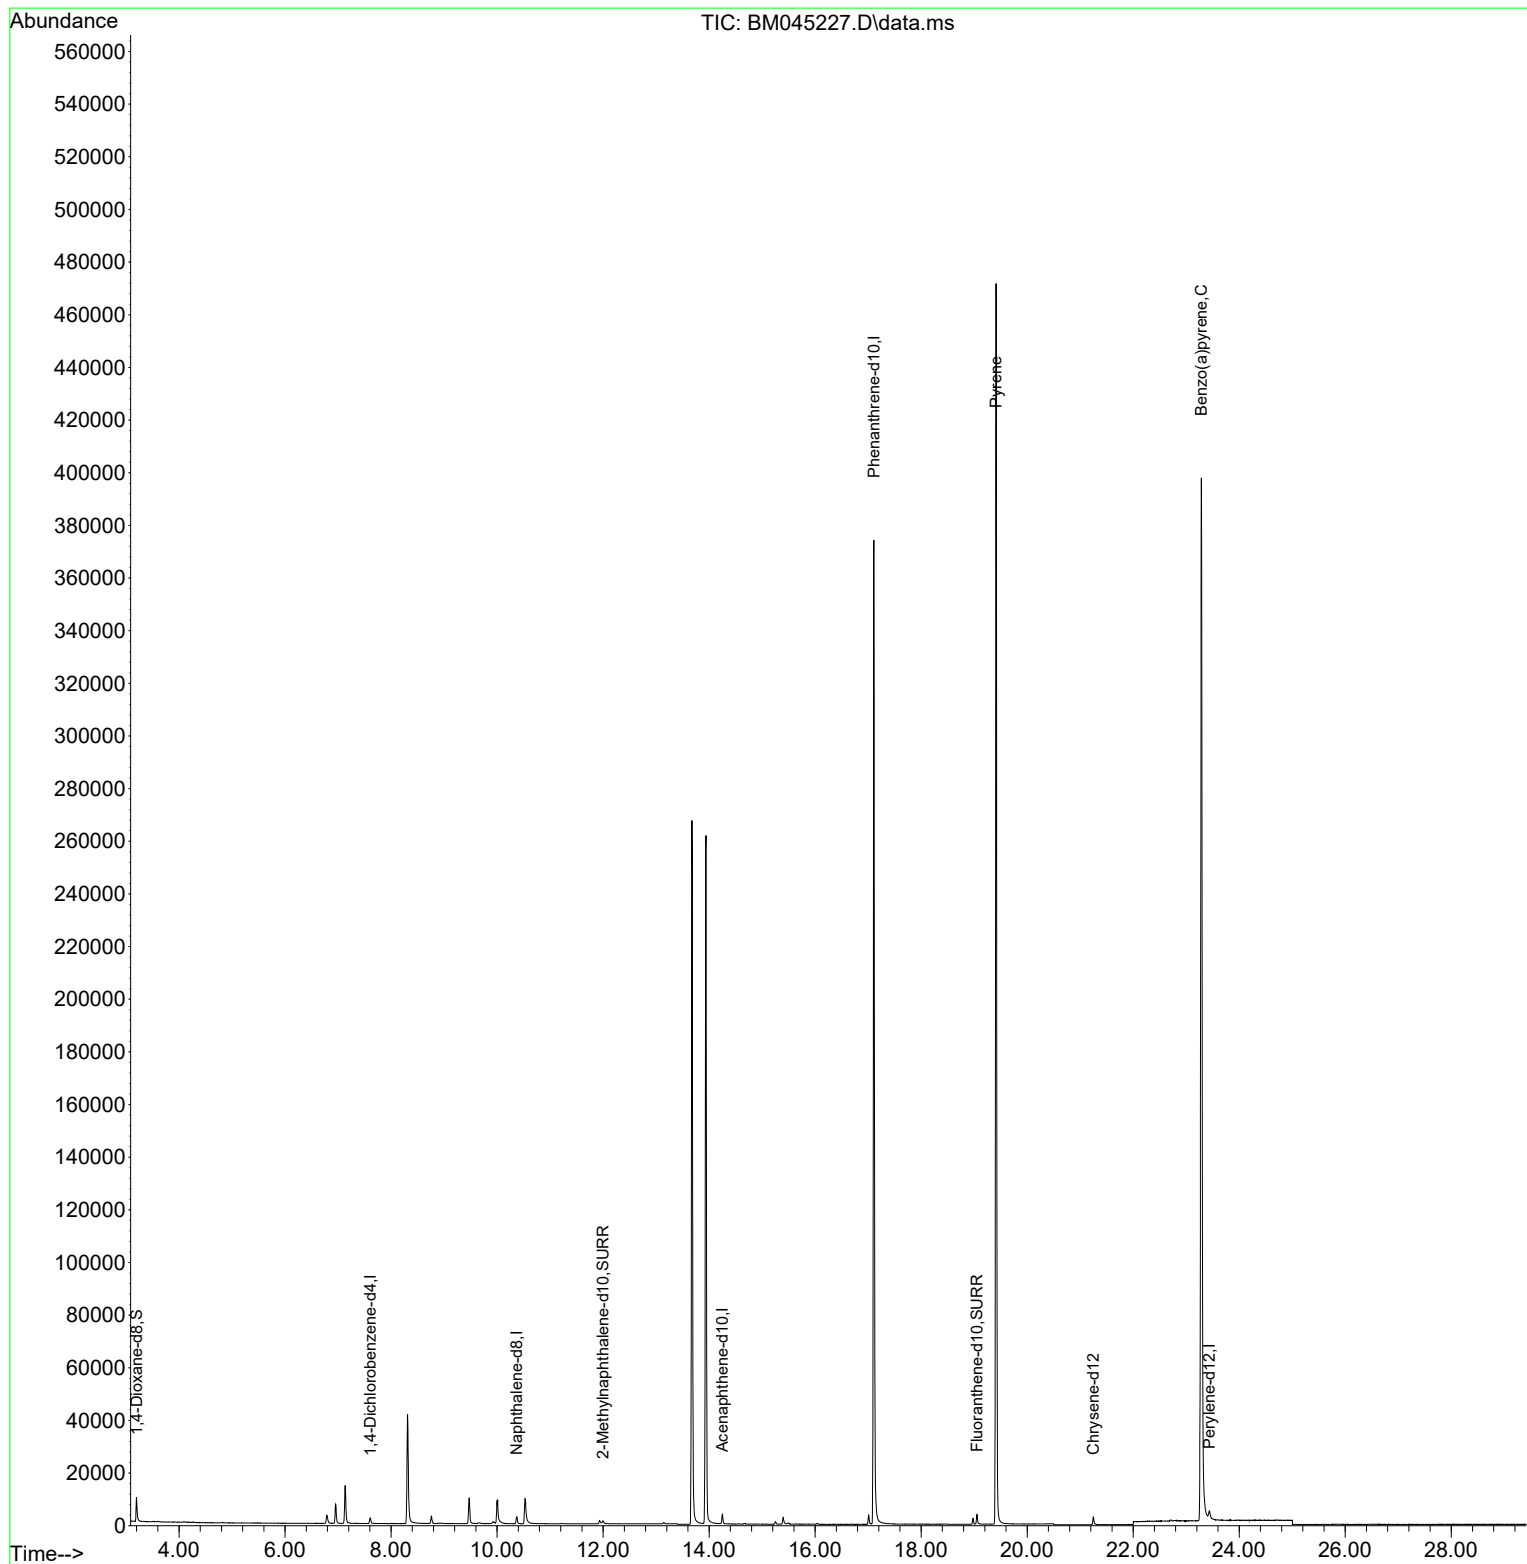


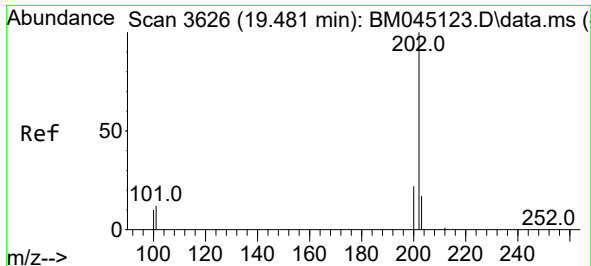

#20
Pyrene
Concen: 0.099 ng/ul
RT: 19.413 min Scan# 30
Delta R.T. -0.049 min
Lab File: BM045227.D
Acq: 14 Apr 2024 05:05

Instrument :
BNA_M
ClientSampleId :
EOME8

Tgt Ion:202 Resp: 987
Ion Ratio Lower Upper
202 100
101 172.8 9.8 14.6#
100 1301.9 8.1 12.1#

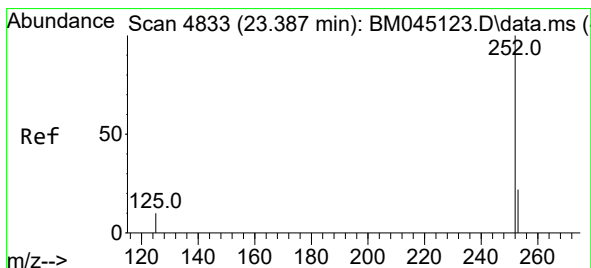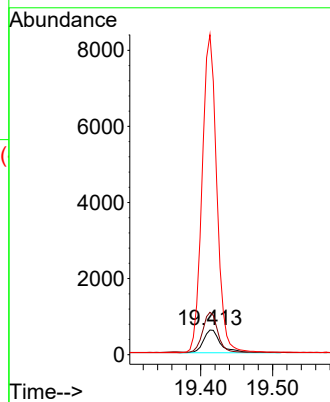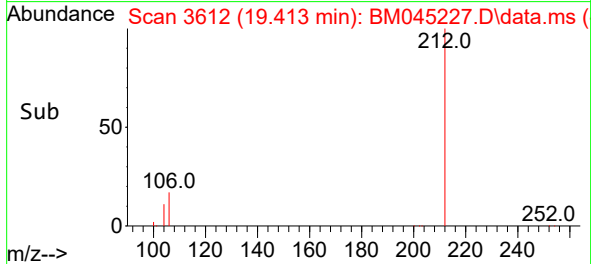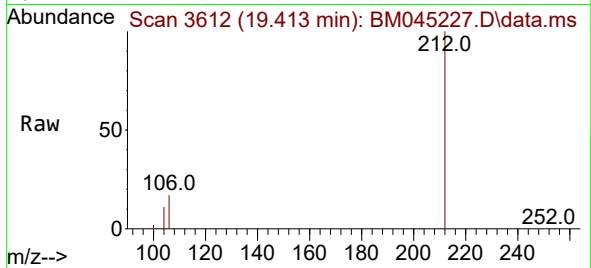

#26
Benzo(a)pyrene
Concen: 0.087 ng/ul
RT: 23.287 min Scan# 4799
Delta R.T. -0.077 min
Lab File: BM045227.D
Acq: 14 Apr 2024 05:05

Tgt Ion:252 Resp: 2328
Ion Ratio Lower Upper
252 100
253 54.9 24.6 37.0#
125 36.1 18.2 27.4#

