

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
 Data File : BM045228.D
 Acq On : 14 Apr 2024 05:41
 Operator : MA/JU
 Sample : P2036-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCSW7

Quant Time: Apr 15 00:38:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 00:32:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.606	152	1217	0.400	ng/ul	0.00
4) Naphthalene-d8	10.375	136	3705	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.251	164	1963	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.106	188	365056	0.400	ng/ul	0.08
17) Chrysene-d12	21.249	240	2963	0.400	ng/ul	0.00
23) Perylene-d12	23.435	264	7101	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.197	96	5331	3.335	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.008	152	1487	0.296	ng/ul	0.01
18) Fluoranthene-d10	19.052	212	3673	0.491	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.415	202	762	0.068	ng/ul#	1
26) Benzo(a)pyrene	23.286	252	1819	0.074	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045228.D
Acq On : 14 Apr 2024 05:41
Operator : MA/JU
Sample : P2036-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSW7

Quant Time: Apr 15 00:38:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration




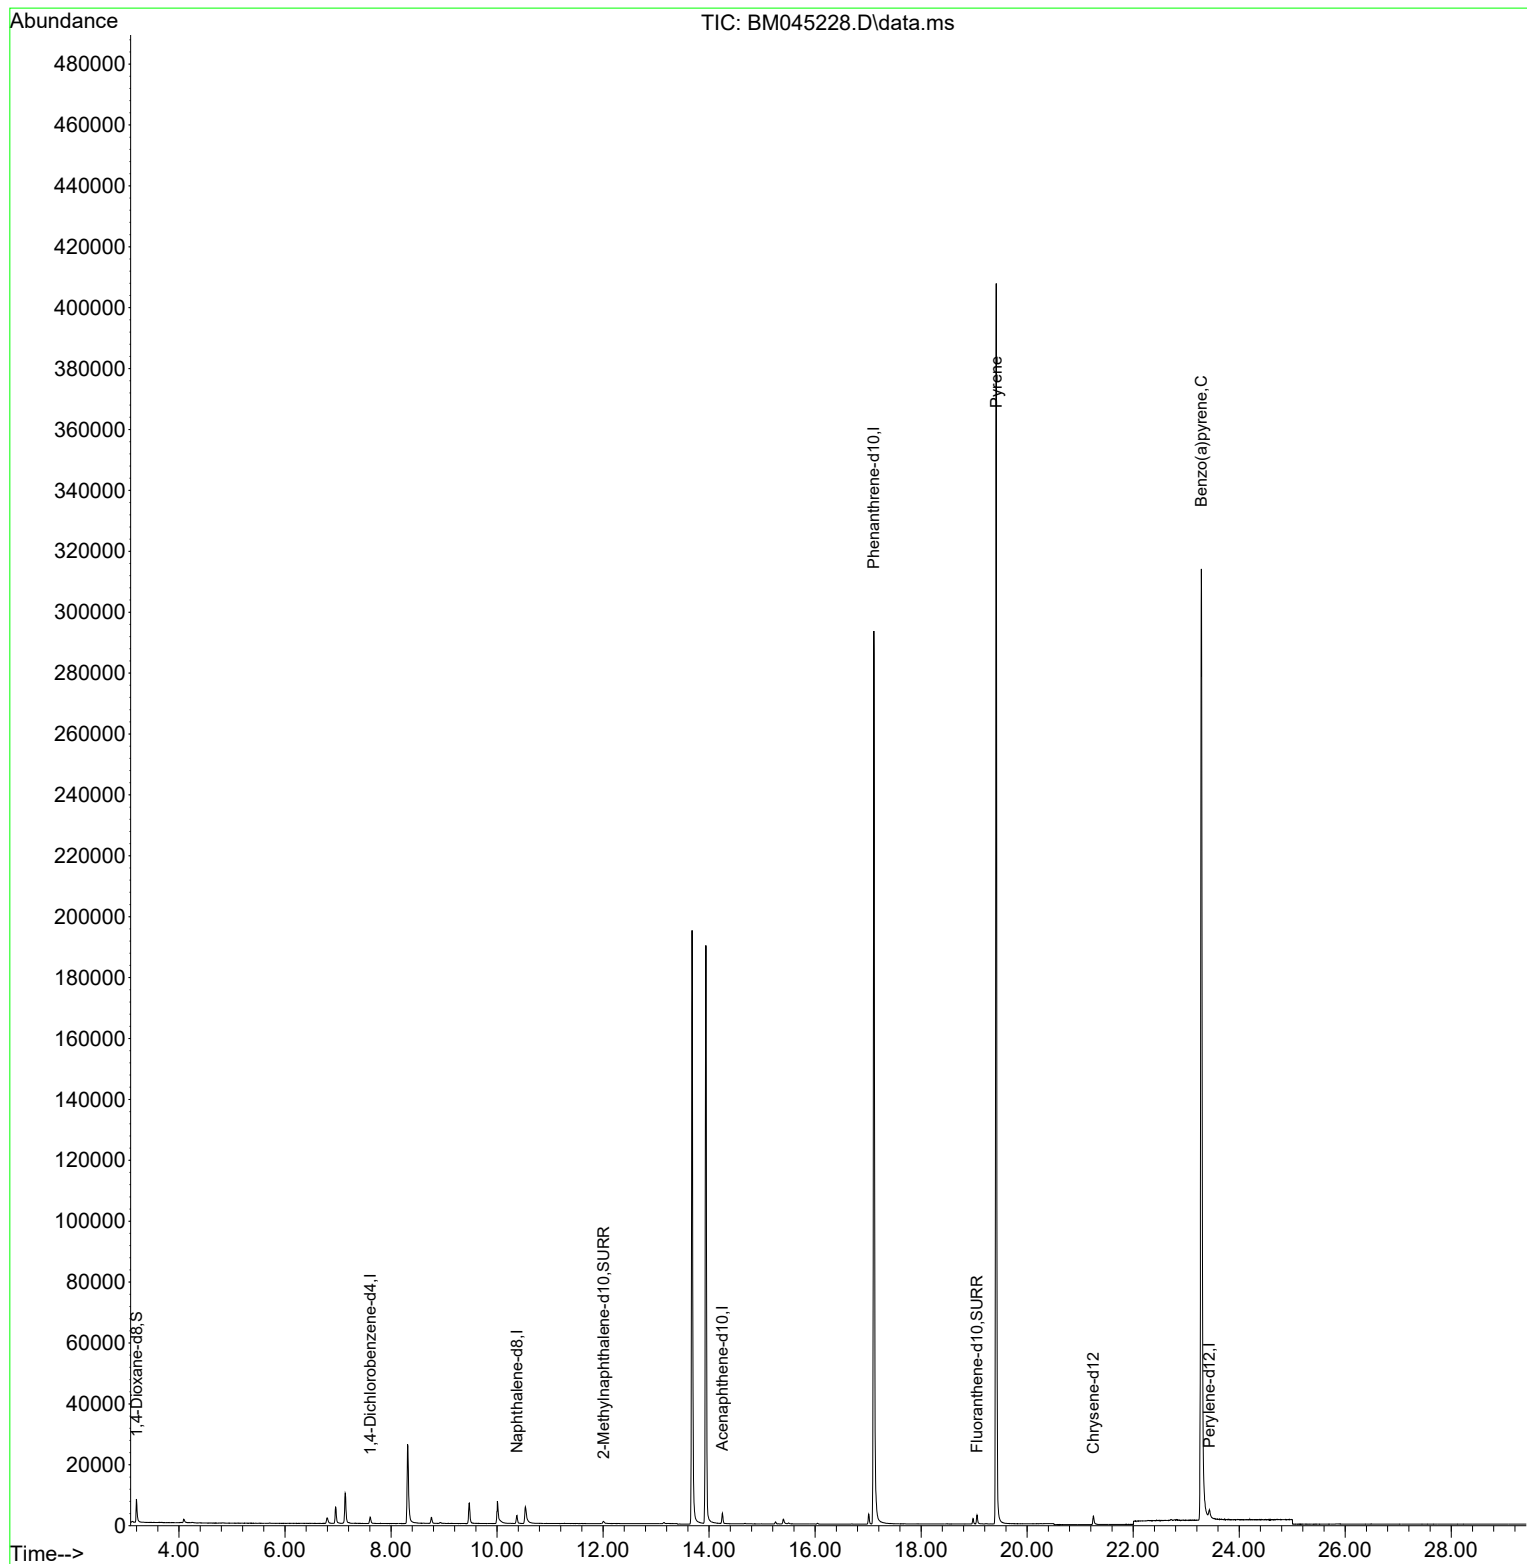


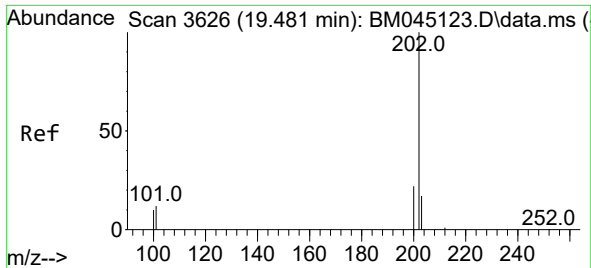

#20
Pyrene
Concen: 0.068 ng/ul
RT: 19.415 min Scan# 30
Delta R.T. -0.047 min
Lab File: BM045228.D
Acq: 14 Apr 2024 05:41

Instrument :
BNA_M
ClientSampleId :
YCSW7

Tgt Ion:202 Resp: 762
Ion Ratio Lower Upper
202 100
101 156.2 9.8 14.6#
100 1181.3 8.1 12.1#

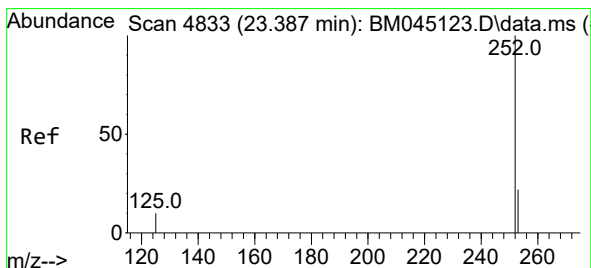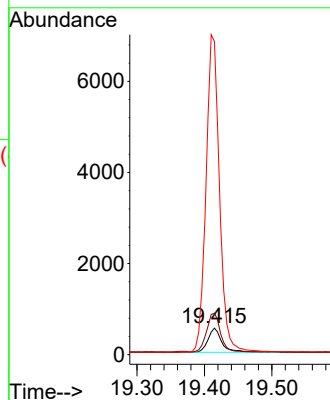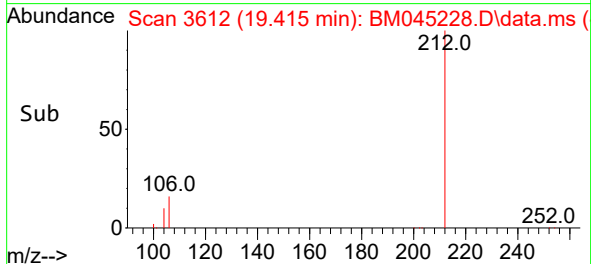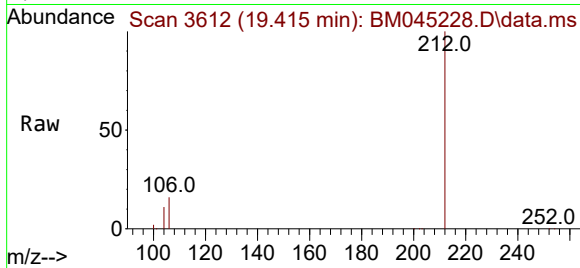

#26
Benzo(a)pyrene
Concen: 0.074 ng/ul
RT: 23.286 min Scan# 4798
Delta R.T. -0.078 min
Lab File: BM045228.D
Acq: 14 Apr 2024 05:41

Tgt Ion:252 Resp: 1819
Ion Ratio Lower Upper
252 100
253 57.8 24.6 37.0#
125 38.7 18.2 27.4#

