

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
 Data File : BM045239.D
 Acq On : 14 Apr 2024 12:52
 Operator : MA/JU
 Sample : PB160205BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK205

Quant Time: Apr 15 00:40:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 00:32:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.606	152	1155	0.400	ng/ul	0.00
4) Naphthalene-d8	10.369	136	3411	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.251	164	1769	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.106	188	316191	0.400	ng/ul	# 0.08
17) Chrysene-d12	21.255	240	2653	0.400	ng/ul	# 0.02
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.46
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.197	96	9373	6.178	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.008	152	1494	0.323	ng/ul	0.01
18) Fluoranthene-d10	19.057	212	3095	0.462	ng/ul	-0.01
Target Compounds						
					Qvalue	
12) Fluorene	15.251	166	626	0.088	ng/ul#	20
20) Pyrene	19.415	202	612	0.061	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045239.D
Acq On : 14 Apr 2024 12:52
Operator : MA/JU
Sample : PB160205BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK205

Quant Time: Apr 15 00:40:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration

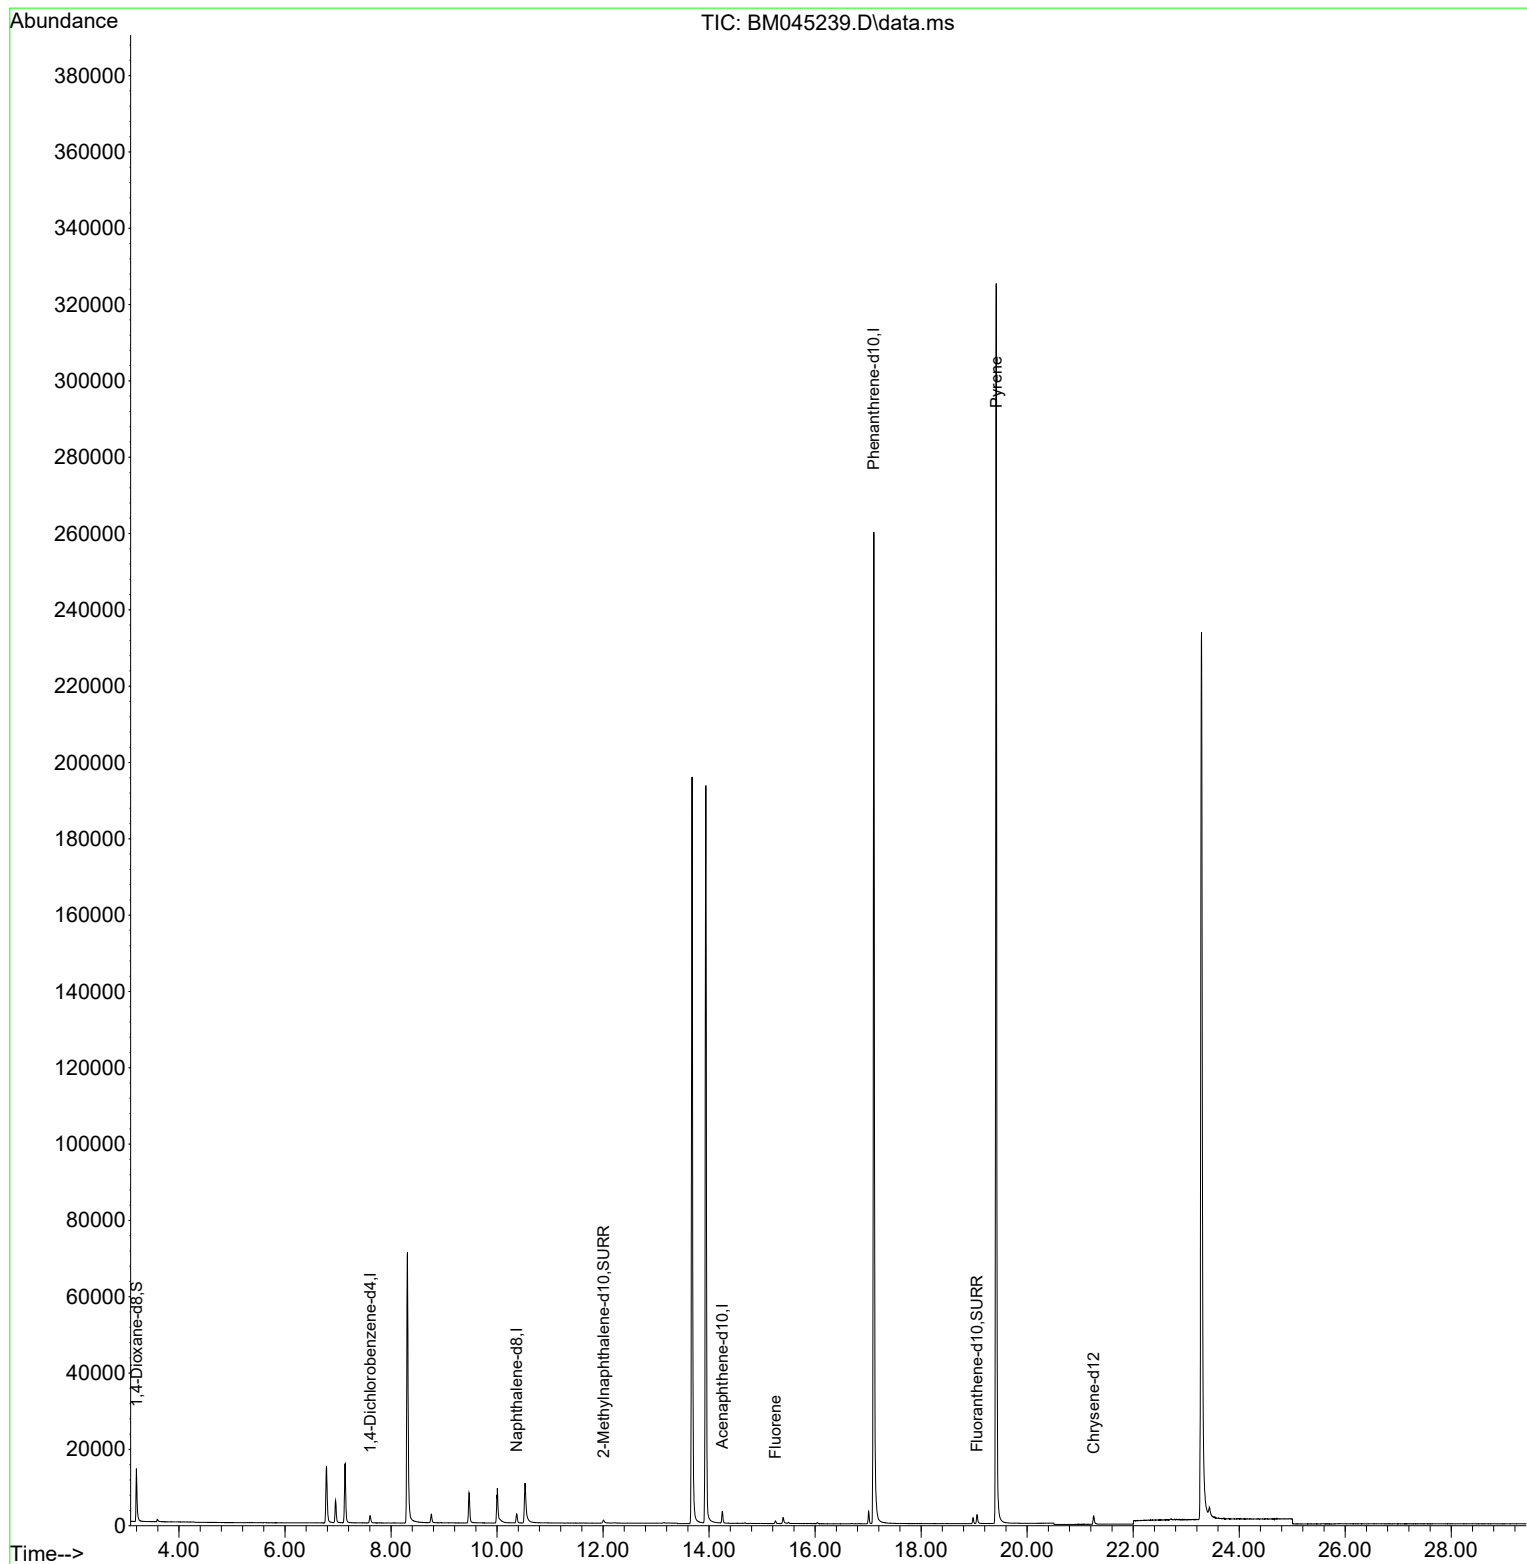

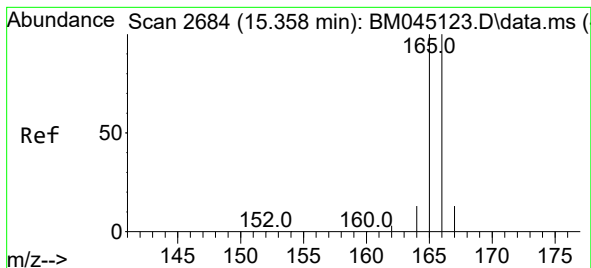

#12

Fluorene

Concen: 0.088 ng/ul

RT: 15.251 min Scan# 2

Delta R.T. -0.079 min

Lab File: BM045239.D

Acq: 14 Apr 2024 12:52

Instrument :

BNA_M

ClientSampleId :

SBLK205





Tgt Ion:166 Resp: 626

Ion Ratio Lower Upper

166 100

165 16.6 79.9 119.9#

167 38.9 12.2 18.2#

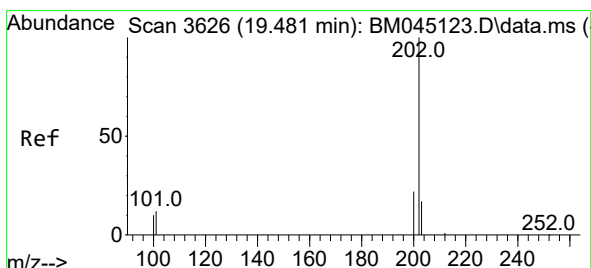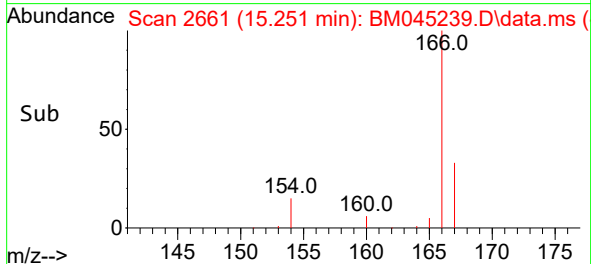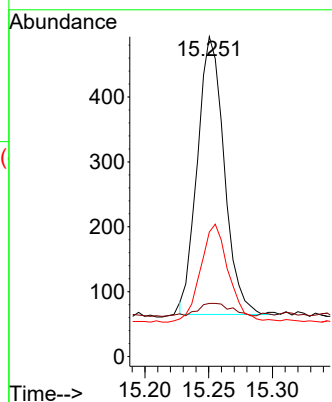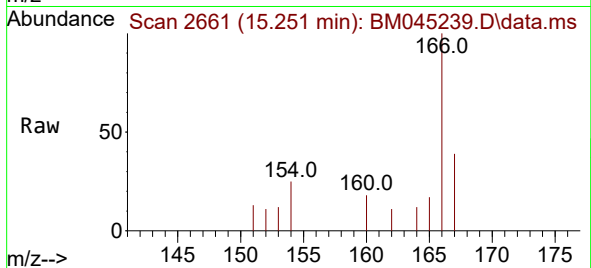

#20

Pyrene

Concen: 0.061 ng/ul

RT: 19.415 min Scan# 3612

Delta R.T. -0.047 min

Lab File: BM045239.D

Acq: 14 Apr 2024 12:52

Tgt Ion:202 Resp: 612

Ion Ratio Lower Upper

202 100

101 173.5 9.8 14.6#

100 1298.9 8.1 12.1#

