




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045211.D
Acq On : 13 Apr 2024 18:53
Operator : MA/JU
Sample : P2014-19
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME4

Manual IntegrationsAPPROVED

Quant Time: Apr 15 00:36:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/17/2024

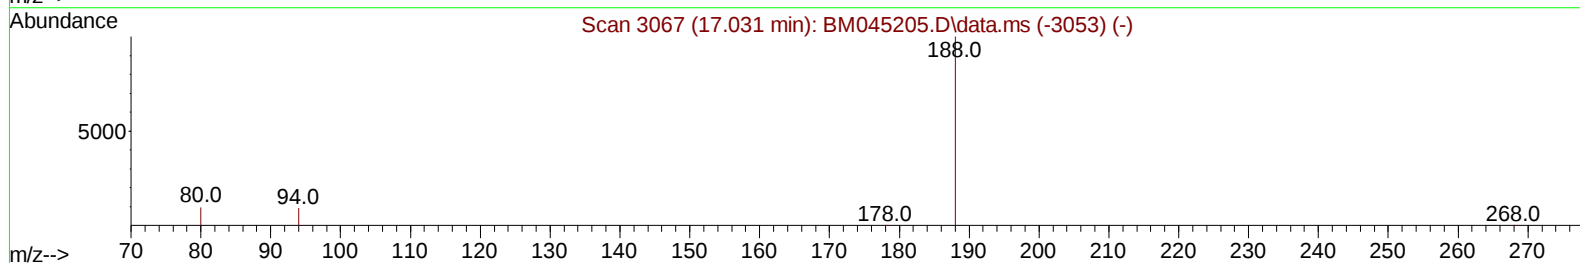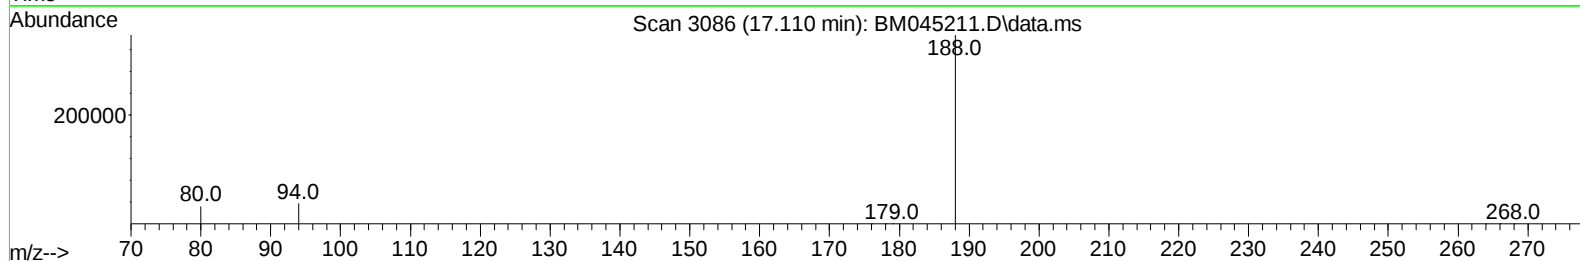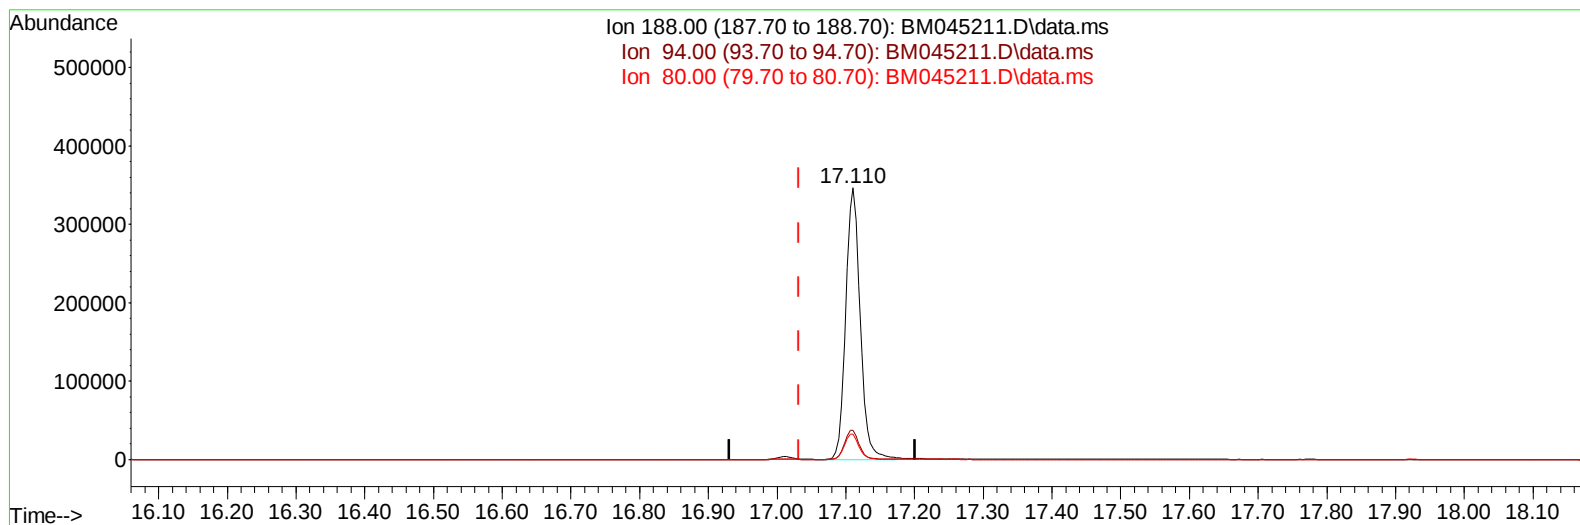

TIC: BM045211.D\data.ms

(13) Phenanthrene-d10 (I)

17.110min (+ 0.079) 0.40 ng/u1

response 510296

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.00	10.72
80.00	11.80	9.24#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045211.D
Acq On : 13 Apr 2024 18:53
Operator : MA/JU
Sample : P2014-19
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME4

Manual IntegrationsAPPROVED

Quant Time: Apr 15 00:36:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/17/2024

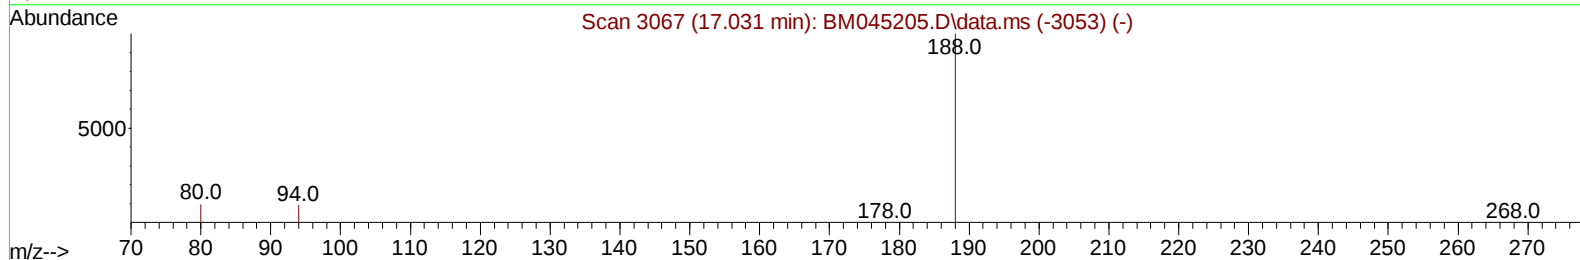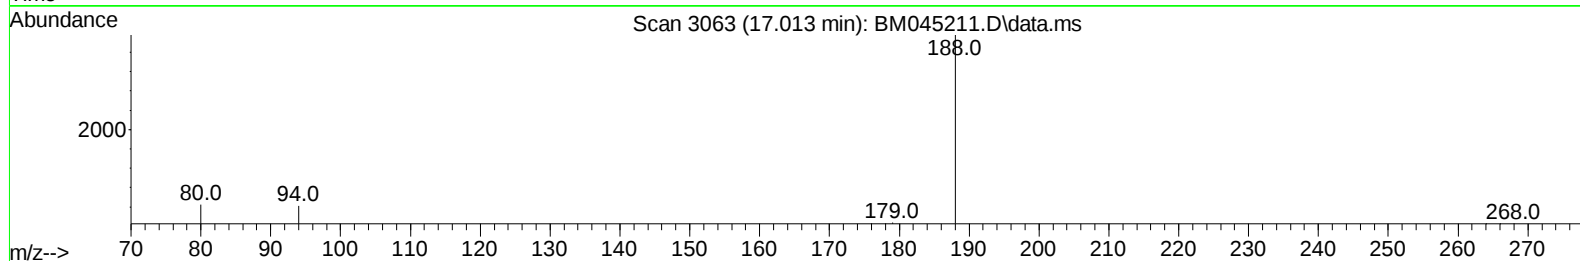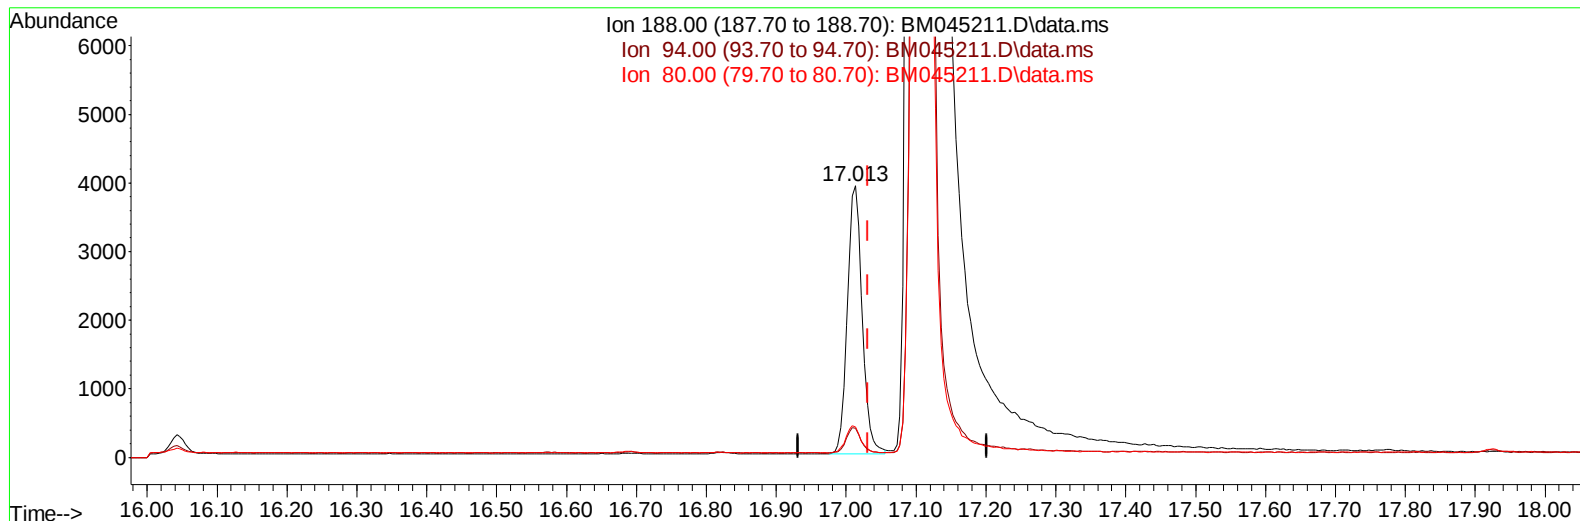

TIC: BM045211.D\data.ms

(13) Phenanthrene-d10 (I)

17.013min (-0.018) 0.40 ng/ul m

response 5730

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.00	10.69
80.00	11.80	11.22
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045211.D
Acq On : 13 Apr 2024 18:53
Operator : MA/JU
Sample : P2014-19
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/17/2024

Quant Time: Apr 15 00:36:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration

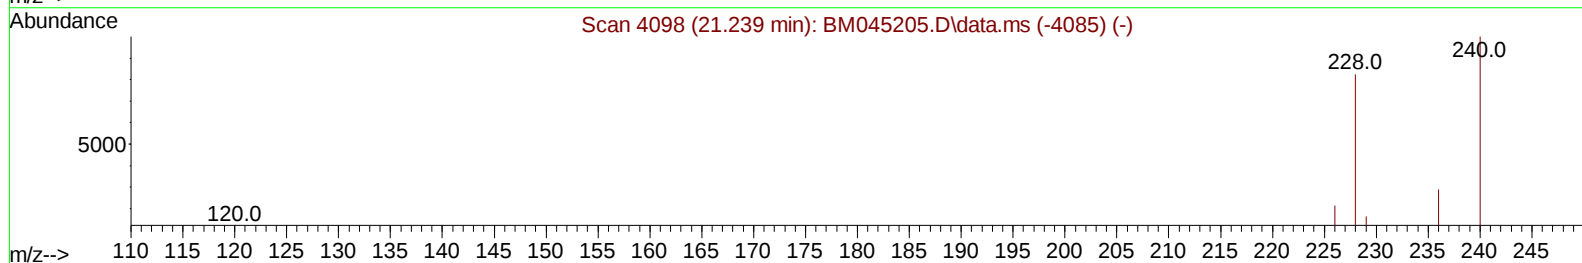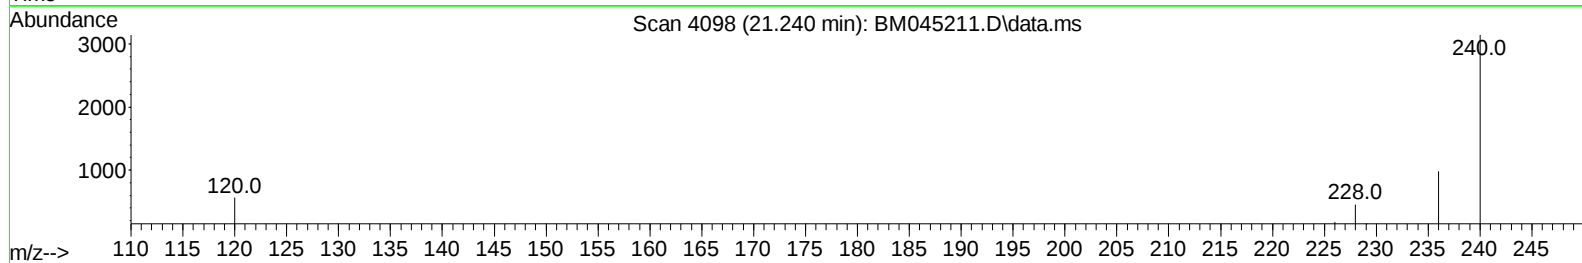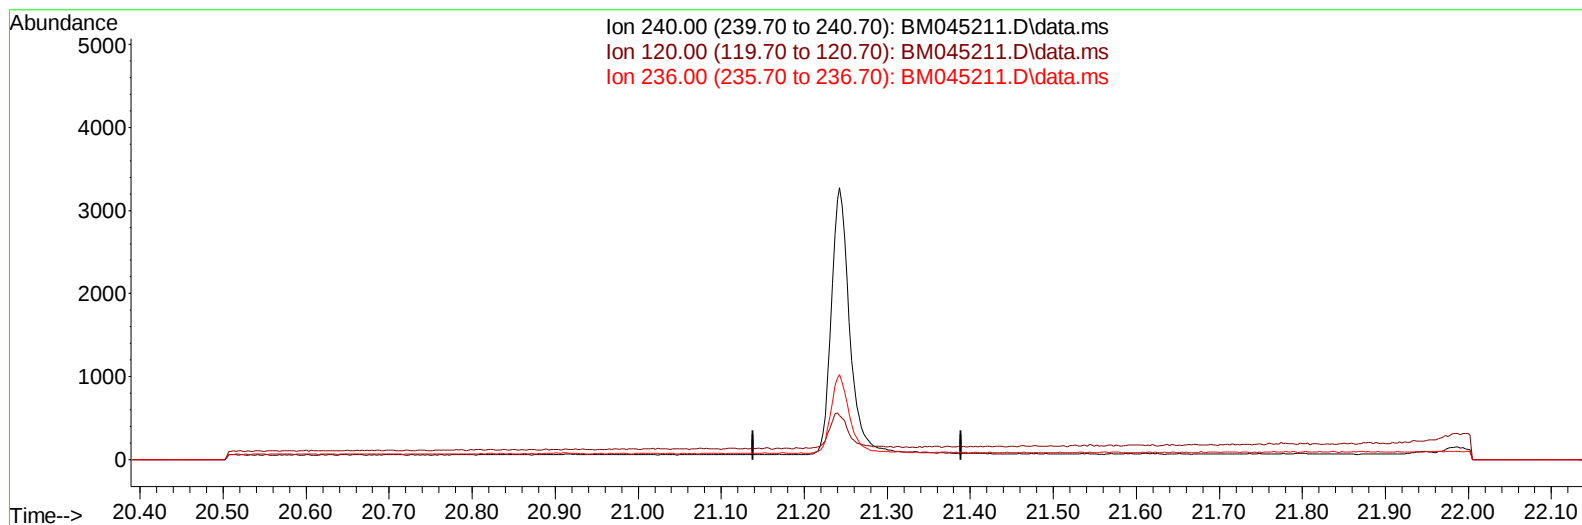

TIC: BM045211.D\data.ms

(17) Chrysene-d12

21.239min (-21.239) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.80	0.00#
236.00	31.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045211.D
Acq On : 13 Apr 2024 18:53
Operator : MA/JU
Sample : P2014-19
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME4

Manual IntegrationsAPPROVED

Quant Time: Apr 15 00:36:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/17/2024

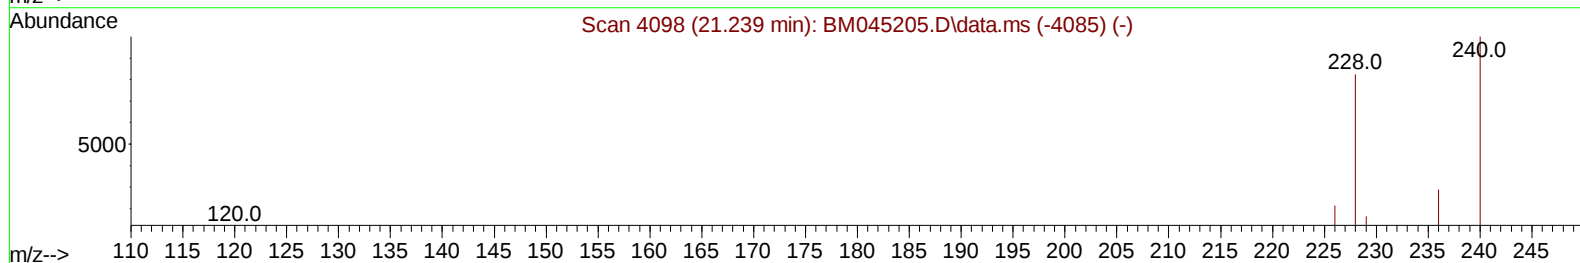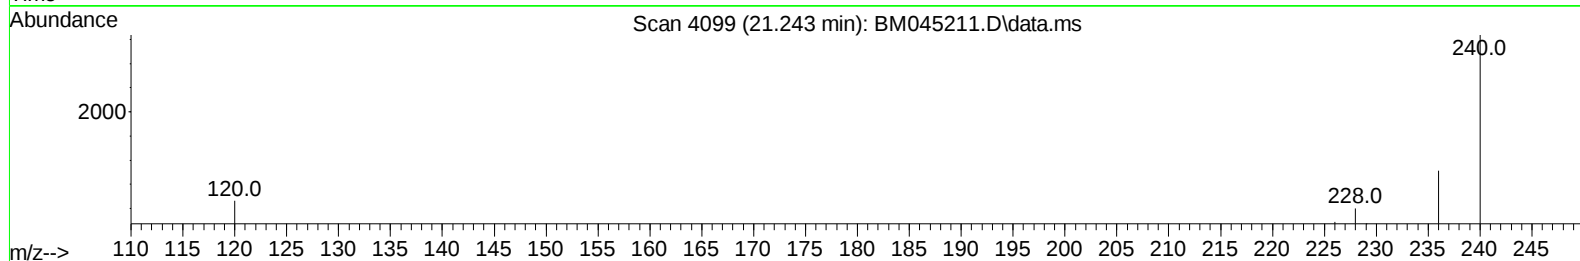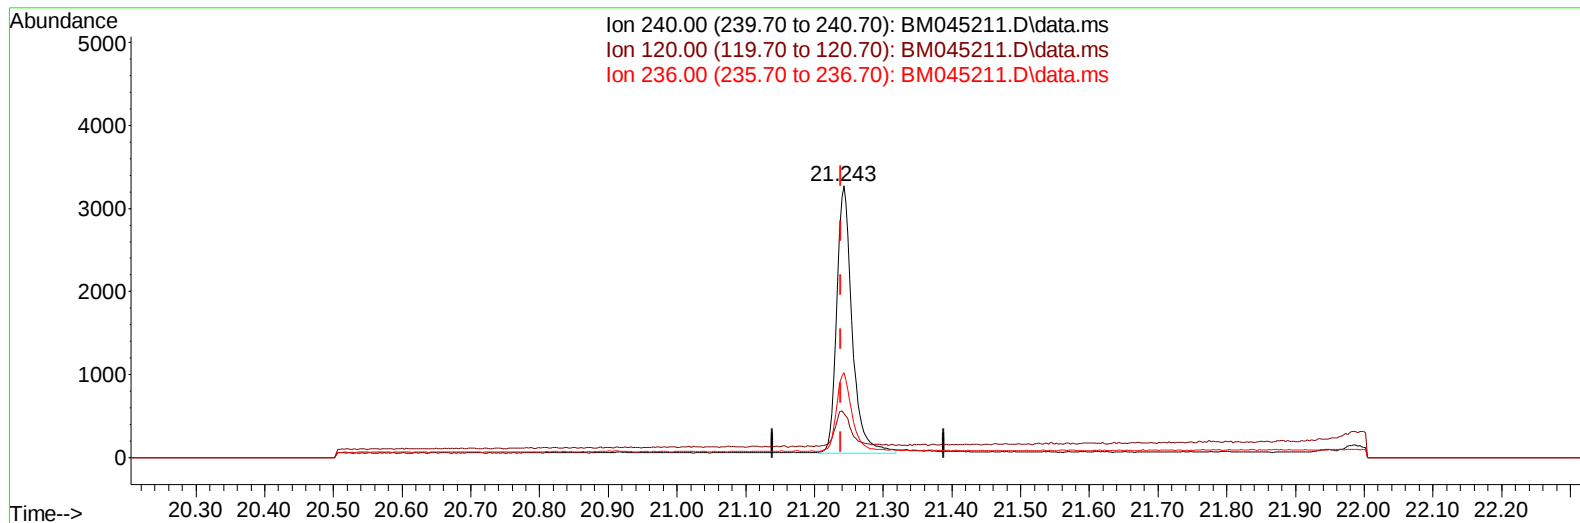

TIC: BM045211.D\data.ms

(17) Chrysene-d12

21.243min (+ 0.004) 0.40 ng/ul m

response 5007

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	16.29
236.00	31.10	31.27
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045211.D
Acq On : 13 Apr 2024 18:53
Operator : MA/JU
Sample : P2014-19
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/17/2024

Quant Time: Apr 15 00:36:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration

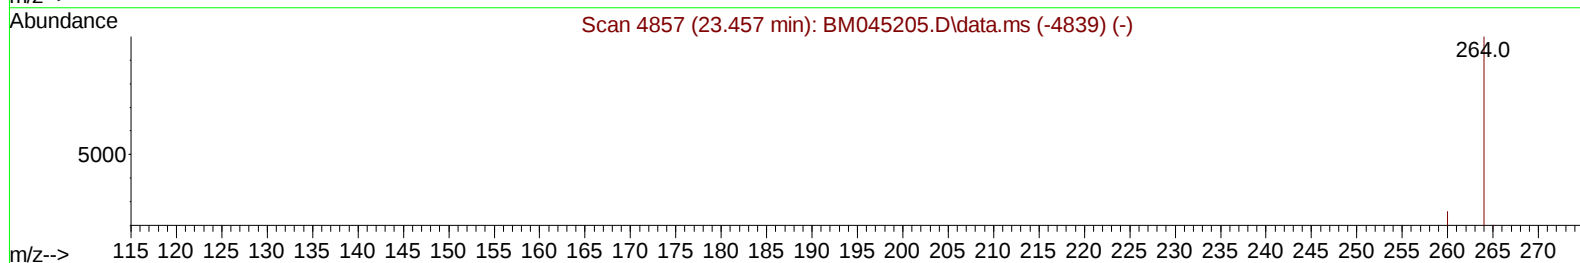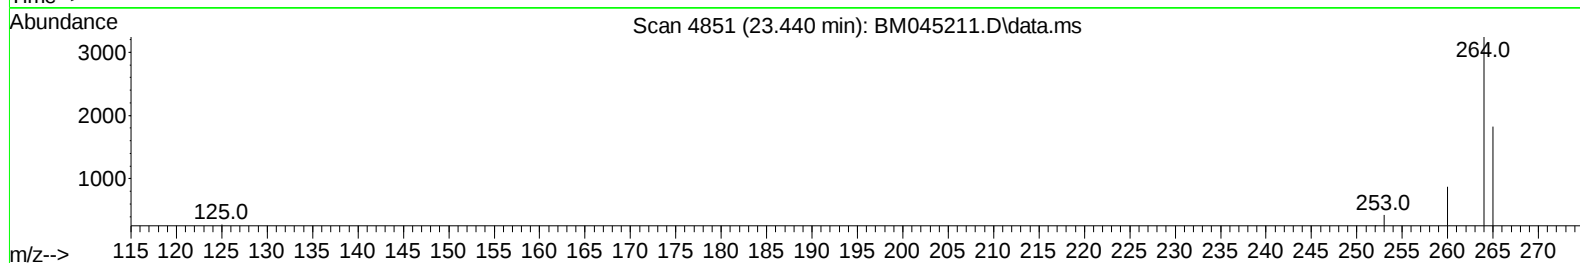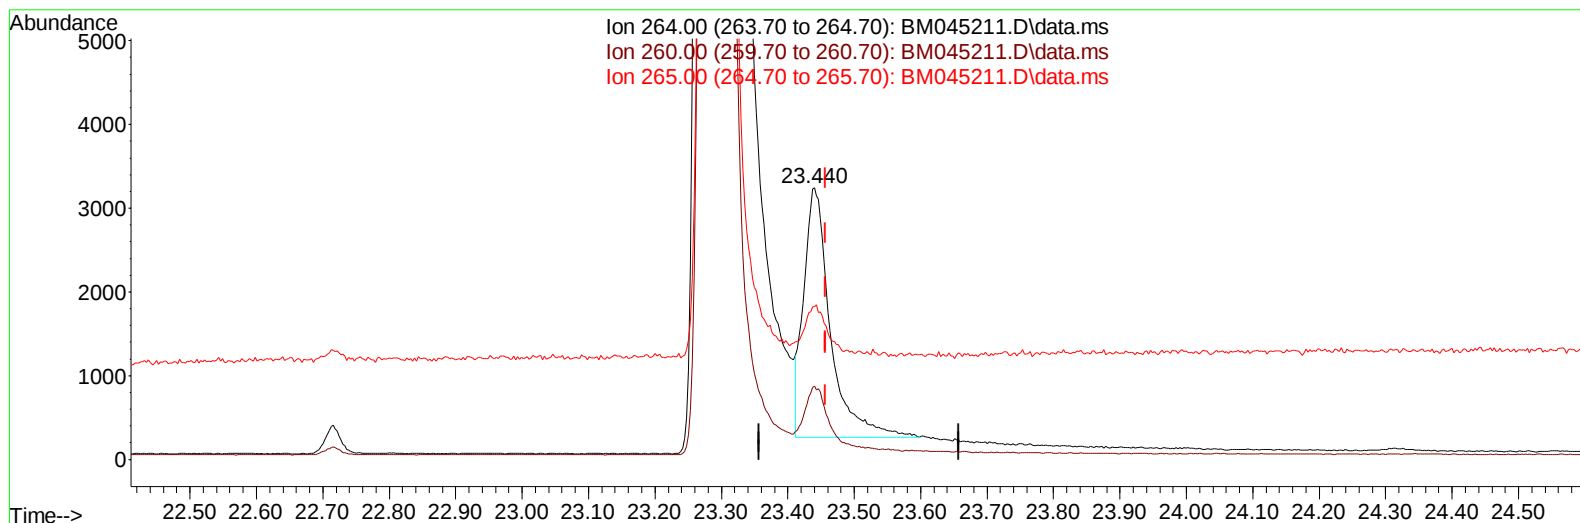

TIC: BM045211.D\data.ms

(23) Perylene-d12 (I)

23.440min (-0.017) 0.40 ng/u1

response 8381

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	27.02
265.00	70.40	56.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
 Data File : BM045211.D
 Acq On : 13 Apr 2024 18:53
 Operator : MA/JU
 Sample : P2014-19
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0ME4

Manual IntegrationsAPPROVED

Quant Time: Apr 15 00:36:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 00:32:25 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/17/2024

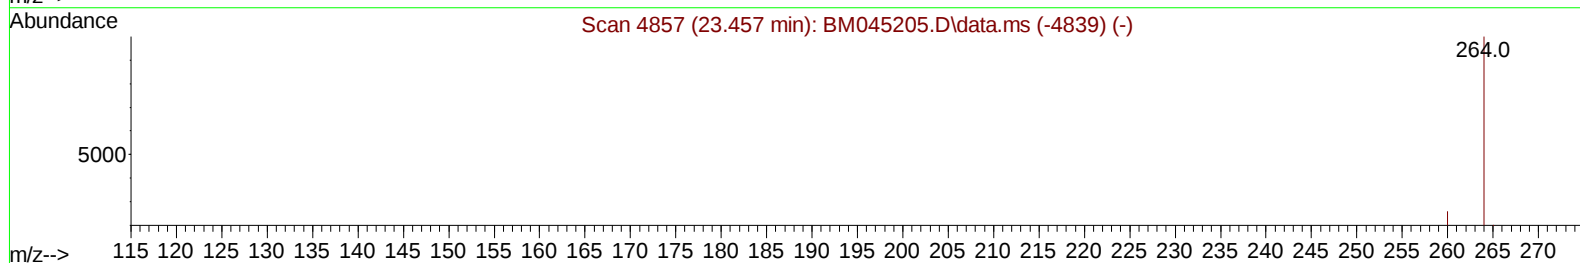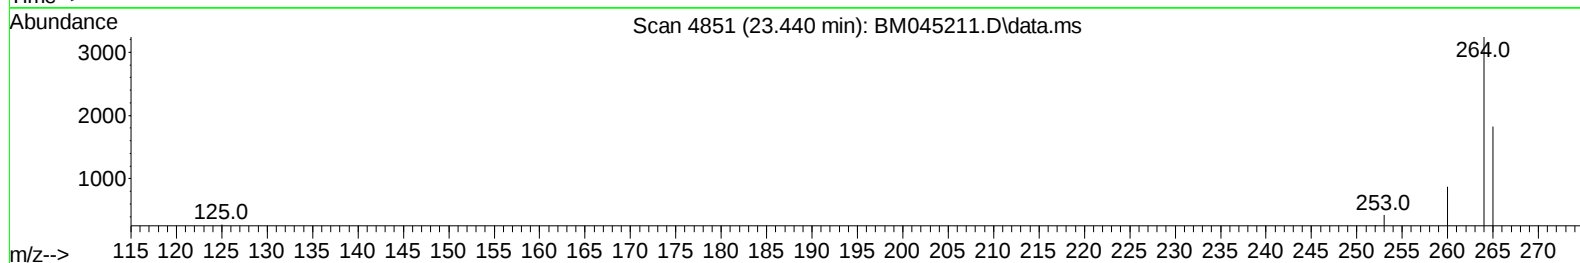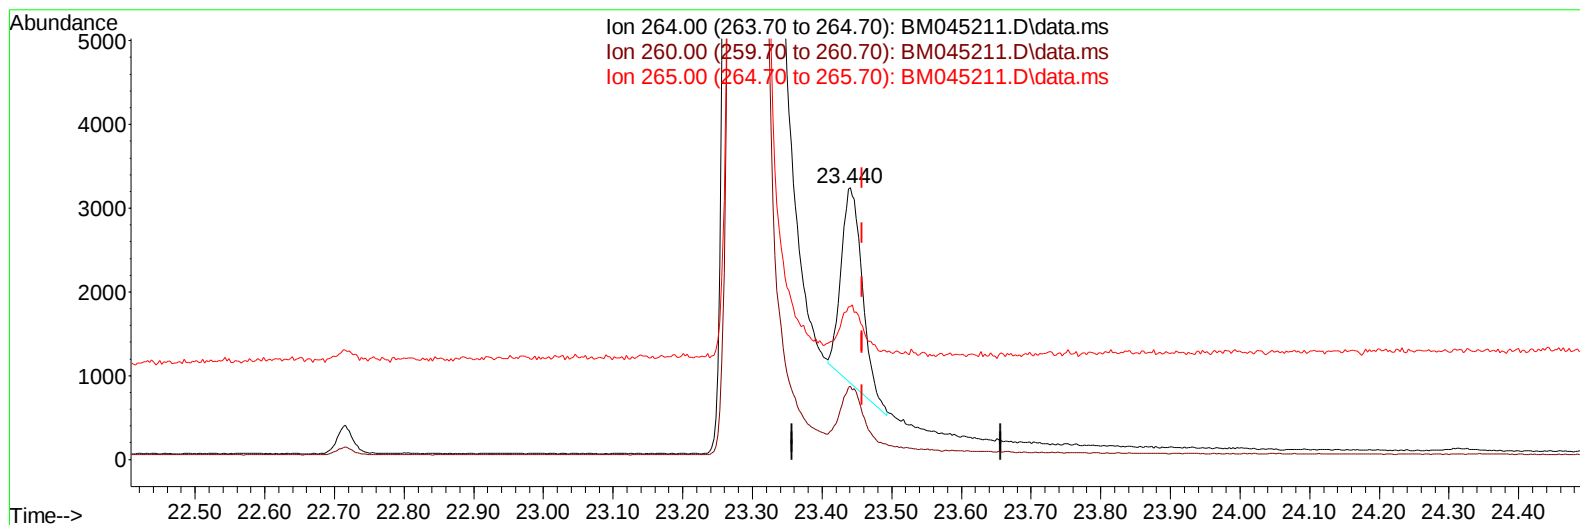

TIC: BM045211.D\data.ms

(23) Perylene-d12 (I)

23.440min (-0.017) 0.40 ng/ul m

response 4932

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	27.02
265.00	70.40	56.23#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
 Data File : BM045211.D
 Acq On : 13 Apr 2024 18:53
 Operator : MA/JU
 Sample : P2014-19
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0ME4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/17/2024

Quant Time: Apr 15 00:36:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 00:32:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.606	152	1603	0.400	ng/ul	0.00
4) Naphthalene-d8	10.374	136	4928	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.251	164	2683	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.013	188	5730m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.243	240	5007m	0.400	ng/ul	0.00
23) Perylene-d12	23.440	264	4932m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	7598	3.608	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.997	152	2261	0.339	ng/ul	0.00
18) Fluoranthene-d10	19.057	212	5314	0.420	ng/ul	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045211.D
Acq On : 13 Apr 2024 18:53
Operator : MA/JU
Sample : P2014-19
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0ME4

Manual IntegrationsAPPROVED

Quant Time: Apr 15 00:36:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/17/2024

