

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
 Data File : BM045233.D
 Acq On : 14 Apr 2024 08:40
 Operator : MA/JU
 Sample : P2036-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCSX3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/17/2024

Quant Time: Apr 15 00:39:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 15 00:32:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.606	152	1224	0.400	ng/ul	0.00
4) Naphthalene-d8	10.375	136	3644	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.252	164	1942	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.010	188	4193m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.245	240	3441m	0.400	ng/ul	0.00
23) Perylene-d12	23.434	264	3285m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.196	96	6009	3.737	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.008	152	1585	0.321	ng/ul	0.01
18) Fluoranthene-d10	19.053	212	3686	0.424	ng/ul	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.234	88	1420	0.921	ng/ul#	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041324\
Data File : BM045233.D
Acq On : 14 Apr 2024 08:40
Operator : MA/JU
Sample : P2036-06
Misc :
ALS Vial : 31 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
YCSX3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/16/2024
Supervised By :mohammad ahmed 04/17/2024


Quant Time: Apr 15 00:39:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 15 00:32:25 2024
Response via : Initial Calibration

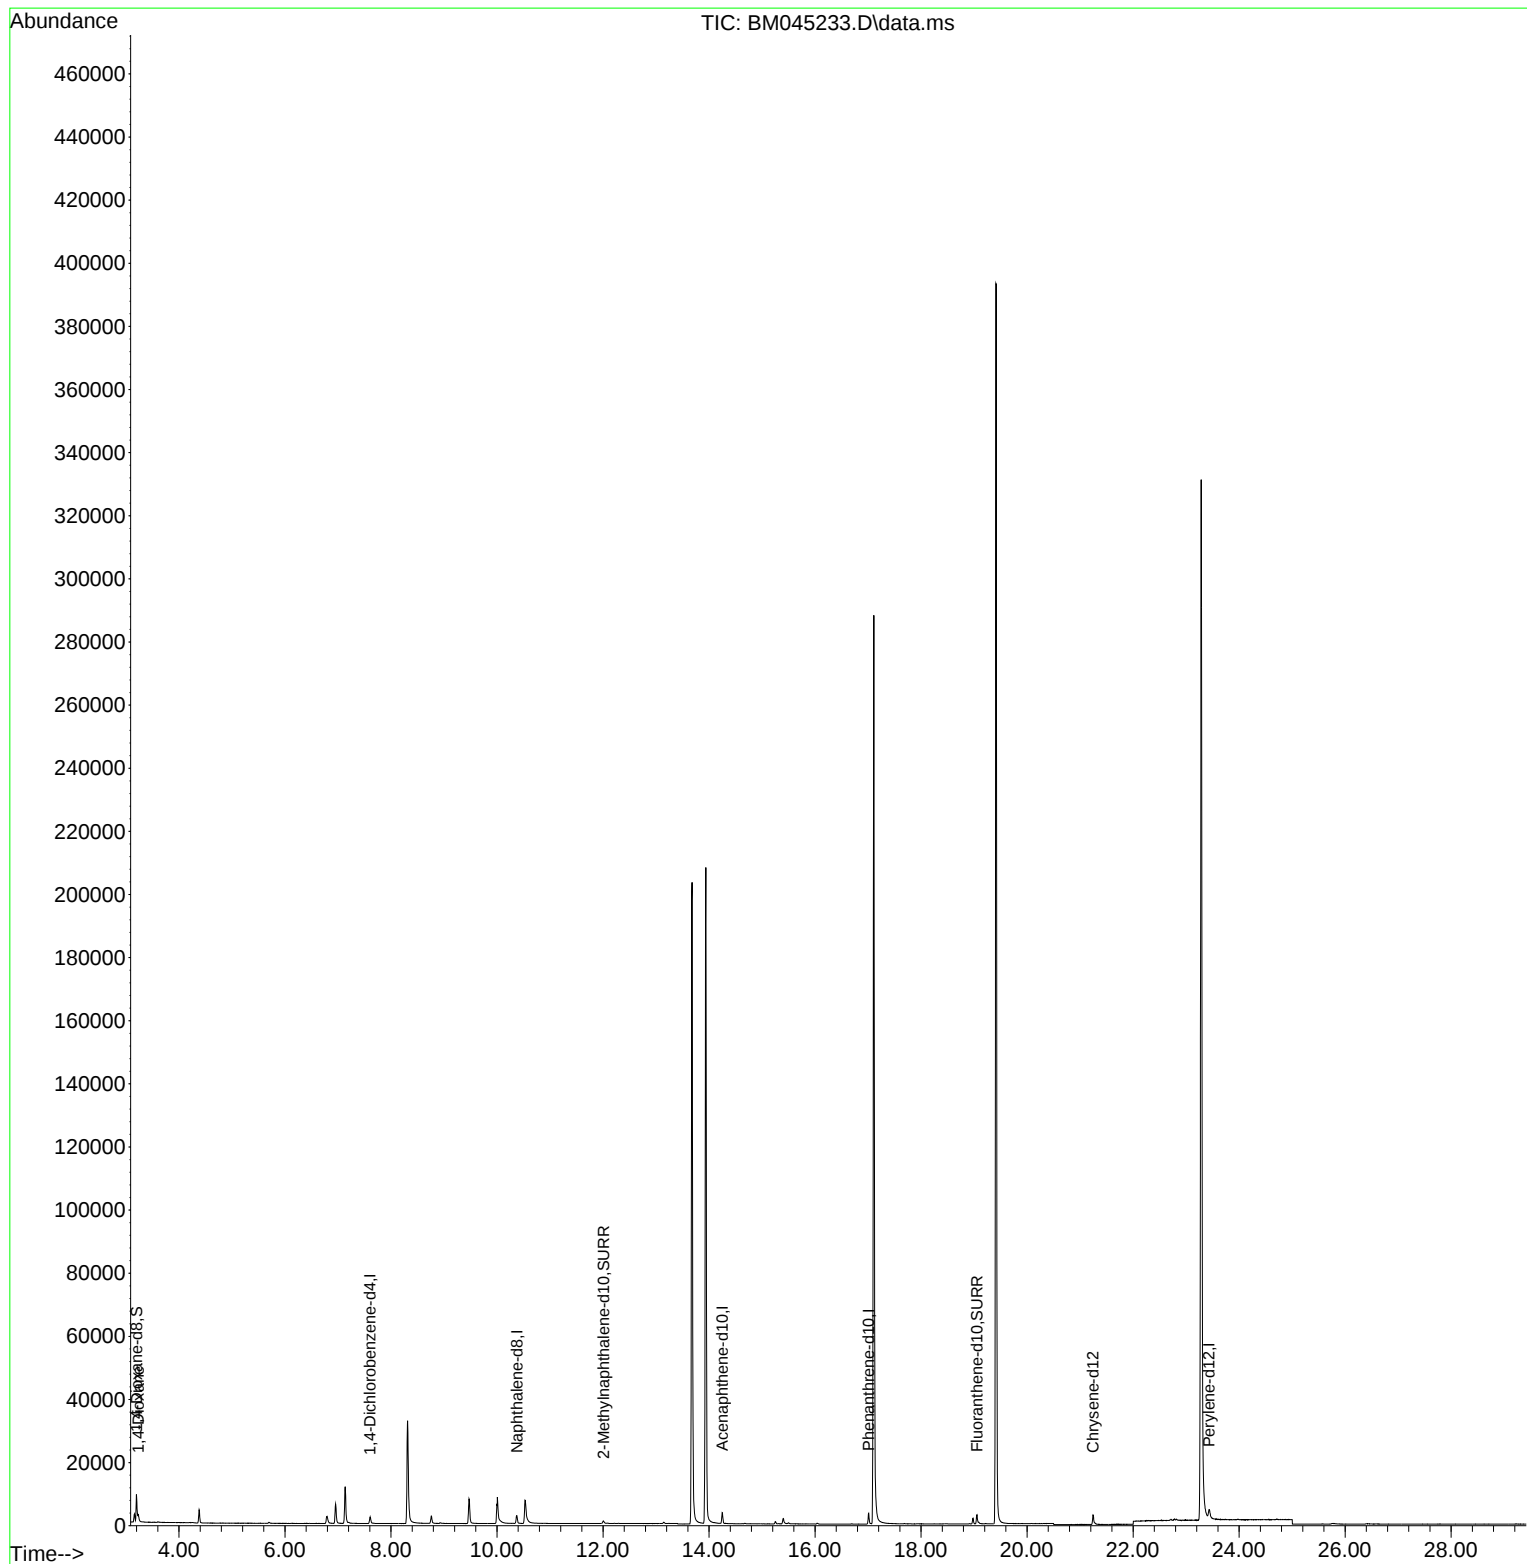

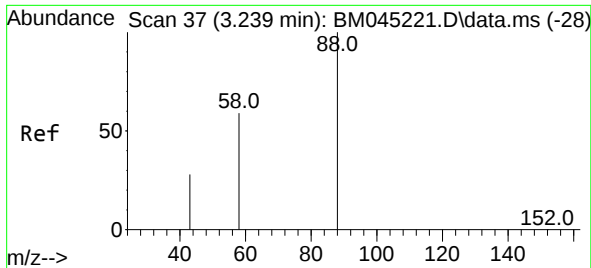

#2
 1,4-Dioxane
 Concen: 0.921 ng/ul
 RT: 3.234 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: BM045233.D
 Acq: 14 Apr 2024 08:40

Instrument :
 BNA_M
 ClientSampleId :
 YCSX3

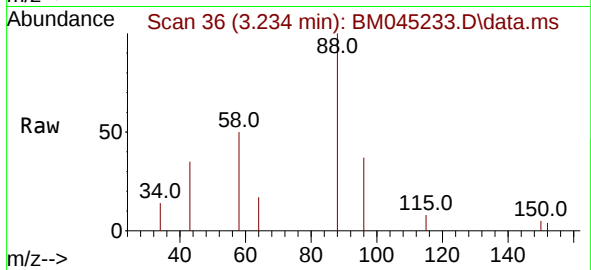

Tgt Ion: 88 Resp: 1420
 Ion Ratio Lower Upper
 88 100
 43 35.5 30.6 46.0
 58 50.3 32.6 48.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/16/2024
 Supervised By :mohammad ahmed 04/17/2024

