


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM041324\  
Data File : BM045204.D  
Acq On : 13 Apr 2024 14:40  
Operator : MA/JU  
Sample : DFTPP014  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
BNA\_M  
**ClientSampleId :**  
DFTPP014

Integration File: rteint.p

```
Method      : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Title       : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update  : Mon Apr 15 00:32:25 2024
```

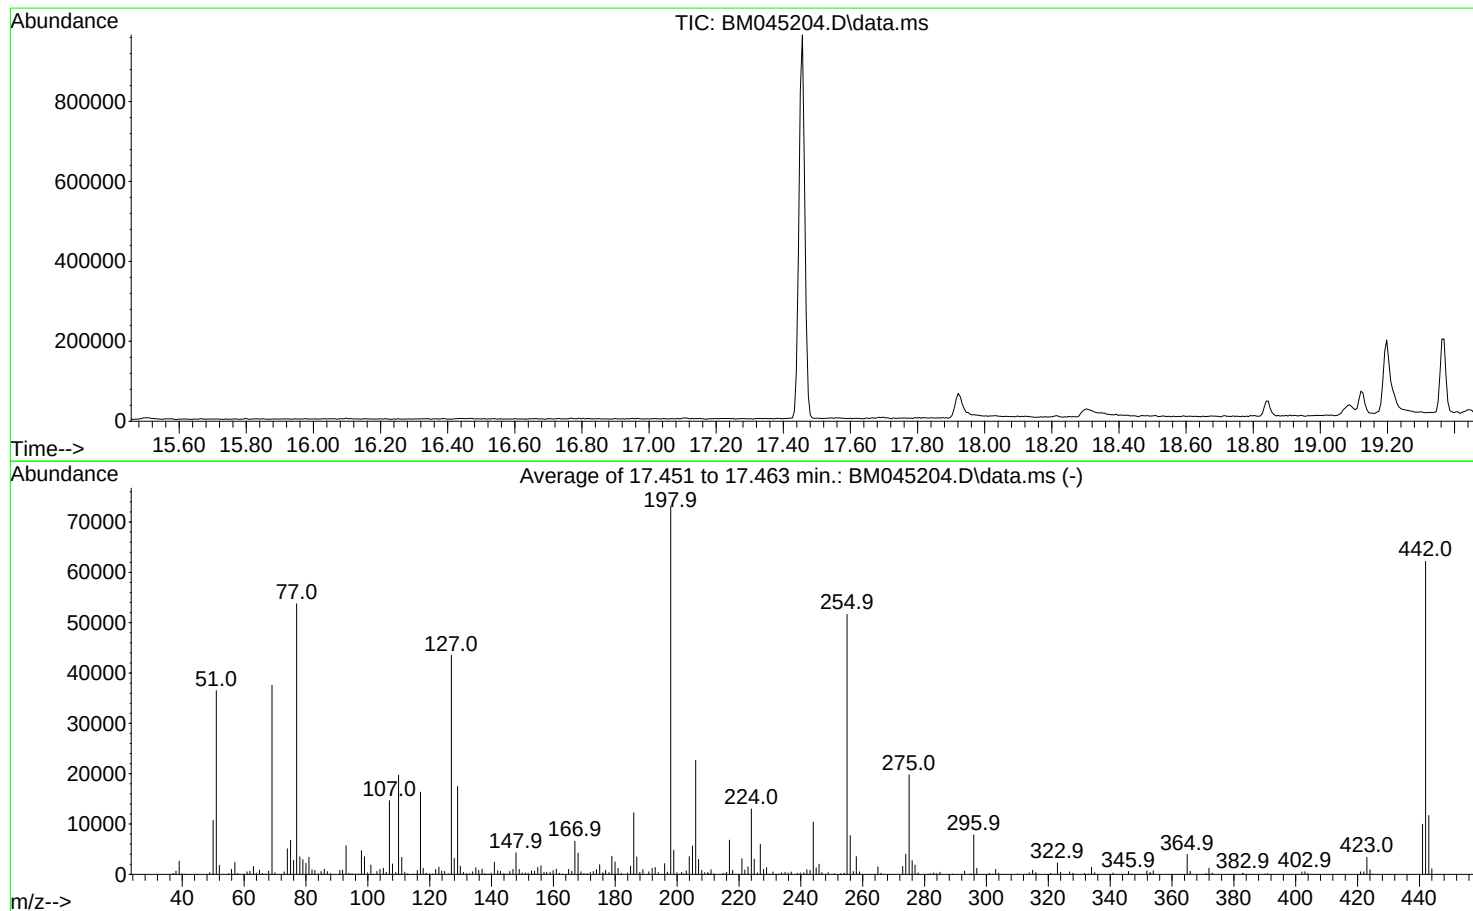

AutoFind: Scans 2442, 2443, 2444; Background Corrected with Scan 2436

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 50.0         | 36515      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 652        | PASS                |
| 69             | 198             | 0.00            | 100             | 51.4         | 37577      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.9          | 326        | PASS                |
| 127            | 198             | 10              | 80              | 59.5         | 43515      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.6          | 440        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 73091      | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 4796       | PASS                |
| 275            | 198             | 10              | 60              | 27.1         | 19805      | PASS                |
| 365            | 198             | 1               | 100             | 5.4          | 3943       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.6         | 9966       | PASS                |
| 442            | 198             | 50              | 100             | 85.1         | 62184      | PASS                |
| 443            | 442             | 15              | 24              | 18.8         | 11690      | PASS                |

| m/z    | Abundance |
|--------|-----------|
| 39.00  | 367.0     |
| 39.90  | 452.0     |
| 41.10  | 275.0     |
| 41.90  | 172.0     |
| 43.00  | 787.0     |
| 44.00  | 1196.0    |
| 44.90  | 348.0     |
| 48.90  | 195.0     |
| 53.10  | 151.0     |
| 55.00  | 341.0     |
| 57.00  | 150.0     |
| 59.90  | 184.0     |
| 69.20  | 308.0     |
| 73.00  | 563.0     |
| 84.00  | 180.0     |
| 96.00  | 184.0     |
| 135.00 | 192.0     |
| 146.90 | 405.0     |
| 192.90 | 242.0     |
| 206.90 | 656.0     |
| 208.00 | 179.0     |
| 281.00 | 227.0     |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP014

| m/z    | Abundance |
|--------|-----------|
| 37.10  | 345.0     |
| 38.00  | 540.0     |
| 39.00  | 3426.0    |
| 40.00  | 546.0     |
| 41.00  | 280.0     |
| 41.90  | 213.0     |
| 43.00  | 747.0     |
| 44.00  | 816.0     |
| 45.00  | 371.0     |
| 49.00  | 639.0     |
| 50.00  | 12567.0   |
| 51.00  | 43168.0   |
| 52.00  | 2241.0    |
| 52.90  | 243.0     |
| 55.00  | 496.0     |
| 56.00  | 984.0     |
| 57.00  | 3338.0    |
| 57.90  | 243.0     |
| 60.00  | 250.0     |
| 61.00  | 667.0     |
| 62.00  | 814.0     |
| 63.00  | 1768.0    |
| 64.00  | 242.0     |
| 65.00  | 939.0     |
| 65.90  | 213.0     |
| 67.00  | 187.0     |
| 68.00  | 723.0     |
| 69.00  | 43064.0   |
| 70.00  | 368.0     |
| 72.90  | 1110.0    |
| 74.00  | 5721.0    |
| 75.00  | 7371.0    |
| 76.00  | 3420.0    |
| 77.00  | 59816.0   |
| 78.00  | 3989.0    |
| 79.00  | 3568.0    |
| 80.00  | 2324.0    |
| 80.90  | 3898.0    |
| 82.00  | 1211.0    |
| 82.90  | 763.0     |
| 83.80  | 403.0     |
| 84.90  | 665.0     |
| 85.90  | 1128.0    |
| 86.90  | 720.0     |
| 87.90  | 294.0     |
| 90.90  | 743.0     |
| 91.80  | 811.0     |
| 92.90  | 5952.0    |
| 93.90  | 264.0     |
| 94.90  | 263.0     |
| 95.90  | 310.0     |
| 96.90  | 161.0     |
| 97.90  | 5441.0    |
| 98.90  | 3739.0    |
| 100.10 | 338.0     |
| 101.00 | 2091.0    |
| 103.00 | 680.0     |
| 103.90 | 1055.0    |
| 104.90 | 1339.0    |
| 105.90 | 393.0     |
| 107.00 | 16331.0   |
| 108.00 | 2524.0    |
| 109.10 | 413.0     |
| 109.90 | 20880.0   |
| 110.90 | 4108.0    |
| 112.00 | 407.0     |
| 112.90 | 206.0     |
| 116.00 | 821.0     |
| 117.00 | 17552.0   |
| 117.90 | 1491.0    |
| 118.90 | 254.0     |
| 120.00 | 214.0     |
| 122.00 | 1017.0    |
| 122.90 | 1387.0    |
| 123.90 | 614.0     |
| 124.90 | 702.0     |
| 125.90 | 159.0     |
| 127.00 | 46296.0   |
| 128.00 | 3361.0    |
| 129.00 | 18568.0   |
| 129.90 | 1664.0    |
| 130.90 | 476.0     |
| 131.90 | 168.0     |
| 133.90 | 459.0     |
| 134.90 | 1528.0    |
| 135.80 | 755.0     |
| 136.90 | 1178.0    |
| 137.70 | 245.0     |
| 139.90 | 229.0     |
| 140.90 | 2727.0    |
| 142.00 | 787.0     |
| 142.90 | 563.0     |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP014

|        |         |
|--------|---------|
| 143.90 | 218.0   |
| 145.90 | 644.0   |
| 147.00 | 1572.0  |
| 147.90 | 4233.0  |
| 148.90 | 1151.0  |
| 149.90 | 347.0   |
| 151.00 | 267.0   |
| 151.90 | 205.0   |
| 153.00 | 714.0   |
| 153.90 | 852.0   |
| 155.00 | 1477.0  |
| 156.00 | 1822.0  |
| 156.90 | 280.0   |
| 157.90 | 469.0   |
| 158.90 | 381.0   |
| 159.90 | 947.0   |
| 161.00 | 982.0   |
| 161.90 | 305.0   |
| 162.90 | 184.0   |
| 164.90 | 996.0   |
| 166.00 | 599.0   |
| 166.90 | 7801.0  |
| 167.90 | 4503.0  |
| 168.90 | 499.0   |
| 170.00 | 155.0   |
| 170.90 | 205.0   |
| 171.90 | 337.0   |
| 172.90 | 557.0   |
| 173.90 | 874.0   |
| 175.00 | 1856.0  |
| 175.90 | 284.0   |
| 176.90 | 912.0   |
| 177.90 | 347.0   |
| 178.90 | 3961.0  |
| 179.90 | 2402.0  |
| 180.90 | 1342.0  |
| 181.80 | 224.0   |
| 183.90 | 251.0   |
| 185.00 | 1584.0  |
| 186.00 | 12581.0 |
| 186.90 | 3581.0  |
| 188.00 | 466.0   |
| 188.90 | 885.0   |
| 190.80 | 532.0   |
| 192.00 | 1269.0  |
| 193.00 | 1638.0  |
| 193.90 | 231.0   |
| 195.90 | 1900.0  |
| 197.00 | 415.0   |
| 197.90 | 74584.0 |
| 198.90 | 5097.0  |
| 200.00 | 422.0   |
| 201.40 | 328.0   |
| 203.00 | 560.0   |
| 203.90 | 3220.0  |
| 204.90 | 5312.0  |
| 206.00 | 22448.0 |
| 207.00 | 3579.0  |
| 208.00 | 870.0   |
| 209.00 | 327.0   |
| 209.90 | 407.0   |
| 211.00 | 875.0   |
| 211.80 | 171.0   |
| 214.80 | 270.0   |
| 215.80 | 365.0   |
| 216.90 | 7038.0  |
| 218.00 | 1036.0  |
| 221.00 | 3070.0  |
| 221.90 | 885.0   |
| 222.90 | 1492.0  |
| 224.00 | 11827.0 |
| 225.00 | 2743.0  |
| 226.00 | 274.0   |
| 226.90 | 5690.0  |
| 227.90 | 828.0   |
| 228.90 | 1295.0  |
| 229.80 | 227.0   |
| 231.00 | 456.0   |
| 233.90 | 198.0   |
| 234.90 | 448.0   |
| 235.90 | 298.0   |
| 236.90 | 531.0   |
| 238.90 | 193.0   |
| 239.90 | 197.0   |
| 240.90 | 271.0   |
| 241.90 | 770.0   |
| 243.00 | 949.0   |
| 244.00 | 10286.0 |
| 245.00 | 1202.0  |
| 245.90 | 1823.0  |
| 246.80 | 332.0   |
| 248.90 | 408.0   |
| 253.80 | 231.0   |
| 255.00 | 49120.0 |
| 255.90 | 7493.0  |
| 257.00 | 633.0   |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP014

|        |         |
|--------|---------|
| 257.90 | 3939.0  |
| 259.00 | 371.0   |
| 264.90 | 1394.0  |
| 266.00 | 180.0   |
| 273.00 | 1484.0  |
| 273.90 | 3990.0  |
| 275.00 | 19264.0 |
| 276.00 | 2466.0  |
| 276.90 | 1636.0  |
| 277.90 | 349.0   |
| 280.90 | 229.0   |
| 282.90 | 283.0   |
| 285.00 | 374.0   |
| 292.90 | 666.0   |
| 295.90 | 7285.0  |
| 296.90 | 1075.0  |
| 300.90 | 222.0   |
| 303.00 | 751.0   |
| 303.90 | 151.0   |
| 313.90 | 290.0   |
| 315.10 | 725.0   |
| 315.80 | 307.0   |
| 320.90 | 234.0   |
| 323.00 | 2130.0  |
| 324.00 | 343.0   |
| 326.90 | 504.0   |
| 327.90 | 325.0   |
| 331.80 | 198.0   |
| 333.90 | 1198.0  |
| 335.00 | 386.0   |
| 341.00 | 204.0   |
| 345.80 | 636.0   |
| 351.90 | 441.0   |
| 352.90 | 630.0   |
| 354.00 | 742.0   |
| 364.90 | 3207.0  |
| 365.90 | 446.0   |
| 371.00 | 218.0   |
| 371.90 | 1101.0  |
| 372.90 | 152.0   |
| 382.80 | 241.0   |
| 390.00 | 163.0   |
| 390.90 | 204.0   |
| 402.00 | 354.0   |
| 402.90 | 547.0   |
| 403.90 | 254.0   |
| 420.80 | 394.0   |
| 422.00 | 424.0   |
| 423.00 | 3085.0  |
| 424.00 | 832.0   |
| 441.00 | 8014.0  |
| 442.00 | 50552.0 |
| 443.00 | 9964.0  |
| 444.00 | 762.0   |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP014

| m/z    | Abundance |
|--------|-----------|
| 37.00  | 247.0     |
| 38.00  | 865.0     |
| 39.00  | 3216.0    |
| 39.90  | 510.0     |
| 40.90  | 425.0     |
| 43.00  | 744.0     |
| 44.00  | 877.0     |
| 45.00  | 495.0     |
| 48.90  | 509.0     |
| 50.00  | 12319.0   |
| 51.00  | 43192.0   |
| 52.00  | 1953.0    |
| 55.00  | 469.0     |
| 55.90  | 1320.0    |
| 57.00  | 2529.0    |
| 58.00  | 322.0     |
| 60.10  | 228.0     |
| 60.90  | 530.0     |
| 61.90  | 552.0     |
| 63.00  | 1780.0    |
| 64.00  | 300.0     |
| 65.00  | 1058.0    |
| 66.00  | 193.0     |
| 67.90  | 900.0     |
| 69.00  | 44496.0   |
| 70.00  | 407.0     |
| 73.00  | 1071.0    |
| 74.00  | 6086.0    |
| 75.00  | 8257.0    |
| 76.00  | 3204.0    |
| 77.00  | 64176.0   |
| 78.00  | 4206.0    |
| 79.00  | 3476.0    |
| 80.00  | 2553.0    |
| 81.00  | 3605.0    |
| 81.90  | 843.0     |
| 82.90  | 1236.0    |
| 83.90  | 238.0     |
| 85.00  | 645.0     |
| 86.00  | 1343.0    |
| 86.80  | 467.0     |
| 87.80  | 163.0     |
| 90.90  | 984.0     |
| 91.90  | 1181.0    |
| 93.00  | 7086.0    |
| 93.90  | 306.0     |
| 94.90  | 153.0     |
| 95.90  | 290.0     |
| 98.00  | 5367.0    |
| 98.90  | 4308.0    |
| 99.90  | 339.0     |
| 101.00 | 2220.0    |
| 101.80 | 227.0     |
| 102.90 | 643.0     |
| 104.00 | 1069.0    |
| 105.00 | 1429.0    |
| 106.00 | 447.0     |
| 107.00 | 17496.0   |
| 108.00 | 2146.0    |
| 109.00 | 467.0     |
| 110.00 | 23328.0   |
| 111.00 | 3852.0    |
| 112.00 | 555.0     |
| 112.90 | 194.0     |
| 114.90 | 157.0     |
| 116.00 | 1001.0    |
| 117.00 | 19696.0   |
| 117.90 | 1352.0    |
| 118.90 | 169.0     |
| 119.90 | 206.0     |
| 121.00 | 208.0     |
| 121.90 | 1307.0    |
| 123.00 | 1997.0    |
| 123.90 | 853.0     |
| 124.80 | 726.0     |
| 126.00 | 255.0     |
| 127.00 | 51440.0   |
| 127.90 | 3927.0    |
| 129.00 | 21256.0   |
| 129.90 | 2156.0    |
| 130.90 | 262.0     |
| 131.90 | 280.0     |
| 132.90 | 246.0     |
| 133.90 | 672.0     |
| 134.90 | 1929.0    |
| 135.90 | 903.0     |
| 136.90 | 1228.0    |
| 137.90 | 261.0     |
| 138.90 | 174.0     |
| 139.90 | 335.0     |
| 140.90 | 2702.0    |
| 142.00 | 928.0     |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP014

|        |         |
|--------|---------|
| 142.90 | 831.0   |
| 143.90 | 178.0   |
| 146.00 | 584.0   |
| 146.90 | 1544.0  |
| 147.90 | 5466.0  |
| 149.00 | 1219.0  |
| 149.90 | 378.0   |
| 150.90 | 380.0   |
| 151.90 | 258.0   |
| 152.90 | 859.0   |
| 153.90 | 753.0   |
| 154.90 | 1678.0  |
| 155.90 | 2152.0  |
| 157.00 | 496.0   |
| 157.80 | 572.0   |
| 158.90 | 453.0   |
| 159.90 | 843.0   |
| 160.90 | 1408.0  |
| 162.00 | 361.0   |
| 164.90 | 1205.0  |
| 165.90 | 809.0   |
| 167.00 | 7365.0  |
| 168.00 | 5306.0  |
| 168.90 | 655.0   |
| 169.80 | 182.0   |
| 170.80 | 319.0   |
| 171.90 | 673.0   |
| 172.90 | 648.0   |
| 173.90 | 1081.0  |
| 175.00 | 2219.0  |
| 175.80 | 607.0   |
| 176.80 | 941.0   |
| 177.90 | 352.0   |
| 178.90 | 4282.0  |
| 179.90 | 3238.0  |
| 180.90 | 1573.0  |
| 181.90 | 204.0   |
| 184.00 | 388.0   |
| 185.00 | 2111.0  |
| 186.00 | 15115.0 |
| 187.00 | 3826.0  |
| 187.90 | 446.0   |
| 188.90 | 1350.0  |
| 190.90 | 589.0   |
| 191.90 | 1331.0  |
| 193.00 | 1901.0  |
| 193.90 | 442.0   |
| 195.90 | 2831.0  |
| 196.80 | 572.0   |
| 197.90 | 86936.0 |
| 198.90 | 5658.0  |
| 199.90 | 430.0   |
| 200.80 | 152.0   |
| 201.40 | 415.0   |
| 202.00 | 259.0   |
| 202.90 | 970.0   |
| 203.90 | 4446.0  |
| 205.00 | 7116.0  |
| 206.00 | 27944.0 |
| 207.00 | 4271.0  |
| 207.90 | 1087.0  |
| 208.90 | 467.0   |
| 209.80 | 395.0   |
| 210.20 | 549.0   |
| 210.90 | 1036.0  |
| 211.90 | 197.0   |
| 214.90 | 269.0   |
| 216.00 | 817.0   |
| 216.90 | 7669.0  |
| 217.90 | 876.0   |
| 221.00 | 3450.0  |
| 221.90 | 976.0   |
| 222.90 | 1770.0  |
| 224.00 | 15897.0 |
| 224.90 | 3767.0  |
| 225.90 | 358.0   |
| 226.90 | 7224.0  |
| 227.90 | 1213.0  |
| 228.90 | 1641.0  |
| 231.10 | 518.0   |
| 232.80 | 160.0   |
| 233.70 | 444.0   |
| 234.90 | 489.0   |
| 235.90 | 397.0   |
| 236.90 | 594.0   |
| 238.90 | 279.0   |
| 239.90 | 382.0   |
| 241.00 | 427.0   |
| 242.00 | 1123.0  |
| 243.00 | 837.0   |
| 244.00 | 12025.0 |
| 244.90 | 1649.0  |
| 245.90 | 2886.0  |
| 246.80 | 488.0   |
| 248.80 | 321.0   |
| 251.00 | 163.0   |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP014

|        |         |
|--------|---------|
| 252.80 | 206.0   |
| 254.00 | 385.0   |
| 255.00 | 62456.0 |
| 255.90 | 9235.0  |
| 256.90 | 777.0   |
| 258.00 | 4114.0  |
| 258.90 | 710.0   |
| 264.90 | 1727.0  |
| 265.90 | 265.0   |
| 272.90 | 1895.0  |
| 273.90 | 4163.0  |
| 275.00 | 23008.0 |
| 276.00 | 3286.0  |
| 276.90 | 2301.0  |
| 277.90 | 414.0   |
| 281.00 | 268.0   |
| 282.00 | 162.0   |
| 282.90 | 306.0   |
| 283.80 | 208.0   |
| 285.00 | 594.0   |
| 289.00 | 190.0   |
| 292.90 | 701.0   |
| 294.90 | 222.0   |
| 295.90 | 9774.0  |
| 296.90 | 1395.0  |
| 300.90 | 151.0   |
| 302.00 | 184.0   |
| 303.00 | 1363.0  |
| 303.90 | 360.0   |
| 309.90 | 176.0   |
| 313.80 | 378.0   |
| 314.90 | 998.0   |
| 316.00 | 615.0   |
| 320.80 | 305.0   |
| 322.00 | 161.0   |
| 323.00 | 2563.0  |
| 323.90 | 469.0   |
| 326.90 | 576.0   |
| 327.90 | 206.0   |
| 331.70 | 353.0   |
| 333.00 | 246.0   |
| 334.00 | 1753.0  |
| 335.10 | 359.0   |
| 340.90 | 462.0   |
| 345.90 | 671.0   |
| 346.90 | 172.0   |
| 351.80 | 1003.0  |
| 352.90 | 531.0   |
| 353.90 | 936.0   |
| 364.90 | 4815.0  |
| 365.90 | 639.0   |
| 371.10 | 179.0   |
| 372.00 | 1347.0  |
| 372.90 | 372.0   |
| 383.00 | 394.0   |
| 390.90 | 157.0   |
| 402.00 | 665.0   |
| 403.00 | 619.0   |
| 403.90 | 160.0   |
| 420.90 | 530.0   |
| 422.00 | 578.0   |
| 423.00 | 3871.0  |
| 424.00 | 1055.0  |
| 441.00 | 12336.0 |
| 442.00 | 72928.0 |
| 443.00 | 13425.0 |
| 444.00 | 1348.0  |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP014



| m/z    | Abundance |
|--------|-----------|
| 38.00  | 563.0     |
| 39.00  | 2276.0    |
| 40.00  | 581.0     |
| 41.00  | 298.0     |
| 41.90  | 150.0     |
| 43.00  | 580.0     |
| 44.00  | 976.0     |
| 45.00  | 292.0     |
| 49.00  | 451.0     |
| 50.00  | 7294.0    |
| 51.00  | 23184.0   |
| 52.10  | 1300.0    |
| 52.90  | 153.0     |
| 55.00  | 515.0     |
| 55.90  | 683.0     |
| 57.00  | 1630.0    |
| 60.00  | 222.0     |
| 60.90  | 326.0     |
| 61.80  | 430.0     |
| 63.00  | 1086.0    |
| 63.90  | 242.0     |
| 65.00  | 457.0     |
| 65.80  | 171.0     |
| 68.00  | 334.0     |
| 69.00  | 26096.0   |
| 69.90  | 204.0     |
| 73.00  | 1081.0    |
| 74.00  | 3485.0    |
| 75.00  | 4620.0    |
| 76.00  | 1844.0    |
| 77.00  | 37288.0   |
| 78.00  | 2333.0    |
| 78.90  | 1752.0    |
| 80.00  | 1700.0    |
| 81.00  | 2687.0    |
| 82.00  | 671.0     |
| 83.00  | 431.0     |
| 83.90  | 350.0     |
| 84.80  | 415.0     |
| 85.90  | 686.0     |
| 87.00  | 444.0     |
| 91.00  | 601.0     |
| 91.90  | 444.0     |
| 92.90  | 3991.0    |
| 94.00  | 188.0     |
| 96.00  | 246.0     |
| 97.90  | 3330.0    |
| 99.00  | 2448.0    |
| 99.90  | 287.0     |
| 100.90 | 1210.0    |
| 102.90 | 411.0     |
| 103.90 | 868.0     |
| 105.10 | 830.0     |
| 105.90 | 380.0     |
| 107.00 | 10145.0   |
| 107.90 | 1565.0    |
| 109.00 | 300.0     |
| 110.00 | 14928.0   |
| 111.00 | 2120.0    |
| 111.90 | 396.0     |
| 116.00 | 498.0     |
| 117.00 | 11818.0   |
| 117.90 | 756.0     |
| 118.90 | 301.0     |
| 122.00 | 643.0     |
| 123.00 | 983.0     |
| 123.90 | 593.0     |
| 124.90 | 397.0     |
| 127.00 | 32808.0   |
| 127.90 | 2333.0    |
| 128.90 | 12591.0   |
| 129.90 | 1186.0    |
| 130.90 | 365.0     |
| 132.90 | 190.0     |
| 133.90 | 371.0     |
| 134.90 | 1133.0    |
| 135.90 | 661.0     |
| 137.00 | 860.0     |
| 139.90 | 220.0     |
| 140.90 | 1784.0    |
| 141.90 | 533.0     |
| 142.90 | 452.0     |
| 144.00 | 160.0     |
| 145.00 | 169.0     |
| 145.80 | 492.0     |
| 147.00 | 1067.0    |
| 147.90 | 3169.0    |
| 149.00 | 636.0     |
| 149.90 | 156.0     |
| 150.90 | 198.0     |
| 151.70 | 262.0     |
| 152.80 | 513.0     |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP014

|        |         |
|--------|---------|
| 154.00 | 334.0   |
| 155.00 | 937.0   |
| 156.00 | 1214.0  |
| 156.90 | 391.0   |
| 157.90 | 334.0   |
| 158.90 | 398.0   |
| 160.00 | 510.0   |
| 161.00 | 748.0   |
| 161.70 | 184.0   |
| 164.90 | 728.0   |
| 165.90 | 553.0   |
| 166.90 | 4590.0  |
| 167.90 | 2967.0  |
| 169.00 | 352.0   |
| 169.90 | 187.0   |
| 171.90 | 181.0   |
| 172.90 | 543.0   |
| 173.90 | 889.0   |
| 174.90 | 1708.0  |
| 176.10 | 479.0   |
| 176.90 | 530.0   |
| 178.00 | 338.0   |
| 178.90 | 2580.0  |
| 179.90 | 1763.0  |
| 180.90 | 765.0   |
| 182.00 | 239.0   |
| 183.90 | 233.0   |
| 184.90 | 1265.0  |
| 185.90 | 8998.0  |
| 186.90 | 2968.0  |
| 187.90 | 363.0   |
| 188.90 | 602.0   |
| 190.80 | 408.0   |
| 191.90 | 1055.0  |
| 192.90 | 1293.0  |
| 193.90 | 340.0   |
| 196.00 | 1666.0  |
| 196.80 | 334.0   |
| 197.90 | 57752.0 |
| 198.90 | 3632.0  |
| 199.90 | 167.0   |
| 201.50 | 390.0   |
| 202.90 | 573.0   |
| 203.90 | 2922.0  |
| 204.90 | 4439.0  |
| 206.00 | 17496.0 |
| 207.00 | 3080.0  |
| 208.00 | 969.0   |
| 209.00 | 301.0   |
| 209.80 | 288.0   |
| 211.00 | 857.0   |
| 214.80 | 165.0   |
| 216.00 | 404.0   |
| 216.90 | 5689.0  |
| 217.90 | 599.0   |
| 220.90 | 2858.0  |
| 221.90 | 702.0   |
| 222.90 | 1181.0  |
| 224.00 | 11302.0 |
| 224.90 | 2530.0  |
| 226.00 | 258.0   |
| 226.90 | 5051.0  |
| 228.00 | 808.0   |
| 228.90 | 1120.0  |
| 230.90 | 499.0   |
| 233.80 | 302.0   |
| 234.90 | 292.0   |
| 235.80 | 161.0   |
| 237.00 | 322.0   |
| 238.70 | 151.0   |
| 239.80 | 273.0   |
| 240.90 | 237.0   |
| 241.90 | 838.0   |
| 243.00 | 700.0   |
| 244.00 | 8850.0  |
| 245.00 | 1082.0  |
| 245.90 | 1412.0  |
| 246.80 | 259.0   |
| 248.90 | 368.0   |
| 250.80 | 205.0   |
| 252.90 | 308.0   |
| 254.00 | 328.0   |
| 254.90 | 43440.0 |
| 256.00 | 6337.0  |
| 256.90 | 339.0   |
| 257.90 | 2538.0  |
| 258.90 | 441.0   |
| 264.90 | 1318.0  |
| 265.80 | 263.0   |
| 273.00 | 1409.0  |
| 273.90 | 3849.0  |
| 275.00 | 17144.0 |
| 276.00 | 2442.0  |
| 276.90 | 1572.0  |
| 277.90 | 185.0   |
| 280.90 | 241.0   |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP014

|        |         |
|--------|---------|
| 281.90 | 227.0   |
| 283.00 | 295.0   |
| 283.90 | 155.0   |
| 284.90 | 251.0   |
| 293.00 | 505.0   |
| 295.00 | 150.0   |
| 295.90 | 6502.0  |
| 296.90 | 1188.0  |
| 300.90 | 184.0   |
| 303.00 | 862.0   |
| 303.90 | 221.0   |
| 312.90 | 150.0   |
| 313.80 | 286.0   |
| 314.90 | 789.0   |
| 315.90 | 447.0   |
| 320.80 | 166.0   |
| 322.90 | 2095.0  |
| 323.90 | 438.0   |
| 326.80 | 312.0   |
| 328.00 | 162.0   |
| 333.90 | 1290.0  |
| 334.90 | 263.0   |
| 341.00 | 226.0   |
| 346.00 | 421.0   |
| 351.90 | 695.0   |
| 353.10 | 462.0   |
| 354.00 | 556.0   |
| 364.90 | 3808.0  |
| 365.90 | 737.0   |
| 370.80 | 170.0   |
| 372.00 | 1276.0  |
| 373.00 | 282.0   |
| 382.90 | 337.0   |
| 402.00 | 399.0   |
| 403.00 | 440.0   |
| 403.90 | 192.0   |
| 421.00 | 600.0   |
| 422.00 | 491.0   |
| 423.00 | 3169.0  |
| 424.10 | 789.0   |
| 424.90 | 159.0   |
| 441.00 | 9548.0  |
| 442.00 | 63072.0 |
| 443.00 | 11682.0 |
| 444.00 | 1207.0  |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP014