

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041415\
 Data File : BM000962.D
 Acq On : 13 Apr 2015 23:09
 Operator : TP/IZ
 Sample : G1858-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P001-SD008-0006-01

Quant Time: Apr 14 18:50:03 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 14 08:28:33 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	147273	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	607343	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	341585	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	746438	20.00	ng/ul	0.00
75) Chrysene-d12	21.20	240	790449	20.00	ng/ul	0.00
83) Perylene-d12	23.37	264	760403	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	6.78	99	174107	15.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	118810	17.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	134535	14.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	162518	18.84	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	65841	16.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	67499	15.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	150699	17.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	188590	18.12	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	627141	28.04	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	662126	20.46	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	53750	13.71	ng/ul	0.00
57) Fluorene-d10	15.26	176	498922	21.97	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	49031	12.29	ng/ul	0.00
70) Anthracene-d10	17.10	188	752805	22.08	ng/ul	0.00
76) Pyrene-d10	19.40	212	759378	21.28	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.24	264	625927	18.82	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Phenol	6.81	94	17680	1.47	ng/ul	95
44) Dimethylphthalate	13.72	163	147396	5.75	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041415\
Data File : BM000962.D
Acq On : 13 Apr 2015 23:09
Operator : TP/IZ
Sample : G1858-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P001-SD008-0006-01

Quant Time: Apr 14 18:50:03 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041415.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 14 08:28:33 2015
Response via : Initial Calibration

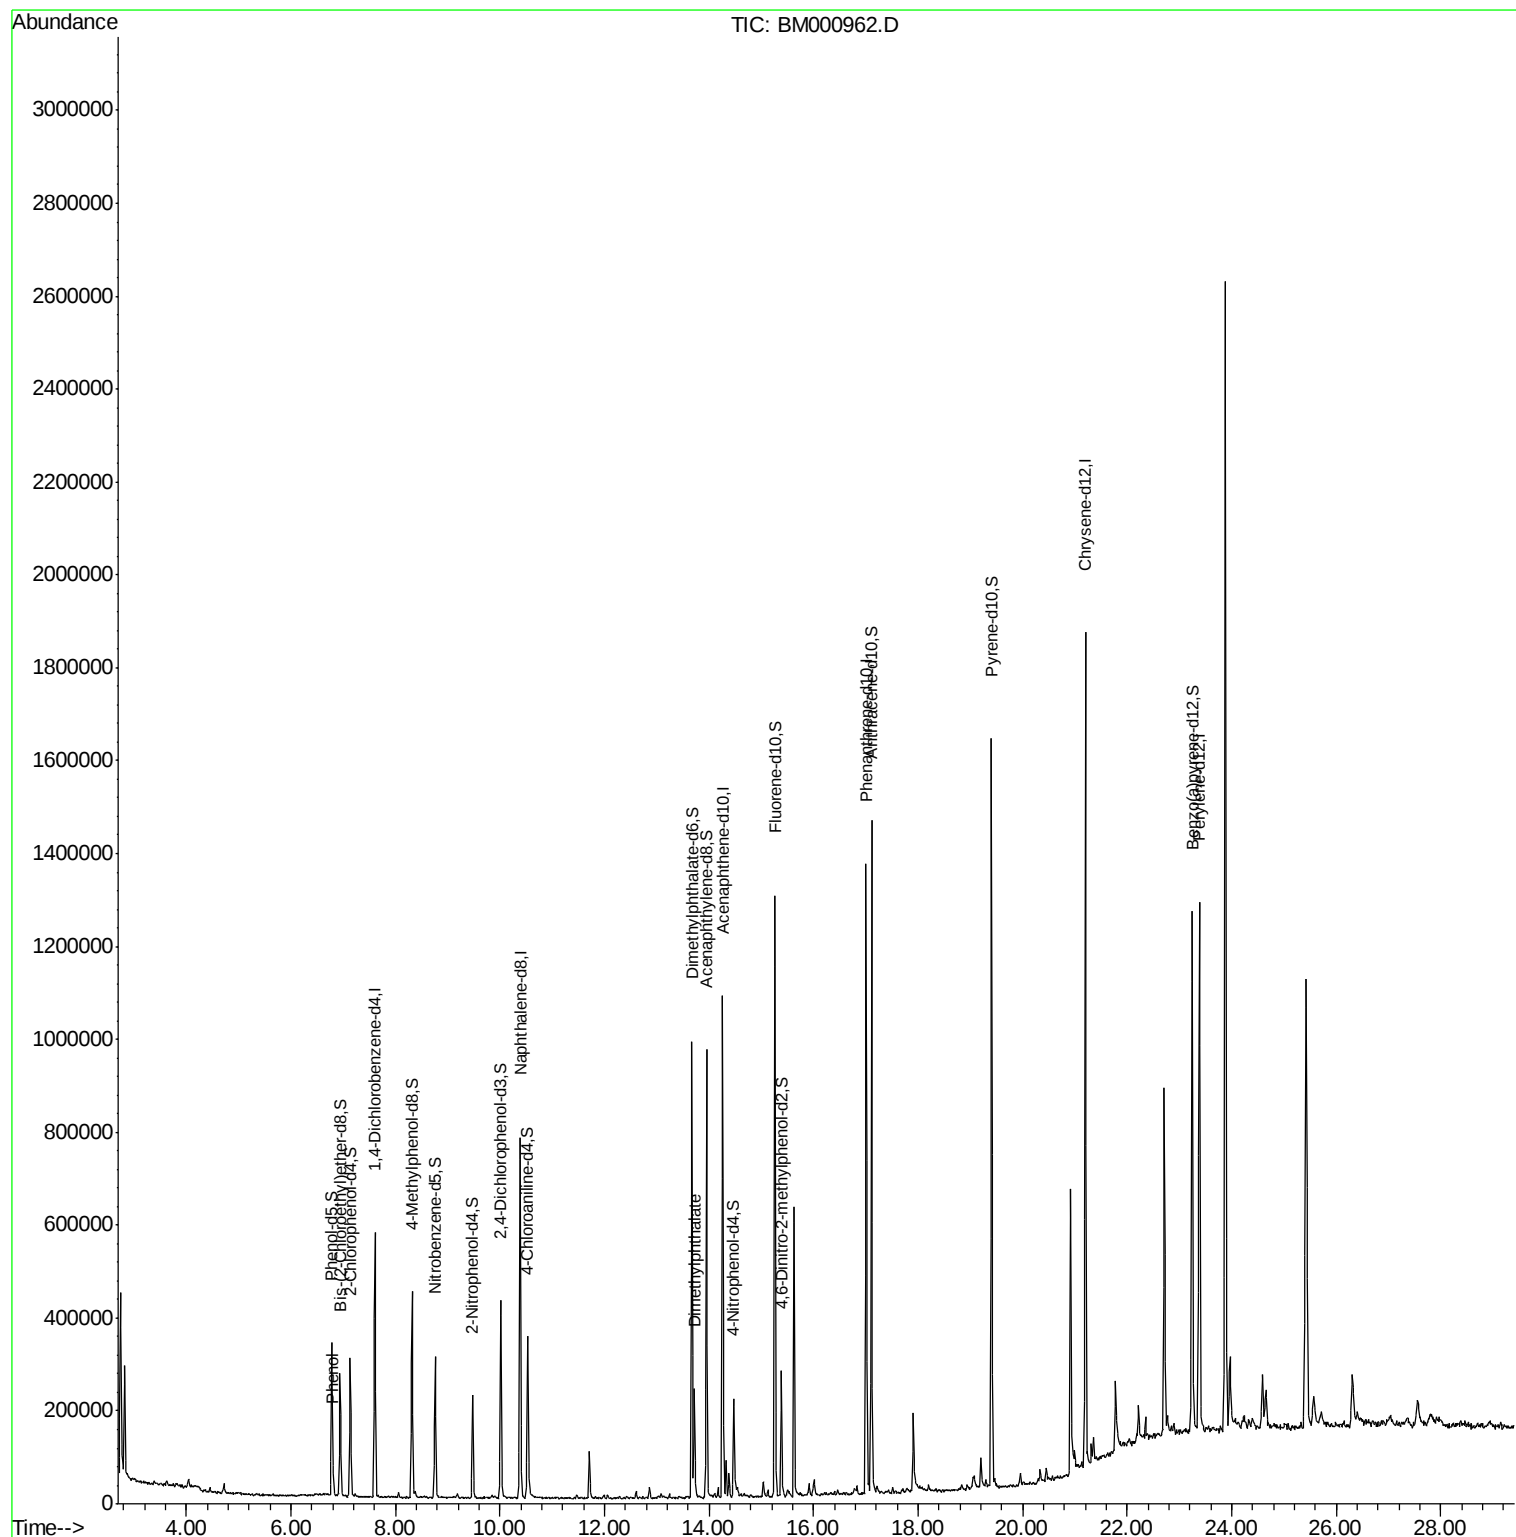

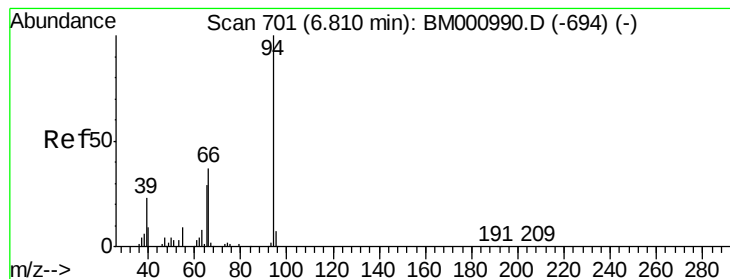

#6

Phenol

Concen: 1.47 ng/ul

RT: 6.81 min Scan# 701

Delta R.T. 0.00 min

Lab File: BM000962.D

Acq: 13 Apr 2015 23:09

Instrument :

BNA_M

ClientSampleId :

P001-SD008-0006-01


Tgt Ion: 94 Resp: 17680

Ion Ratio Lower Upper

94 100

65 26.0 23.5 35.3




66 40.6 30.6 45.8

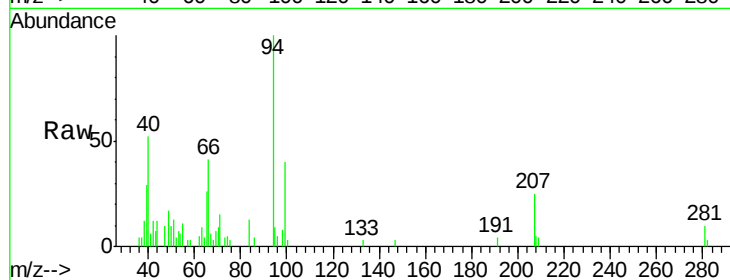

Abundance Ion 94.00 (93.70 to 94.70): BM000990.D (-694) (-)

Ion 65.00 (64.70 to 65.70): BM000990.D (-694) (-)

Ion 66.00 (65.70 to 66.70): BM000990.D (-694) (-)

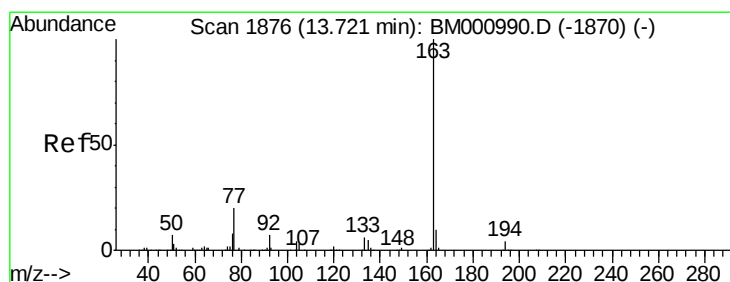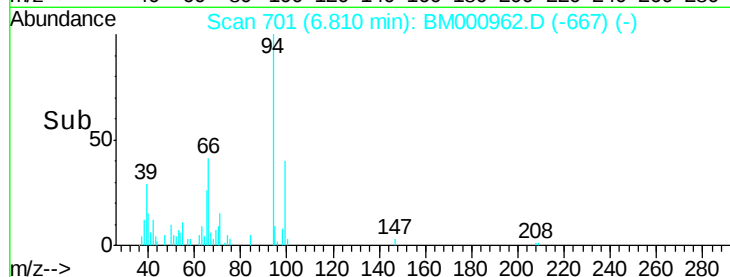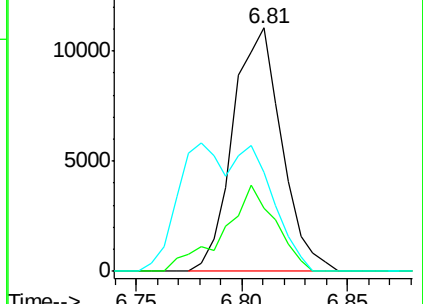

#44

Dimethylphthalate

Concen: 5.75 ng/ul

RT: 13.72 min Scan# 1876

Delta R.T. 0.00 min

Lab File: BM000962.D

Acq: 13 Apr 2015 23:09


Tgt Ion: 163 Resp: 147396

Ion Ratio Lower Upper

163 100

194 3.6 3.3 4.9

164 9.5 8.6 12.8

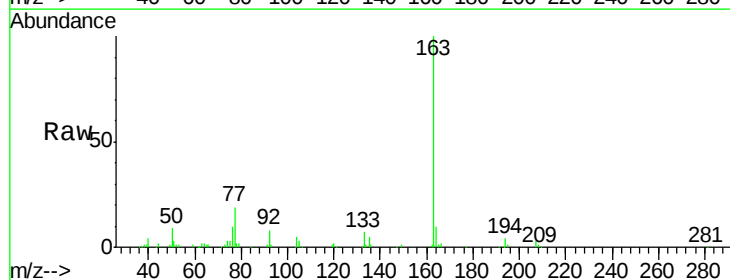

Abundance Ion 163.00 (162.70 to 163.70): BM000990.D (-1870) (-)

Ion 194.00 (193.70 to 194.70): BM000990.D (-1870) (-)

Ion 164.00 (163.70 to 164.70): BM000990.D (-1870) (-)

