

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041415\
 Data File : BM000988.D
 Acq On : 14 Apr 2015 17:50
 Operator : TP/IZ
 Sample : G1858-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P001-SS016-0006-01

Quant Time: Apr 15 17:11:40 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 15 06:02:42 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	389603	20.00	ng/ul	0.00
18) Naphthalene-d8	10.38	136	1620054	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	894295	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	1930718	20.00	ng/ul	0.00
75) Chrysene-d12	21.20	240	2018701	20.00	ng/ul	-0.01
83) Perylene-d12	23.38	264	1912071	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	6.78	99	482753	16.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	323666	17.70	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	375805	15.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	337349	14.78	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	206711	19.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.47	143	222268	19.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.01	165	423508	18.27	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	575602	20.73	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	1573818	26.88	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1967265	23.21	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	211204	20.57	ng/ul	0.00
57) Fluorene-d10	15.25	176	1418808	23.87	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.38	200	162683	15.77	ng/ul	0.00
70) Anthracene-d10	17.10	188	2143698	24.30	ng/ul	0.00
76) Pyrene-d10	19.40	212	2426176	26.62	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.24	264	2124630	25.40	ng/ul	0.00

Target Compounds


					Qvalue
6) Phenol	6.80	94	37745	1.18 ng/ul	97
44) Dimethylphthalate	13.72	163	477948	7.13 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041415\
Data File : BM000988.D
Acq On : 14 Apr 2015 17:50
Operator : TP/IZ
Sample : G1858-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P001-SS016-0006-01

Quant Time: Apr 15 17:11:40 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041415.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 15 06:02:42 2015
Response via : Initial Calibration

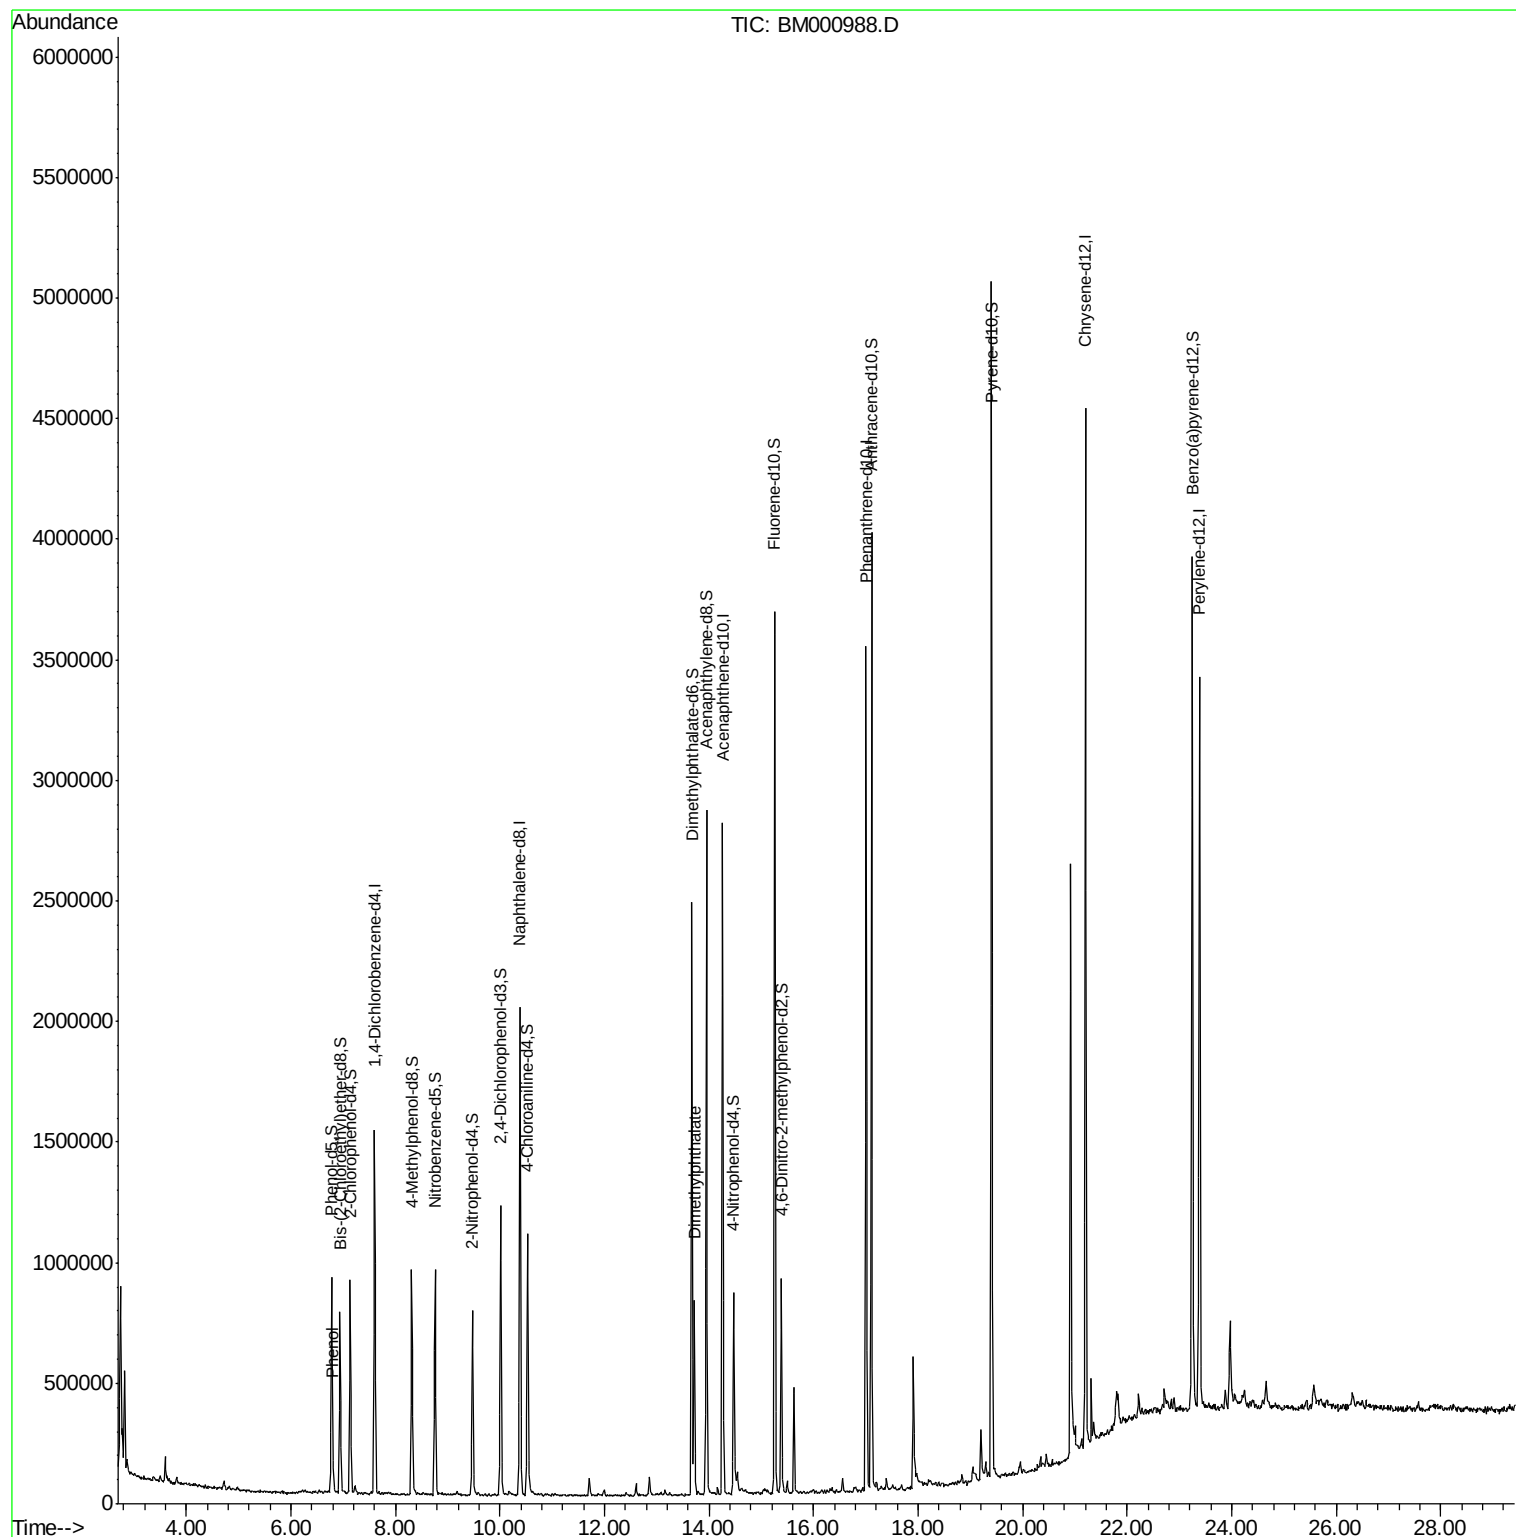

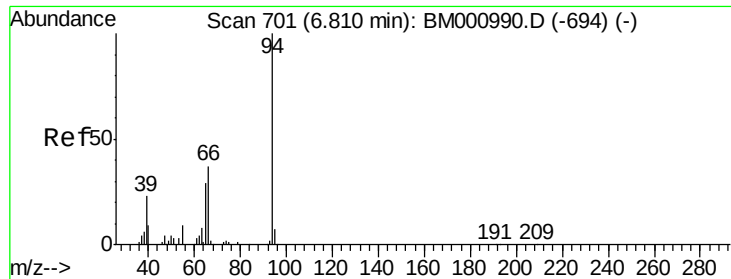

#6

Phenol

Concen: 1.18 ng/ul

RT: 6.80 min Scan# 700

Delta R.T. -0.01 min

Lab File: BM000988.D

Acq: 14 Apr 2015 17:50

Instrument :

BNA_M

ClientSampleId :

P001-SS016-0006-01


Tgt Ion: 94 Resp: 37745

Ion Ratio Lower Upper

94 100

65 29.9 23.5 35.3




66 41.5 30.6 45.8

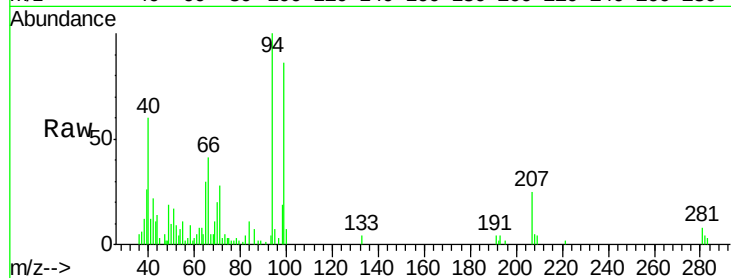

Abundance Ion 94.00 (93.70 to 94.70): BM000990.D (-694) (-)

Ion 65.00 (64.70 to 65.70): BM000990.D (-694) (-)

Ion 66.00 (65.70 to 66.70): BM000990.D (-694) (-)

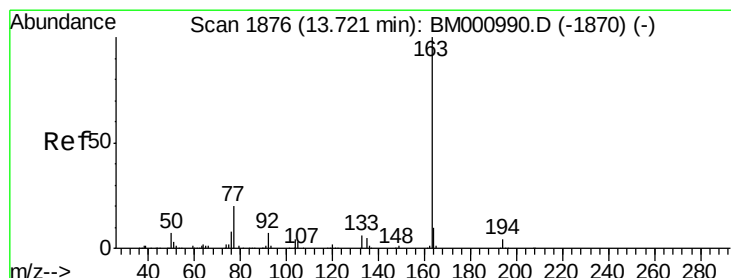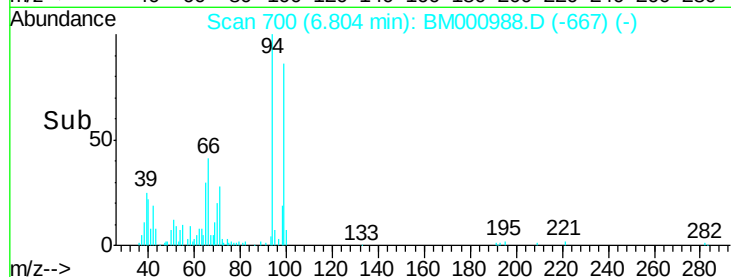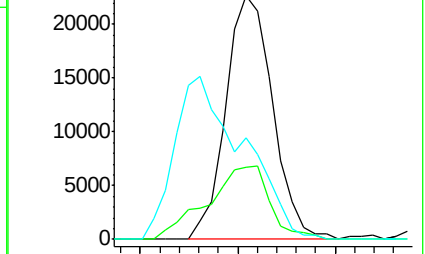

#44

Dimethylphthalate

Concen: 7.13 ng/ul

RT: 13.72 min Scan# 1875

Delta R.T. -0.01 min

Lab File: BM000988.D

Acq: 14 Apr 2015 17:50


Tgt Ion: 163 Resp: 477948

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 10.5 8.6 12.8

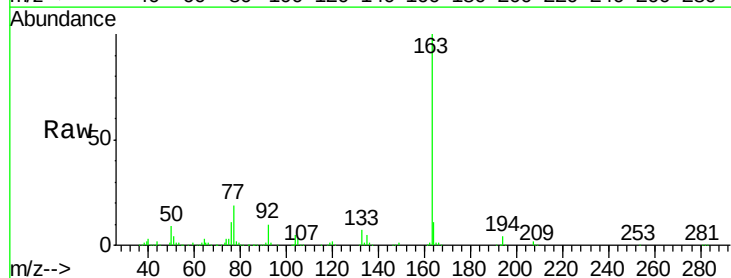

Abundance Ion 163.00 (162.70 to 163.70): BM000990.D (-1870) (-)

Ion 194.00 (193.70 to 194.70): BM000990.D (-1870) (-)

Ion 164.00 (163.70 to 164.70): BM000990.D (-1870) (-)

