

Data Path : Z:\HPCHEM1\BNA_M\Data\BM041415\
 Data File : BM000982.D
 Acq On : 14 Apr 2015 13:58
 Operator : TP/IZ
 Sample : PB82670BL
 Misc : SBLK43
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041415.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.728	3	7	17	rVB	328165	637378	6.82%	0.625%
2	2.816	18	22	28	rVB	118992	181020	1.94%	0.177%
3	3.528	141	143	145	rBV3	9030	9398	0.10%	0.009%
4	3.628	156	160	165	rVV	83679	115993	1.24%	0.114%
5	4.004	223	224	227	rBV3	11986	11668	0.12%	0.011%
6	4.269	264	269	270	rBV4	28222	37020	0.40%	0.036%
7	4.851	362	368	371	rBV6	28523	37255	0.40%	0.037%
8	5.657	502	505	506	rBV3	25725	22630	0.24%	0.022%
9	5.822	528	533	539	rVB7	24435	51186	0.55%	0.050%
10	6.081	571	577	580	rBV8	7843	15331	0.16%	0.015%
11	6.381	625	628	632	rVB6	6865	9490	0.10%	0.009%
12	6.657	671	675	676	rBV4	9540	10892	0.12%	0.011%
13	6.781	690	696	708	rBV	1963199	3035901	32.47%	2.976%
14	6.857	708	709	713	rVV4	16493	19333	0.21%	0.019%
15	6.940	717	723	738	rVV	1381353	2153000	23.02%	2.110%
16	7.034	738	739	742	rVB3	12519	9465	0.10%	0.009%
17	7.134	750	756	767	rBV	1914028	2979834	31.87%	2.921%
18	7.228	767	772	779	rVB	89117	137378	1.47%	0.135%
19	7.598	828	835	843	rBV	1560016	2441699	26.11%	2.393%
20	7.910	885	888	895	rBV6	9050	13142	0.14%	0.013%
21	8.316	949	957	972	rBV	2157810	3515914	37.60%	3.446%
22	8.757	1024	1032	1044	rBV	1602920	2580681	27.60%	2.530%
23	9.181	1101	1104	1109	rVB5	6276	11066	0.12%	0.011%
24	9.392	1138	1140	1143	rVB3	9075	9860	0.11%	0.010%
25	9.475	1146	1154	1163	rBV	1273253	2073341	22.17%	2.032%
26	9.616	1175	1178	1181	rBV5	6852	9637	0.10%	0.009%
27	10.010	1237	1245	1257	rBV	2064920	3438200	36.77%	3.370%
28	10.098	1259	1260	1265	rVB3	9358	10677	0.11%	0.010%
29	10.228	1279	1282	1287	rVB6	9478	14340	0.15%	0.014%
30	10.381	1301	1308	1319	rVB	2048496	3407333	36.44%	3.340%
31	10.528	1324	1333	1347	rBV	1935469	3296781	35.26%	3.232%
32	10.816	1380	1382	1386	rVB5	9057	9916	0.11%	0.010%
33	11.033	1412	1419	1425	rBV2	79253	145460	1.56%	0.143%
34	11.186	1444	1445	1449	rBV3	8737	11311	0.12%	0.011%

Data Path : Z:\HPCHEM1\BNA_M\Data\BM041415\
 Data File : BM000982.D
 Acq On : 14 Apr 2015 13:58
 Operator : TP/IZ
 Sample : PB82670BL
 Misc : SBLK43
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041415.M
 Title : SVOA CALIBRATION

35	11.980	1574	1580	1586	rBV4	43703	74744	0.80%	0.073%
36	12.622	1685	1689	1692	rBV6	10164	12622	0.13%	0.012%
37	13.669	1861	1867	1877	rBV	3138467	4509876	48.23%	4.421%
38	13.945	1906	1914	1925	rBV	3923850	5809370	62.13%	5.694%
39	14.257	1960	1967	1976	rBV2	2913344	4415013	47.22%	4.328%
40	14.333	1979	1980	1985	rVB4	11788	15640	0.17%	0.015%
41	14.469	1996	2003	2019	rBV	1085740	1850472	19.79%	1.814%
42	14.592	2023	2024	2027	rVV3	17335	20687	0.22%	0.020%
43	14.627	2028	2030	2036	rVV7	15260	26158	0.28%	0.026%
44	14.692	2036	2041	2045	rVV8	12430	25439	0.27%	0.025%
45	14.927	2078	2081	2085	rVV5	11791	20479	0.22%	0.020%
46	14.998	2091	2093	2097	rVB4	8414	10077	0.11%	0.010%
47	15.068	2103	2105	2107	rBV2	10891	9629	0.10%	0.009%
48	15.257	2130	2137	2146	rBV	5002734	7275933	77.81%	7.132%
49	15.380	2152	2158	2170	rBV	854695	1211267	12.95%	1.187%
50	15.492	2170	2177	2183	rVB4	65761	124409	1.33%	0.122%
51	15.815	2230	2232	2240	rVB6	11770	24052	0.26%	0.024%
52	15.957	2250	2256	2257	rBV5	12209	19562	0.21%	0.019%
53	16.045	2267	2271	2274	rVB6	7244	11052	0.12%	0.011%
54	16.204	2297	2298	2301	rBV3	10914	10207	0.11%	0.010%
55	16.533	2352	2354	2357	rBV4	6676	9706	0.10%	0.010%
56	16.798	2393	2399	2402	rVV7	15861	25088	0.27%	0.025%
57	16.862	2407	2410	2411	rBV3	11042	9630	0.10%	0.009%
58	17.004	2427	2434	2444	rBV	3684489	5236648	56.00%	5.133%
59	17.104	2444	2451	2465	rVV2	5690795	7937750	84.89%	7.781%
60	17.298	2481	2484	2489	rVB6	15205	25269	0.27%	0.025%
61	17.627	2537	2540	2543	rBV5	10775	17425	0.19%	0.017%
62	17.674	2546	2548	2553	rVB5	16810	22920	0.25%	0.022%
63	17.915	2585	2589	2591	rBV5	11243	13905	0.15%	0.014%
64	17.974	2596	2599	2602	rVB5	12816	13651	0.15%	0.013%
65	18.192	2632	2636	2640	rBV6	18618	27481	0.29%	0.027%
66	18.239	2643	2644	2647	rBV3	9350	11013	0.12%	0.011%
67	18.498	2685	2688	2689	rBV3	12672	12177	0.13%	0.012%
68	18.815	2740	2742	2743	rBV2	10780	9703	0.10%	0.010%
69	18.827	2743	2744	2746	rBV2	12061	11672	0.12%	0.011%
70	19.039	2776	2780	2785	rBV2	62797	87211	0.93%	0.085%
71	19.292	2819	2823	2828	rBV2	55979	80361	0.86%	0.079%

Data Path : Z:\HPCHEM1\BNA_M\Data\BM041415\
Data File : BM000982.D
Acq On : 14 Apr 2015 13:58
Operator : TP/IZ
Sample : PB82670BL
Misc : SBLK43
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041415.M
Title : SVOA CALIBRATION

72	19.345	2828	2832	2835	rBV4	41058	58624	0.63%	0.057%
73	19.403	2836	2842	2849	rVV	6712343	9312915	99.59%	9.129%
74	19.462	2849	2852	2857	rVB3	102107	130645	1.40%	0.128%
75	19.762	2899	2903	2906	rVB2	38706	41410	0.44%	0.041%
76	19.962	2934	2937	2941	rBV2	66537	76785	0.82%	0.075%
77	20.392	3007	3010	3014	rBV4	64523	85060	0.91%	0.083%
78	20.456	3017	3021	3024	rVV	120449	139485	1.49%	0.137%
79	20.498	3024	3028	3030	rVB4	47386	55910	0.60%	0.055%
80	20.656	3051	3055	3057	rBV4	40229	51101	0.55%	0.050%
81	20.786	3074	3077	3082	rBV2	68715	95419	1.02%	0.094%
82	20.921	3097	3100	3103	rVB	99778	97359	1.04%	0.095%
83	21.003	3110	3114	3118	rVB5	64363	87815	0.94%	0.086%
84	21.203	3143	3148	3162	rVB	5251544	6421746	68.68%	6.295%
85	21.356	3171	3174	3179	rBV	168416	179259	1.92%	0.176%
86	21.780	3243	3246	3250	rVB	100508	115921	1.24%	0.114%
87	23.244	3488	3495	3510	rBV2	5224956	9350863	100.00%	9.166%
88	23.380	3511	3518	3529	rVB	3420239	6226605	66.59%	6.103%


Sum of corrected areas: 102018750

Data Path : Z:\HPCHEM1\BNA_M\Data\BM041415\
Data File : BM000982.D
Acq On : 14 Apr 2015 13:58
Operator : TP/IZ
Sample : PB82670BL
Misc : SBLK43
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK43

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

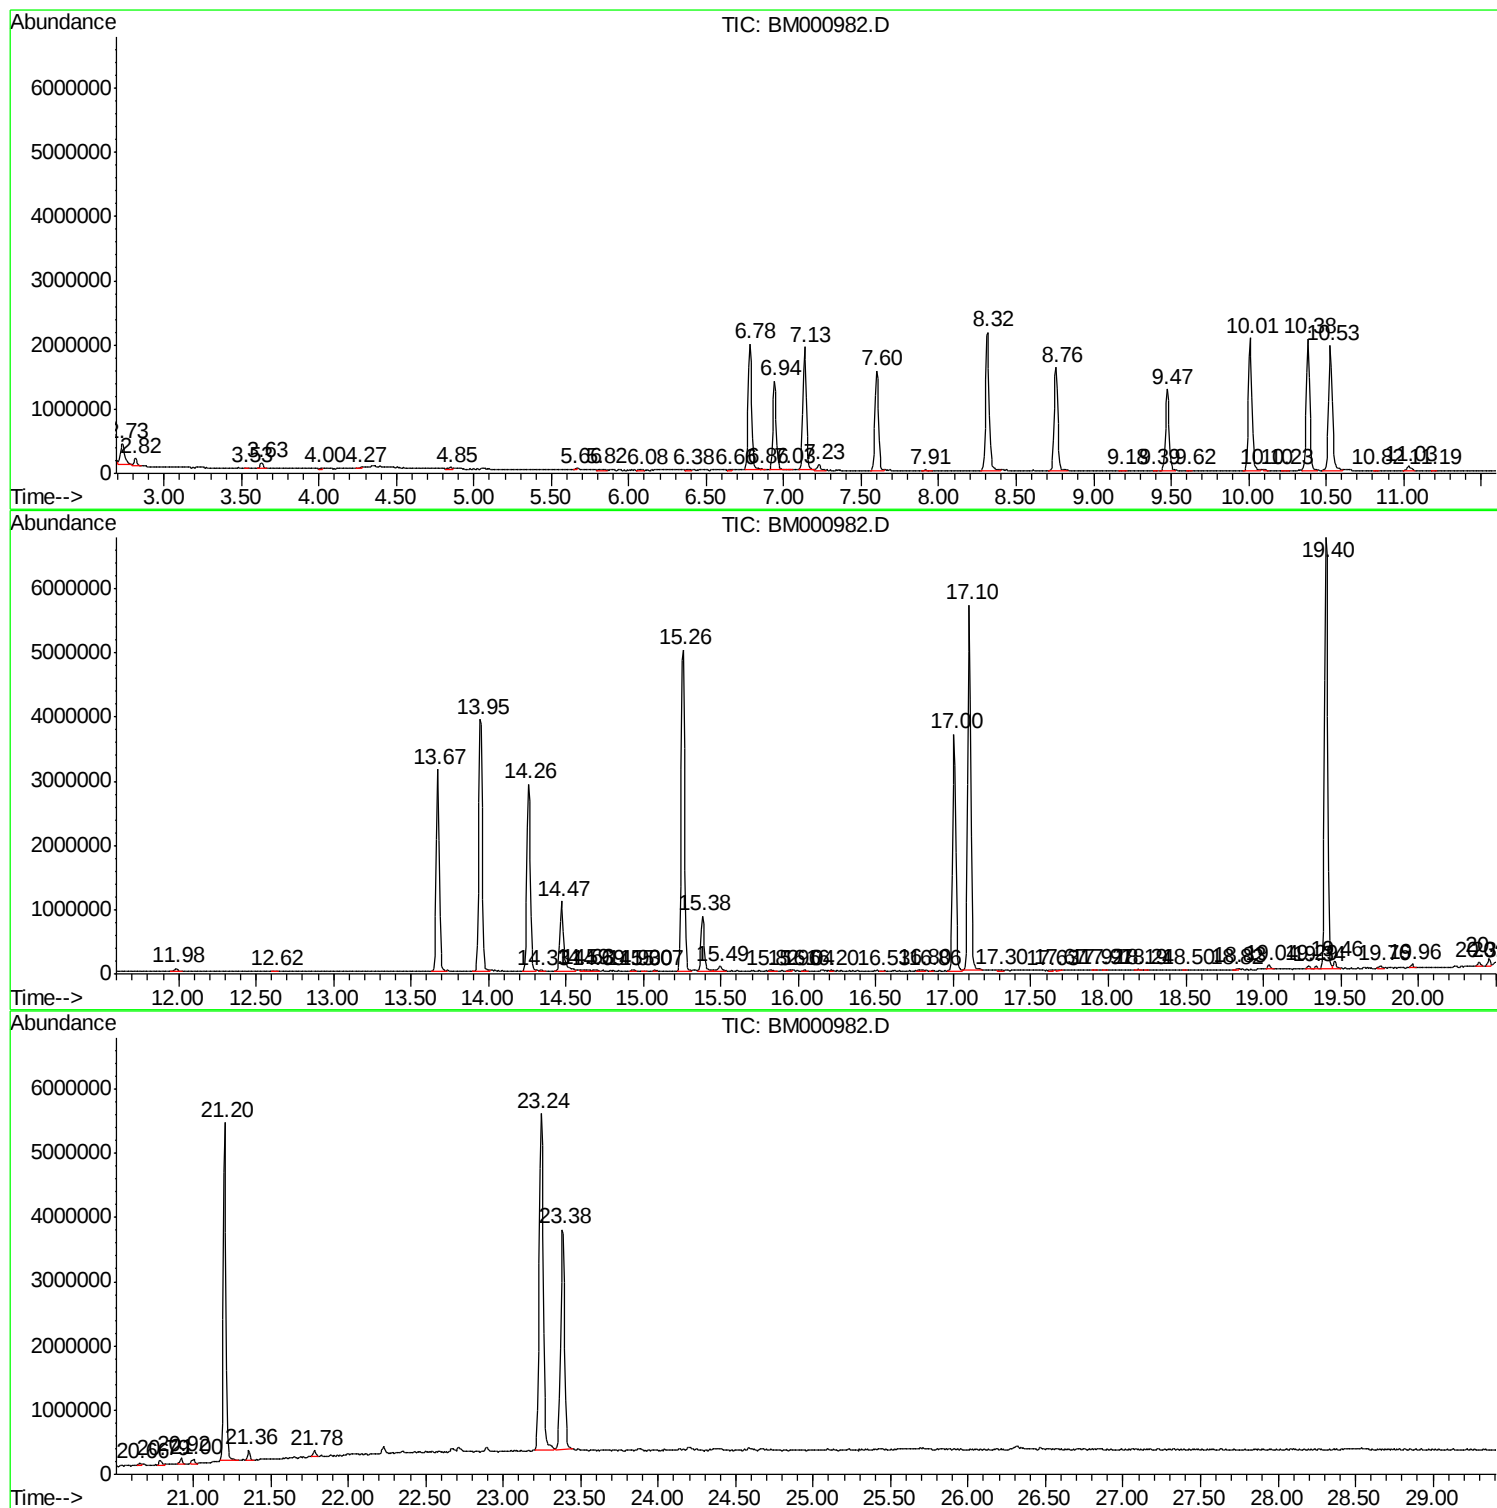

Data Path : Z:\HPCHEM1\BNA_M\Data\BM041415\
Data File : BM000982.D
Acq On : 14 Apr 2015 13:58
Operator : TP/IZ
Sample : PB82670BL
Misc : SBLK43
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\Data\BM041415\
Data File : BM000982.D
Acq On : 14 Apr 2015 13:58
Operator : TP/IZ
Sample : PB82670BL
Misc : SBLK43
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc