




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034664.D
Acq On : 14 Apr 2022 12:27
Operator : CG/JU
Sample : N2342-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J09

Manual IntegrationsAPPROVED

Quant Time: Apr 15 00:16:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 14 23:42:00 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/23/2022

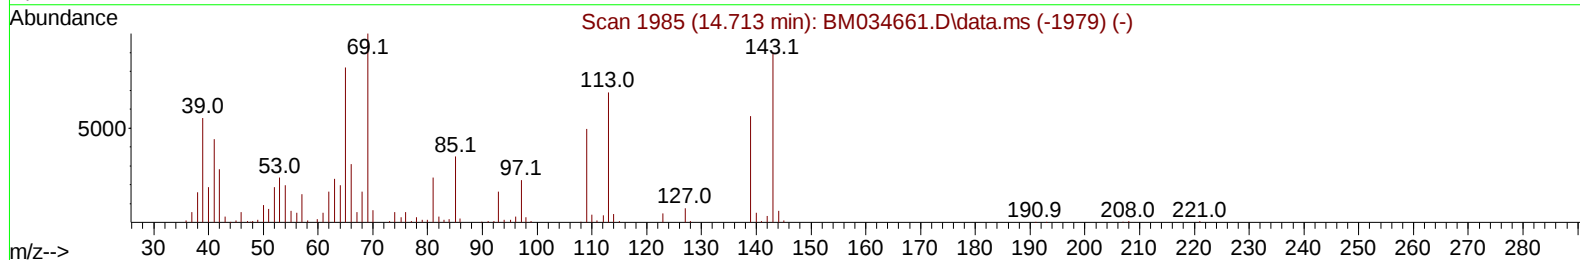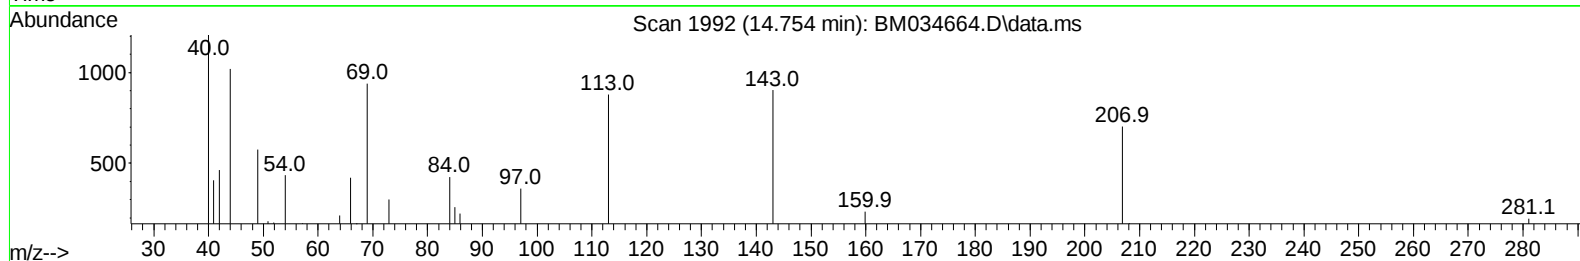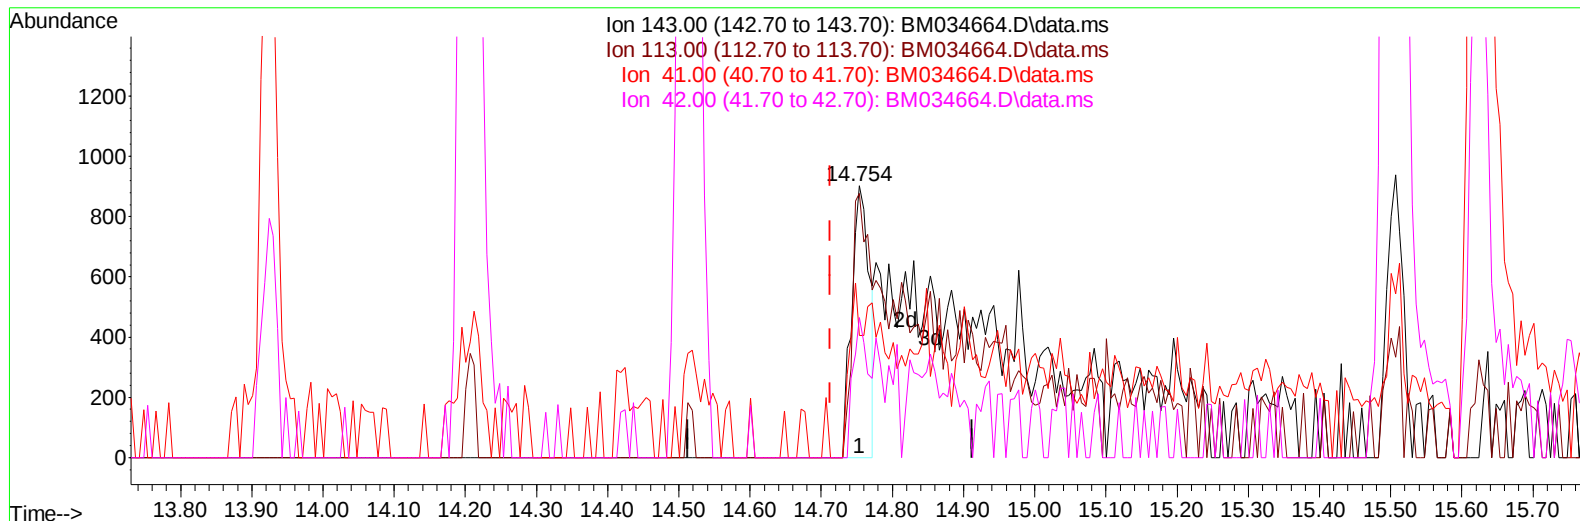

TIC: BM034664.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.754min (+ 0.041) 0.50 ng/ul

response 1561

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	97.34#
41.00	31.90	44.90#
42.00	19.10	51.44#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034664.D
 Acq On : 14 Apr 2022 12:27
 Operator : CG/JU
 Sample : N2342-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0J09

Manual IntegrationsAPPROVED

Quant Time: Apr 15 00:16:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 14 23:42:00 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/23/2022

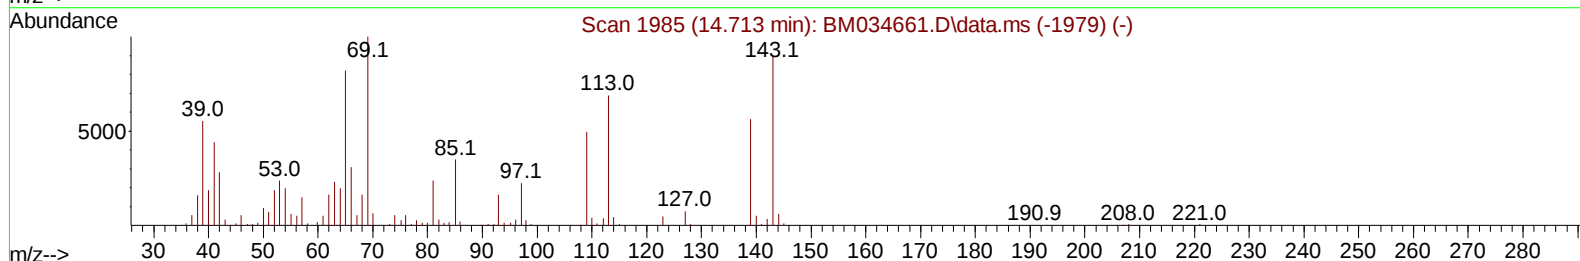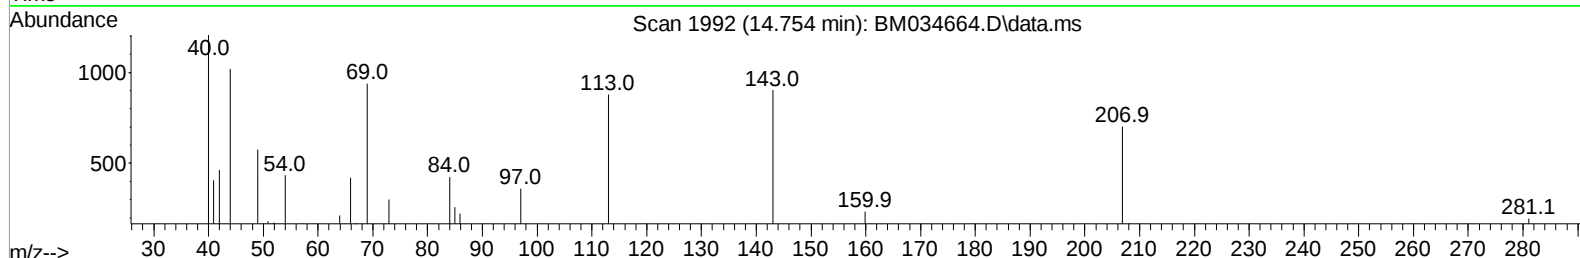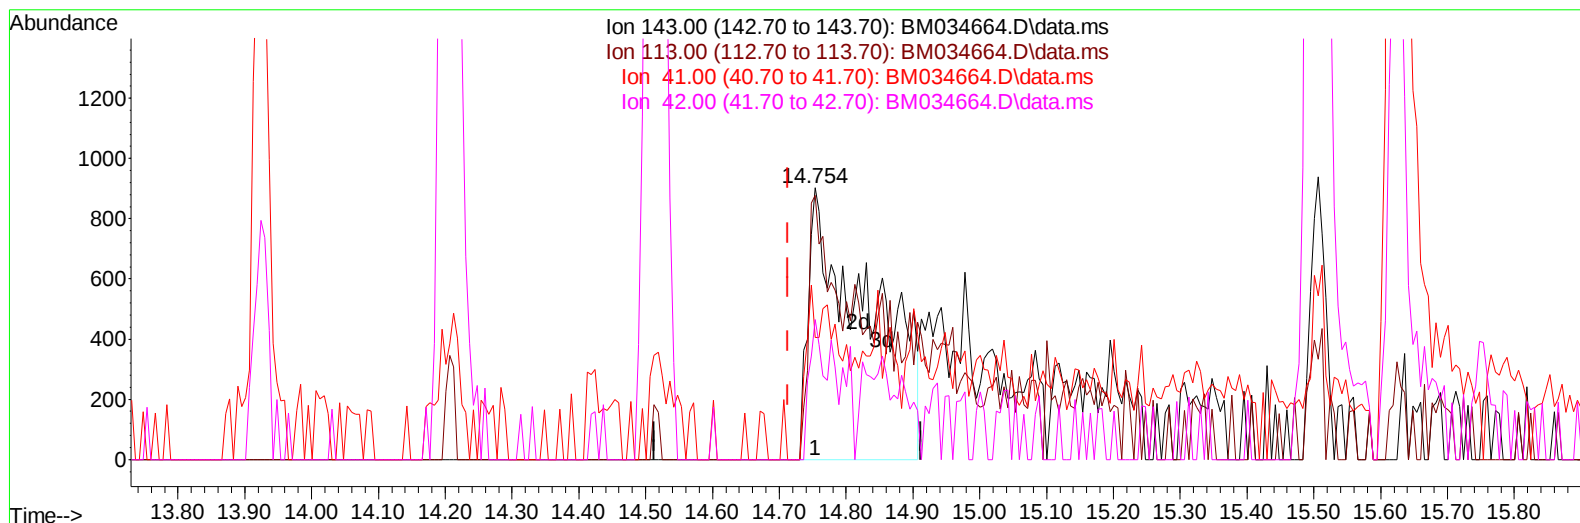

TIC: BM034664.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.754min (+ 0.041) 1.80 ng/ul m

response 5652

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	97.34#
41.00	31.90	44.90#
42.00	19.10	51.44#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034664.D
 Acq On : 14 Apr 2022 12:27
 Operator : CG/JU
 Sample : N2342-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0J09

Manual IntegrationsAPPROVED

Quant Time: Apr 15 00:16:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 14 23:42:00 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/23/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.866	152	117146	20.000	ng/ul	0.00
20) Naphthalene-d8	10.678	136	485033	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.513	164	285633	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.259	188	547520	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.436	240	475964	20.000	ng/ul	# 0.00
88) Perylene-d12	23.806	264	518065	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.249	96	13890	4.228	ng/uL	0.00
4) Pyridine-d5	3.678	84	81152	10.236	ng/ul	0.00
7) Phenol-d5	7.031	99	61439	6.301	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.195	67	202396	31.151	ng/ul	0.00
11) 2-Chlorophenol-d4	7.395	132	184697	24.504	ng/ul	0.00
15) 4-Methylphenol-d8	8.584	113	116544	15.302	ng/ul	0.00
21) Nitrobenzene-d5	9.031	128	107712	30.216	ng/ul	0.00
24) 2-Nitrophenol-d4	9.754	143	107449	28.952	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.301	165	170662	24.421	ng/ul	0.00
31) 4-Chloroaniline-d4	10.813	131	226846	23.528	ng/ul	0.00
46) Dimethylphthalate-d6	13.924	166	669774	32.452	ng/ul	0.00
49) Acenaphthylene-d8	14.207	160	766086	28.879	ng/ul	0.00
54) 4-Nitrophenol-d4	14.754	143	5652m	1.796	ng/ul	0.04
60) Fluorene-d10	15.507	176	583243	32.701	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.624	200	87428	26.157	ng/ul	0.00
73) Anthracene-d10	17.354	188	947726	36.306	ng/ul	0.00
81) Pyrene-d10	19.648	212	1113118	42.849	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.653	264	1012892	38.868	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034664.D
Acq On : 14 Apr 2022 12:27
Operator : CG/JU
Sample : N2342-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J09

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/23/2022

Quant Time: Apr 15 00:16:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 14 23:42:00 2022
Response via : Initial Calibration

