




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034676.D
 Acq On : 14 Apr 2022 20:25
 Operator : CG/JU
 Sample : PB144054BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK054

Manual IntegrationsAPPROVED

Quant Time: Apr 14 23:44:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 14 23:42:00 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/23/2022

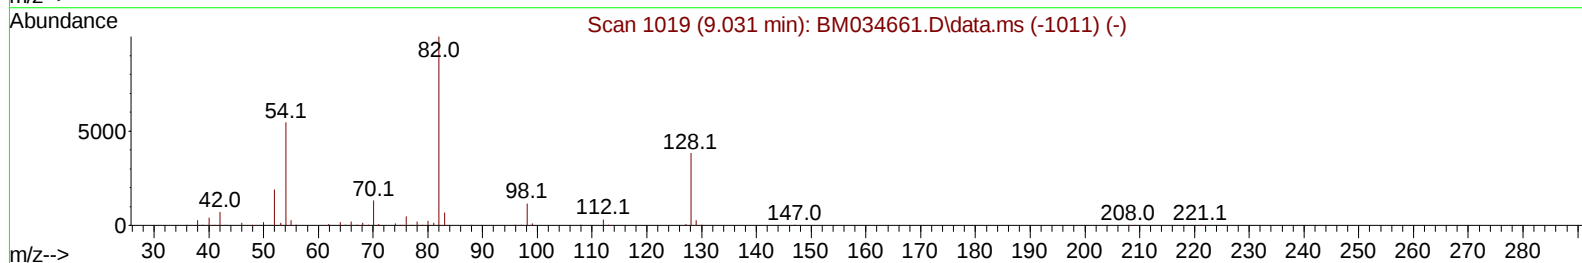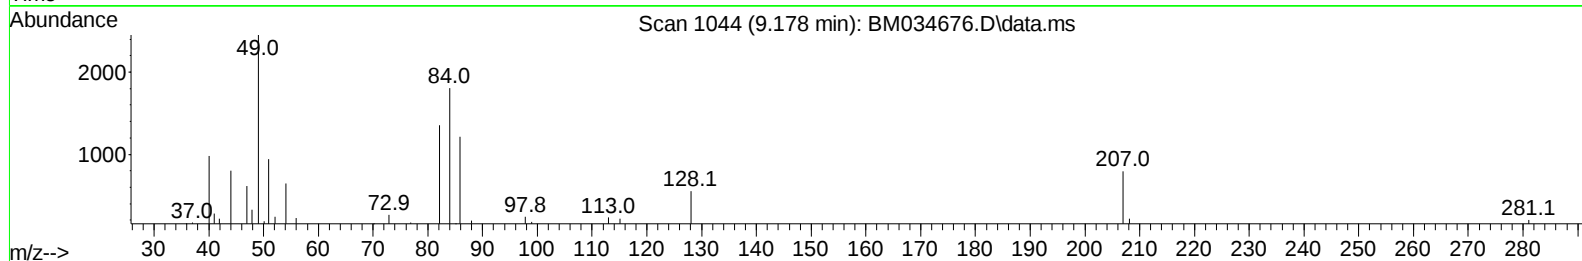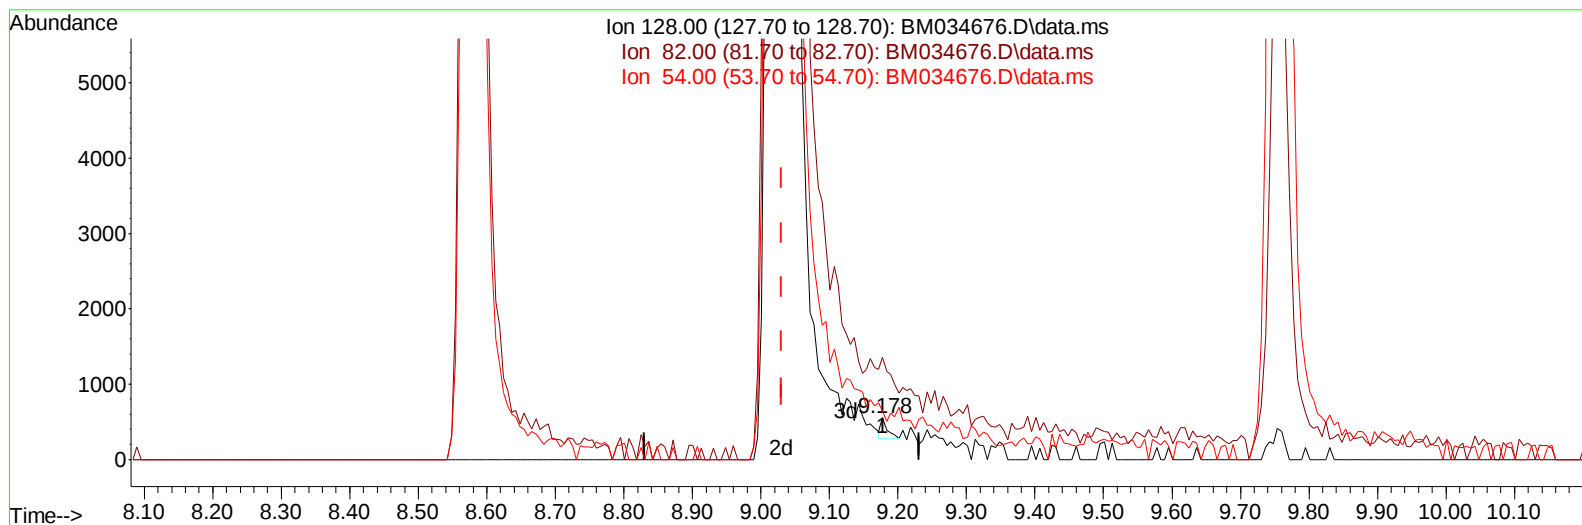

TIC: BM034676.D\data.ms

(21) Nitrobenzene-d5 (S)

9.178min (+ 0.147) 0.04 ng/u1

response 179

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	228.00	243.53
54.00	100.50	116.01
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034676.D
 Acq On : 14 Apr 2022 20:25
 Operator : CG/JU
 Sample : PB144054BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK054

Manual IntegrationsAPPROVED

Quant Time: Apr 14 23:44:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 14 23:42:00 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/23/2022

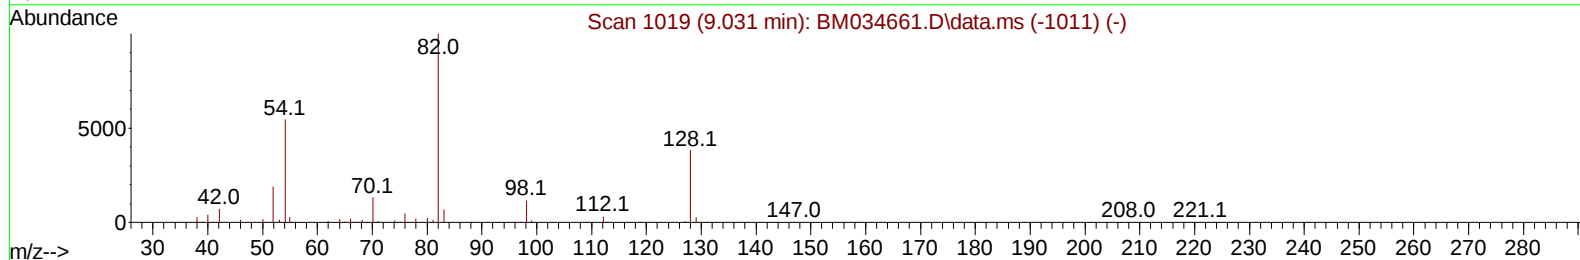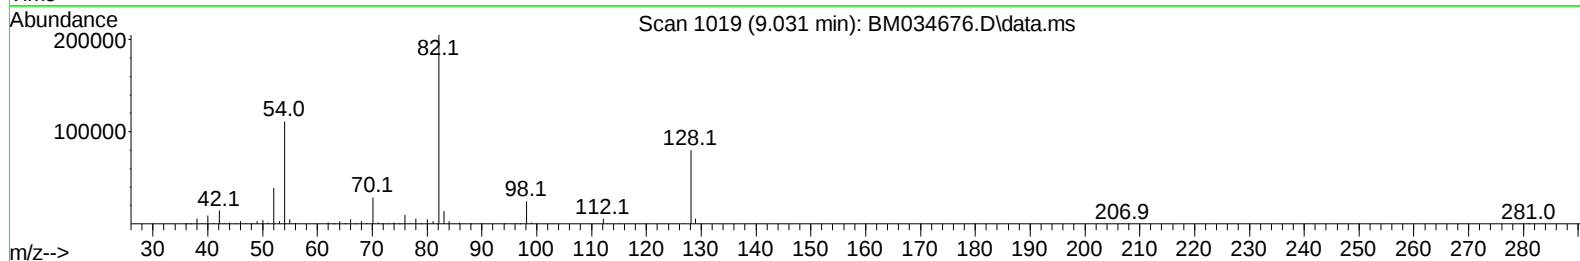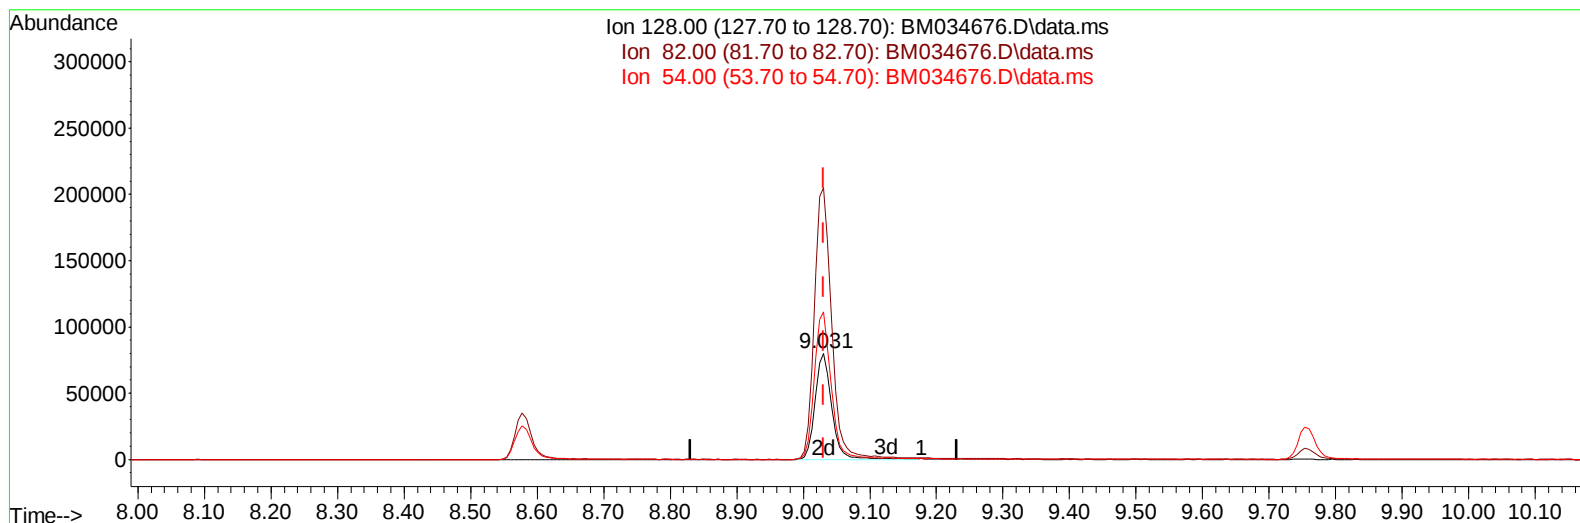

TIC: BM034676.D\data.ms

(21) Nitrobenzene-d5 (S)

9.031min (-0.000) 29.66 ng/u1 m

response 138784

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	228.00	256.03
54.00	100.50	138.98#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034676.D
Acq On : 14 Apr 2022 20:25
Operator : CG/JU
Sample : PB144054BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK054

Manual IntegrationsAPPROVED

Quant Time: Apr 14 23:44:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 14 23:42:00 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/23/2022

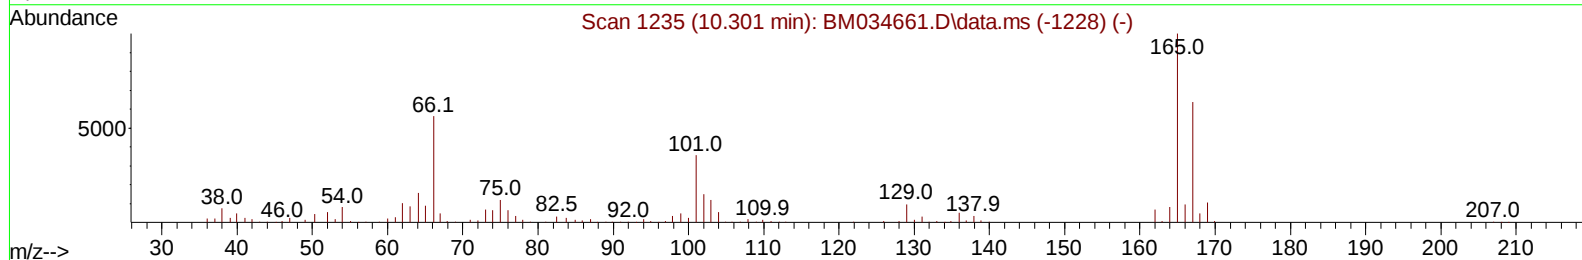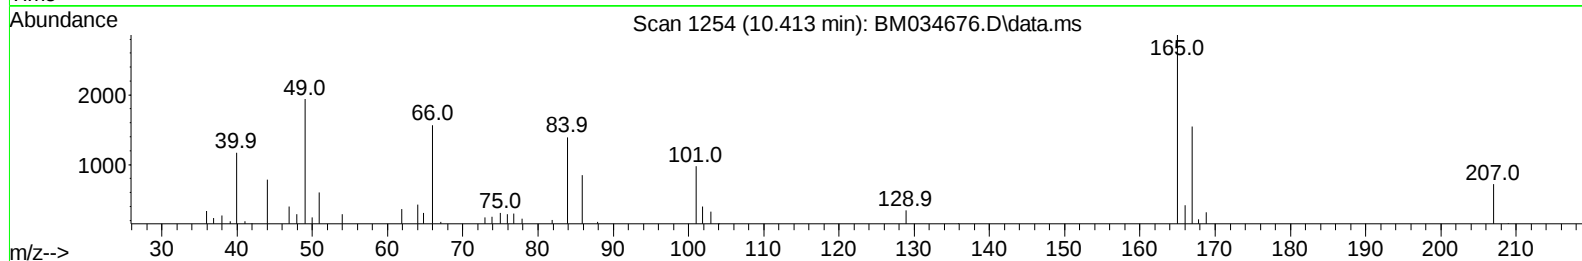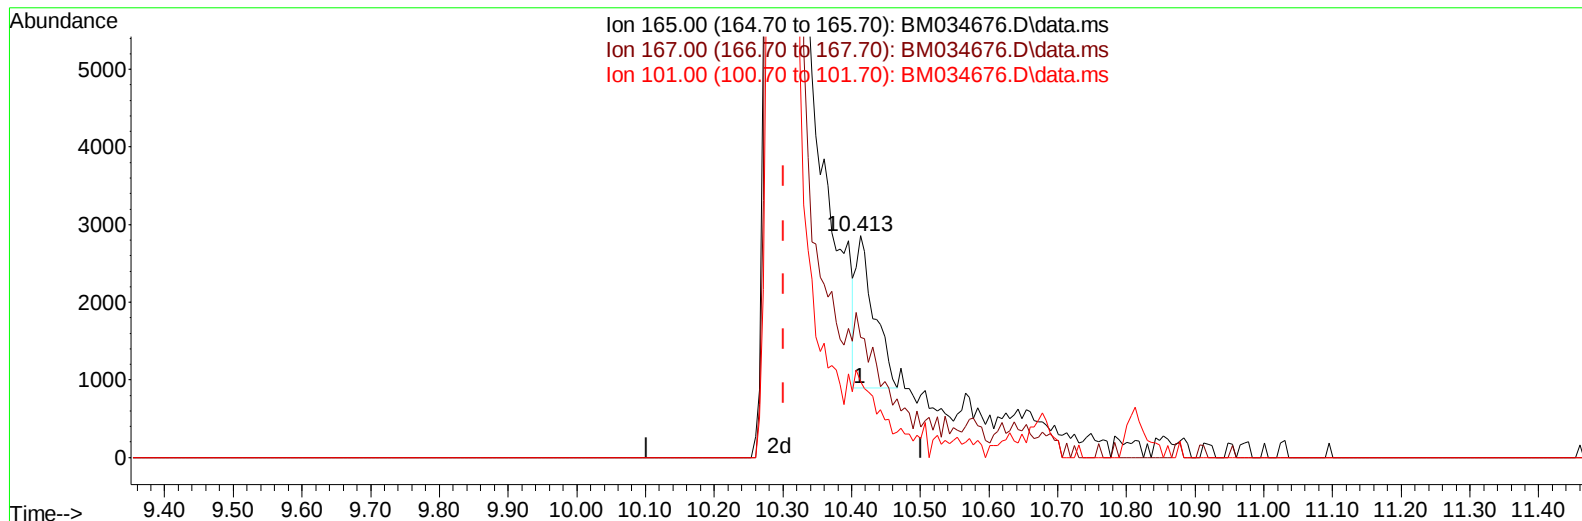

TIC: BM034676.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.413min (+ 0.112) 0.39 ng/u1

response 3611

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	63.20	54.04
101.00	30.30	34.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034676.D
 Acq On : 14 Apr 2022 20:25
 Operator : CG/JU
 Sample : PB144054BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK054

Manual IntegrationsAPPROVED

Quant Time: Apr 14 23:44:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 14 23:42:00 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/23/2022

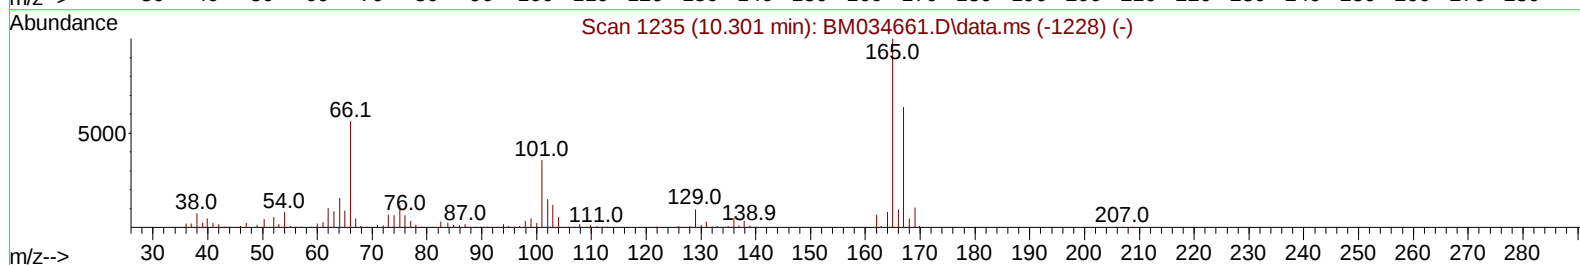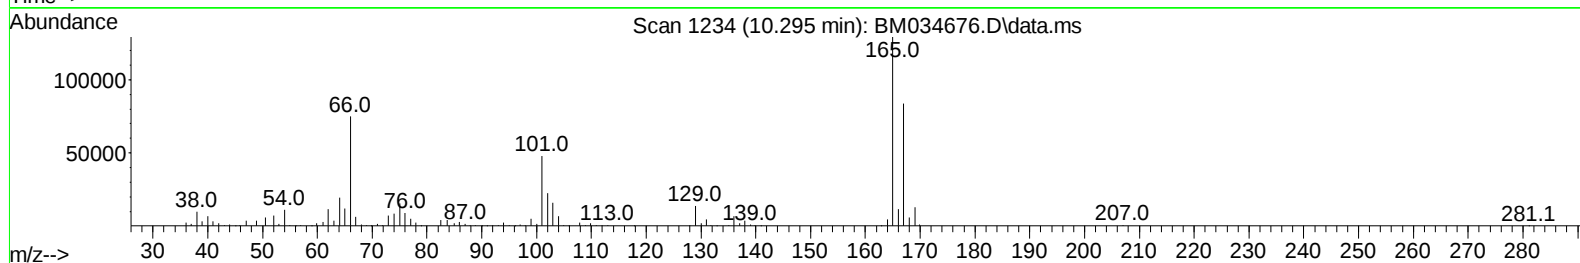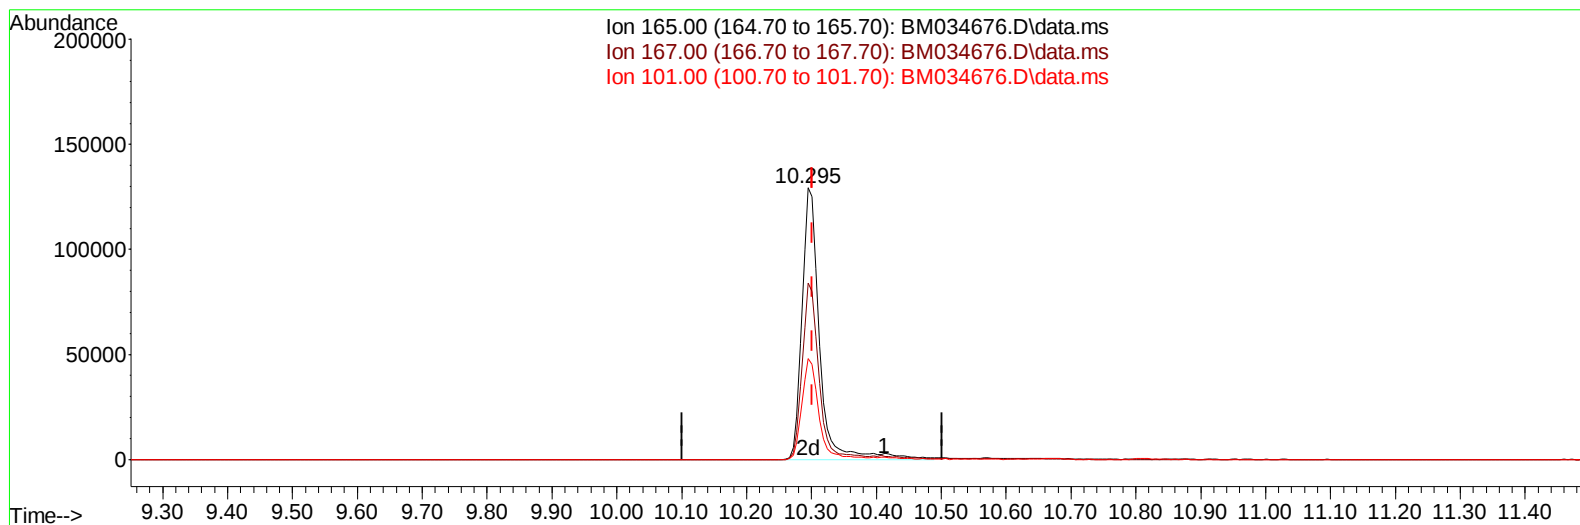

TIC: BM034676.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.295min (-0.006) 26.86 ng/ul m

response 246364

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	63.20	64.86
101.00	30.30	37.08#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034676.D
 Acq On : 14 Apr 2022 20:25
 Operator : CG/JU
 Sample : PB144054BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK054

Manual IntegrationsAPPROVED

Quant Time: Apr 14 23:44:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 14 23:42:00 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/23/2022

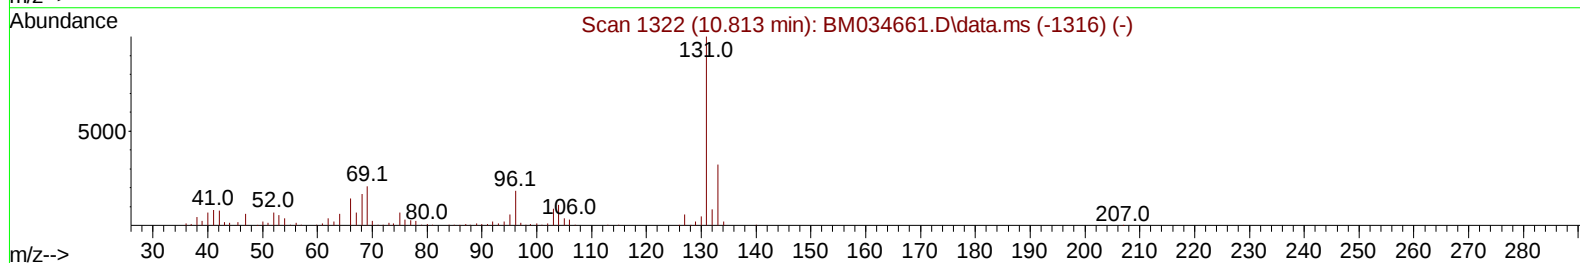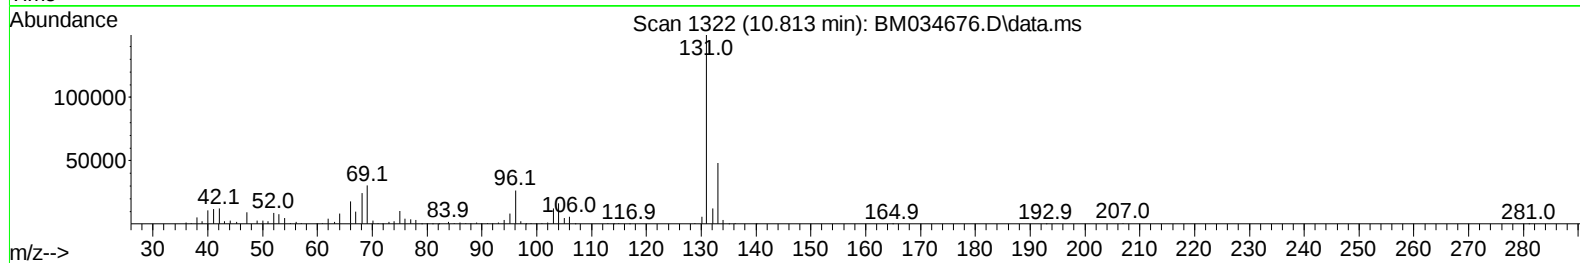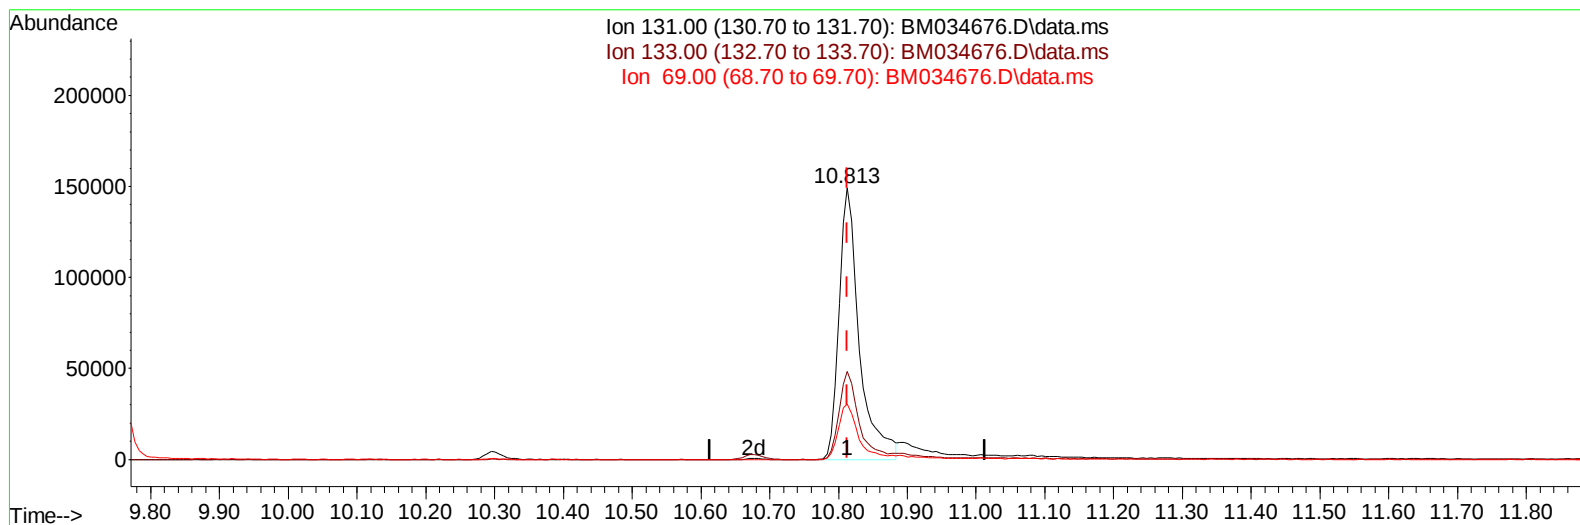

TIC: BM034676.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.813min (-0.000) 24.20 ng/u1

response 306299

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.00	32.44
69.00	16.80	20.34#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034676.D
 Acq On : 14 Apr 2022 20:25
 Operator : CG/JU
 Sample : PB144054BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK054

Manual IntegrationsAPPROVED

Quant Time: Apr 14 23:44:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 14 23:42:00 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/23/2022

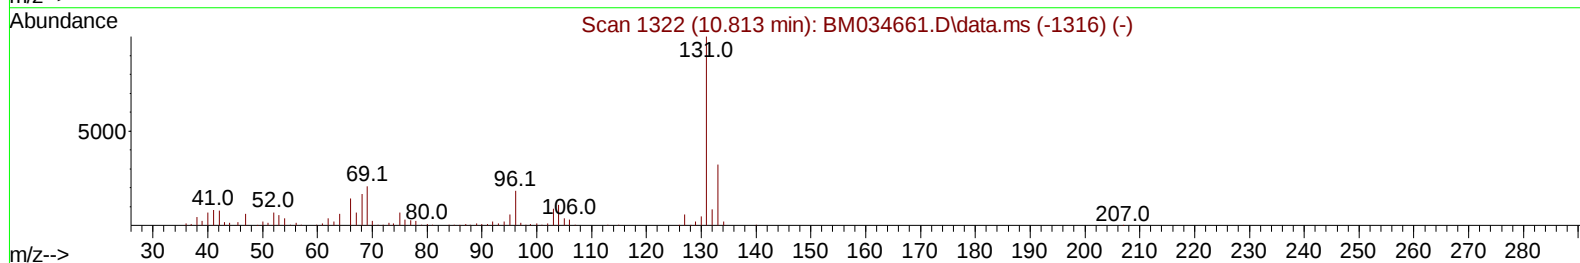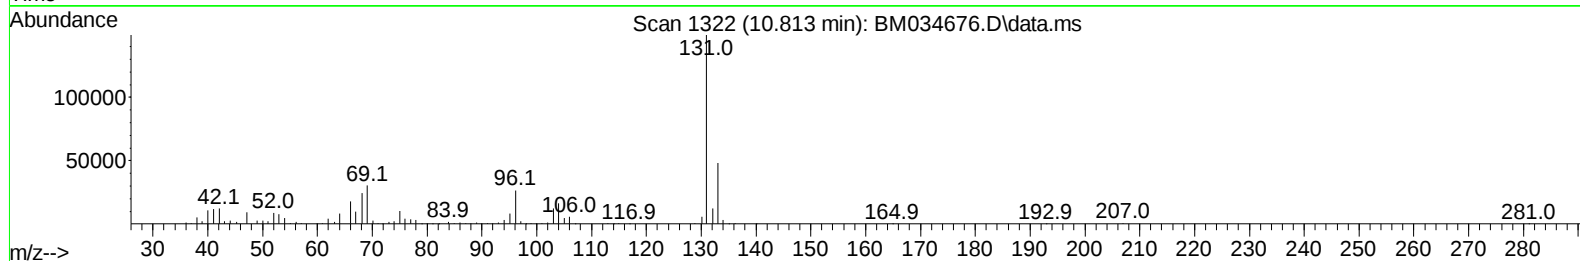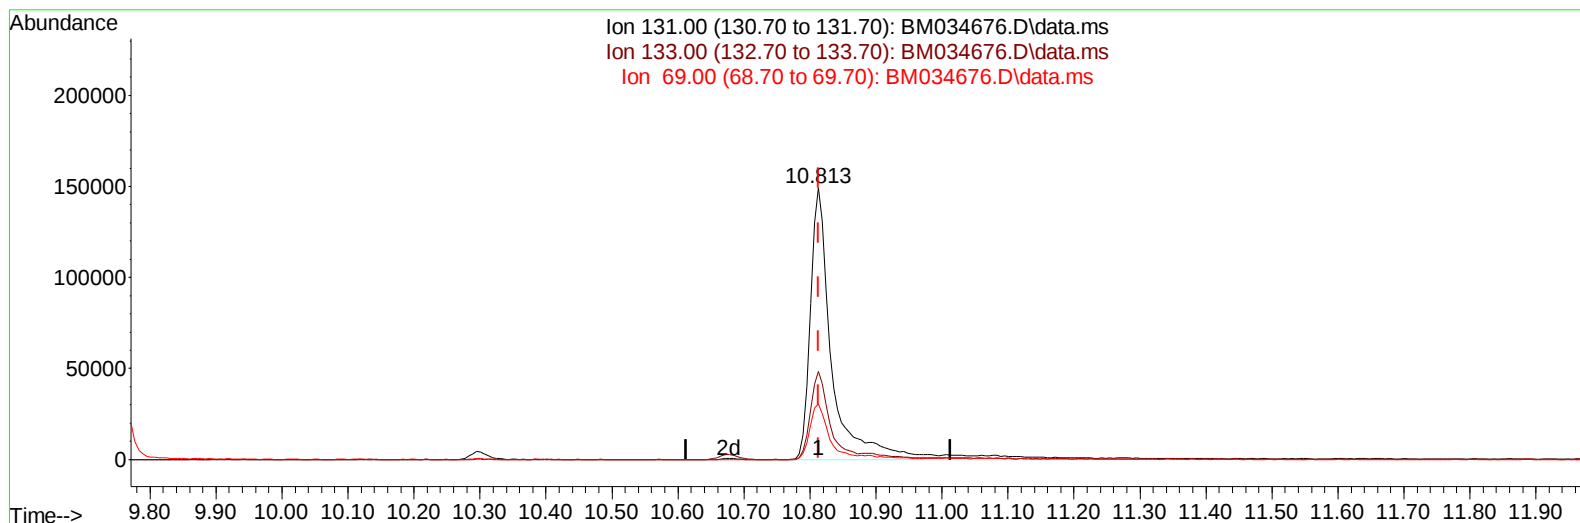

TIC: BM034676.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.813min (-0.000) 26.45 ng/ul m

response 334683

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.00	32.44
69.00	16.80	20.34#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034676.D
Acq On : 14 Apr 2022 20:25
Operator : CG/JU
Sample : PB144054BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK054

Manual IntegrationsAPPROVED

Quant Time: Apr 14 23:44:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 14 23:42:00 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/23/2022

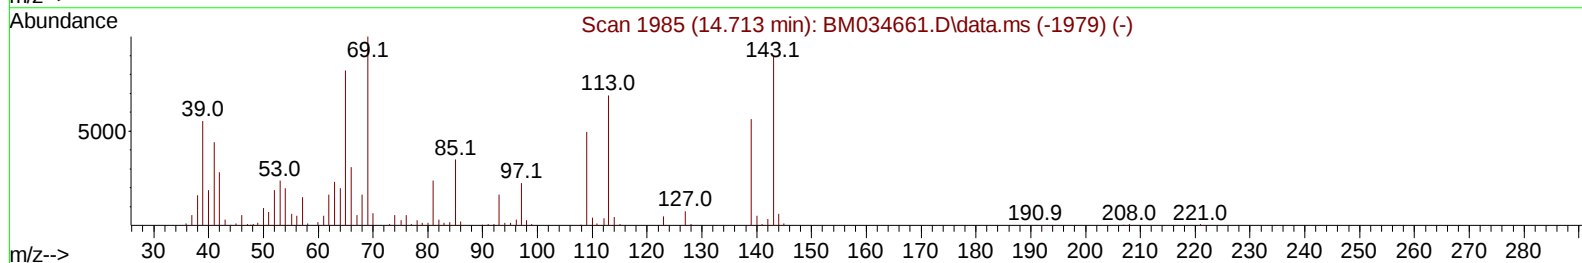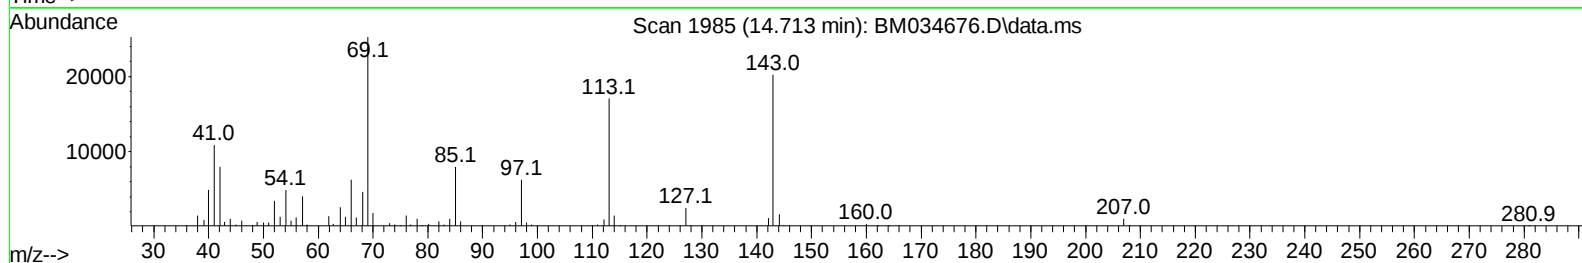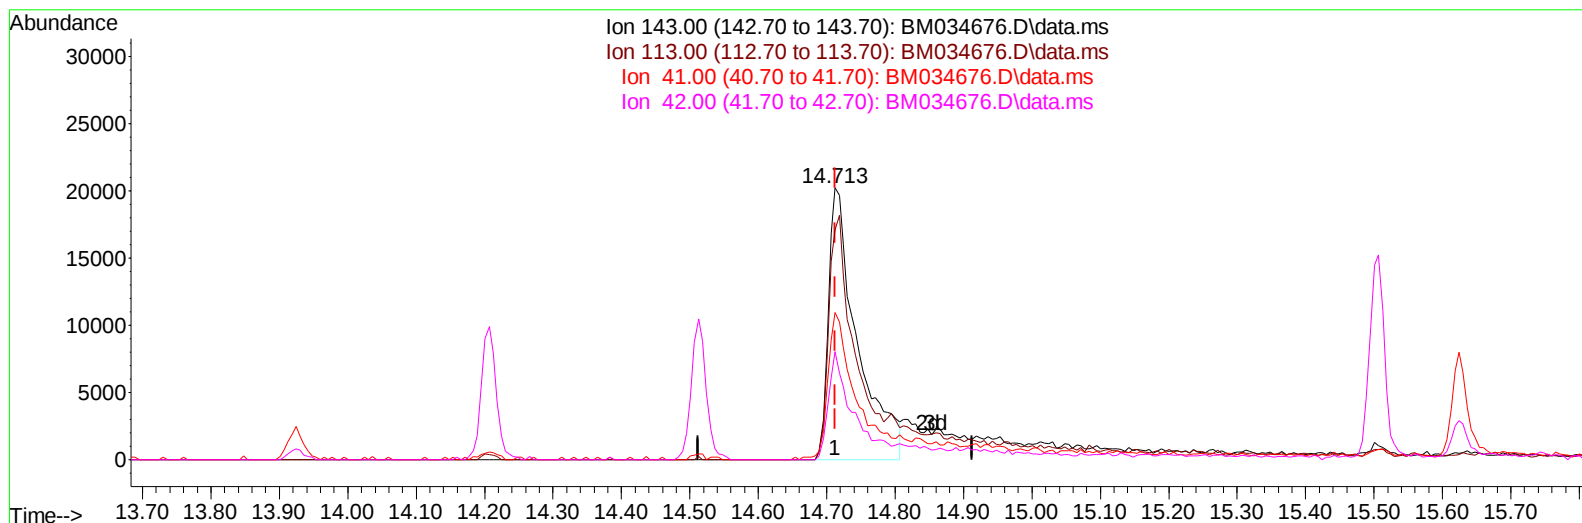

TIC: BM034676.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.713min (-0.000) 14.02 ng/u1

response 58934

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	84.52
41.00	31.90	54.02#
42.00	19.10	39.68#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034676.D
Acq On : 14 Apr 2022 20:25
Operator : CG/JU
Sample : PB144054BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK054

Manual IntegrationsAPPROVED

Quant Time: Apr 14 23:44:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 14 23:42:00 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/23/2022

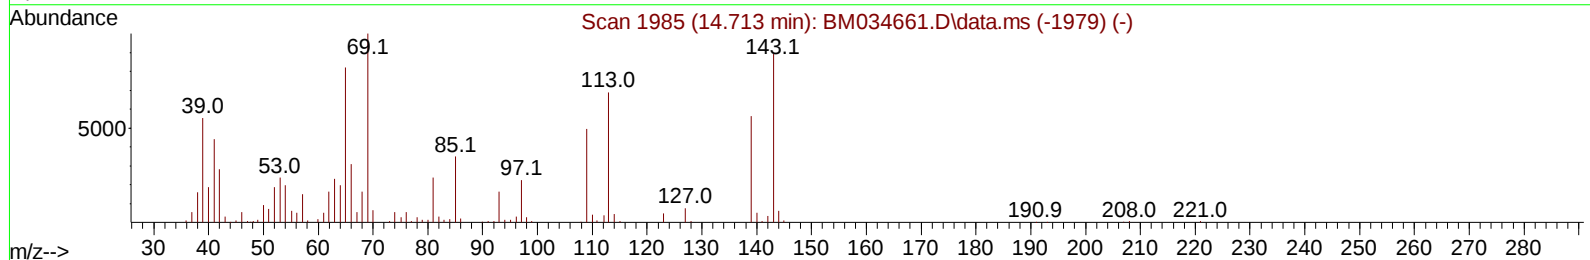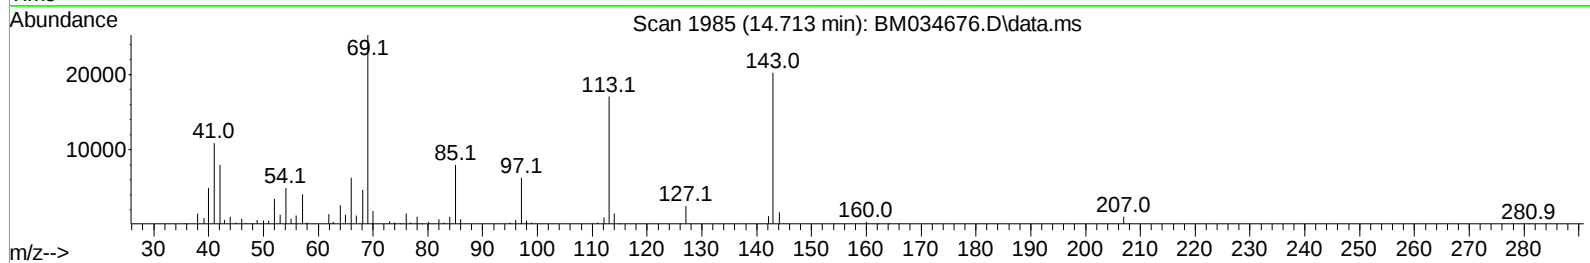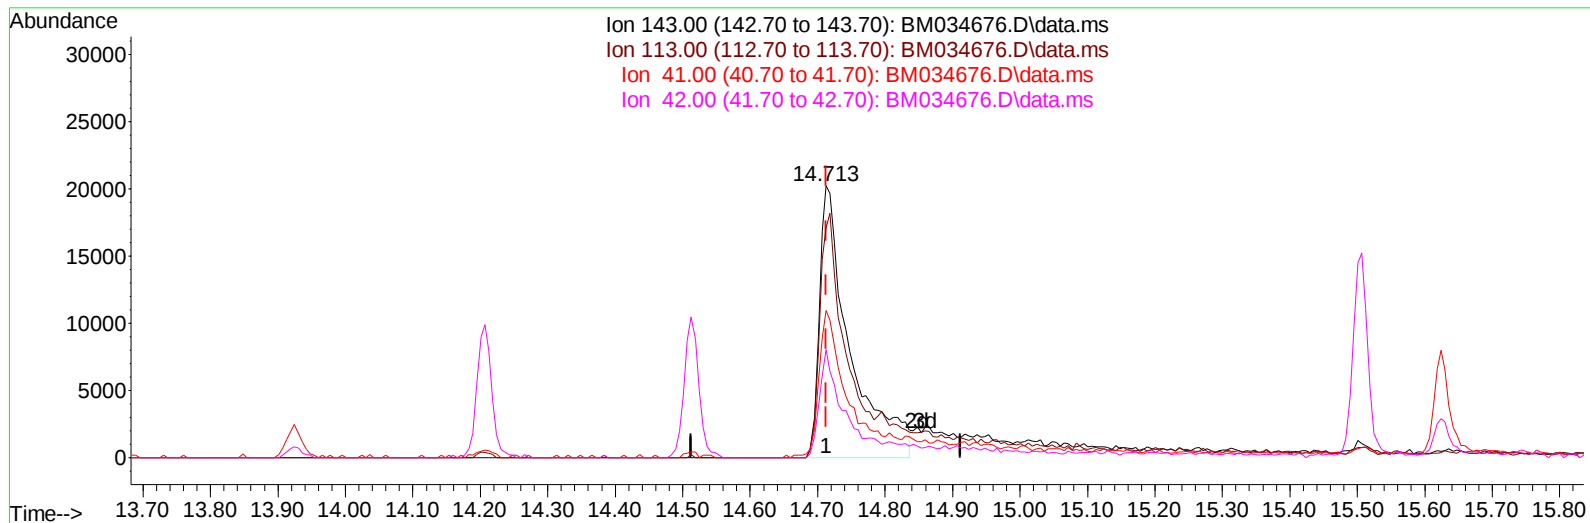

TIC: BM034676.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.713min (-0.000) 15.13 ng/ul m

response 63619

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	84.52
41.00	31.90	54.02#
42.00	19.10	39.68#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034676.D
 Acq On : 14 Apr 2022 20:25
 Operator : CG/JU
 Sample : PB144054BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK054

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/23/2022

Quant Time: Apr 14 23:44:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 14 23:42:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.866	152	149329	20.000	ng/ul	0.00
20) Naphthalene-d8	10.678	136	636676	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.513	164	381539	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.254	188	746804	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.430	240	682155	20.000	ng/ul	# 0.00
88) Perylene-d12	23.806	264	748148	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.249	96	24015	5.735	ng/uL	0.00
4) Pyridine-d5	3.672	84	282696	27.973	ng/ul	0.00
7) Phenol-d5	7.031	99	334425	26.907	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.195	67	250652	30.264	ng/ul	0.00
11) 2-Chlorophenol-d4	7.395	132	289194	30.099	ng/ul	0.00
15) 4-Methylphenol-d8	8.578	113	274184	28.241	ng/ul	0.00
21) Nitrobenzene-d5	9.031	128	138784m	29.660	ng/ul	0.00
24) 2-Nitrophenol-d4	9.754	143	141100	28.963	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.295	165	246364m	26.857	ng/ul	0.00
31) 4-Chloroaniline-d4	10.813	131	334683m	26.445	ng/ul	0.00
46) Dimethylphthalate-d6	13.924	166	834718	30.277	ng/ul	0.00
49) Acenaphthylene-d8	14.207	160	979094	27.631	ng/ul	0.00
54) 4-Nitrophenol-d4	14.713	143	63619m	15.134	ng/ul	0.00
60) Fluorene-d10	15.507	176	701490	29.444	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.624	200	109574	24.034	ng/ul	0.00
73) Anthracene-d10	17.354	188	1065840	29.935	ng/ul	0.00
81) Pyrene-d10	19.648	212	1225223	32.908	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.653	264	1109627	29.485	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034676.D
Acq On : 14 Apr 2022 20:25
Operator : CG/JU
Sample : PB144054BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK054

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/23/2022

Quant Time: Apr 14 23:44:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 14 23:42:00 2022
Response via : Initial Calibration

