

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034678.D
 Acq On : 14 Apr 2022 21:38
 Operator : CG/JU
 Sample : N2316-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETNQ3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
 Supervised By :Yogesh Patel 04/23/2022

Quant Time: Apr 14 23:45:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 14 23:42:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.866	152	112890	20.000	ng/u1	0.00
20) Naphthalene-d8	10.672	136	462026	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.513	164	272201	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.254	188	538077	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.430	240	478354m	20.000	ng/u1	0.00
88) Perylene-d12	23.806	264	534635	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.243	96	13158m	4.156	ng/uL	0.00
4) Pyridine-d5	3.666	84	150445	19.692	ng/u1	0.00
7) Phenol-d5	7.025	99	186601	19.860	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.190	67	144947	23.150	ng/u1	0.00
11) 2-Chlorophenol-d4	7.395	132	161700	22.262	ng/u1	0.00
15) 4-Methylphenol-d8	8.578	113	160611	21.883	ng/u1	0.00
21) Nitrobenzene-d5	9.025	128	76457	22.516	ng/u1	0.00
24) 2-Nitrophenol-d4	9.754	143	77136	21.819	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.295	165	144183	21.659	ng/u1	0.00
31) 4-Chloroaniline-d4	10.813	131	184276	20.065	ng/u1	0.00
46) Dimethylphthalate-d6	13.924	166	485463	24.682	ng/u1	0.00
49) Acenaphthylene-d8	14.207	160	570687	22.575	ng/u1	0.00
54) 4-Nitrophenol-d4	14.718	143	33053	11.021	ng/u1	0.00
60) Fluorene-d10	15.501	176	418251	24.607	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.624	200	59521	18.120	ng/u1	0.00
73) Anthracene-d10	17.354	188	616996	24.051	ng/u1	0.00
81) Pyrene-d10	19.642	212	728983	27.921	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.653	264	638490	23.742	ng/u1	0.00
Target Compounds						
8) Phenol	7.054	94	12985m	1.368	ng/u1	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034678.D
Acq On : 14 Apr 2022 21:38
Operator : CG/JU
Sample : N2316-05
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
ETNQ3

Quant Time: Apr 14 23:45:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 14 23:42:00 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/23/2022

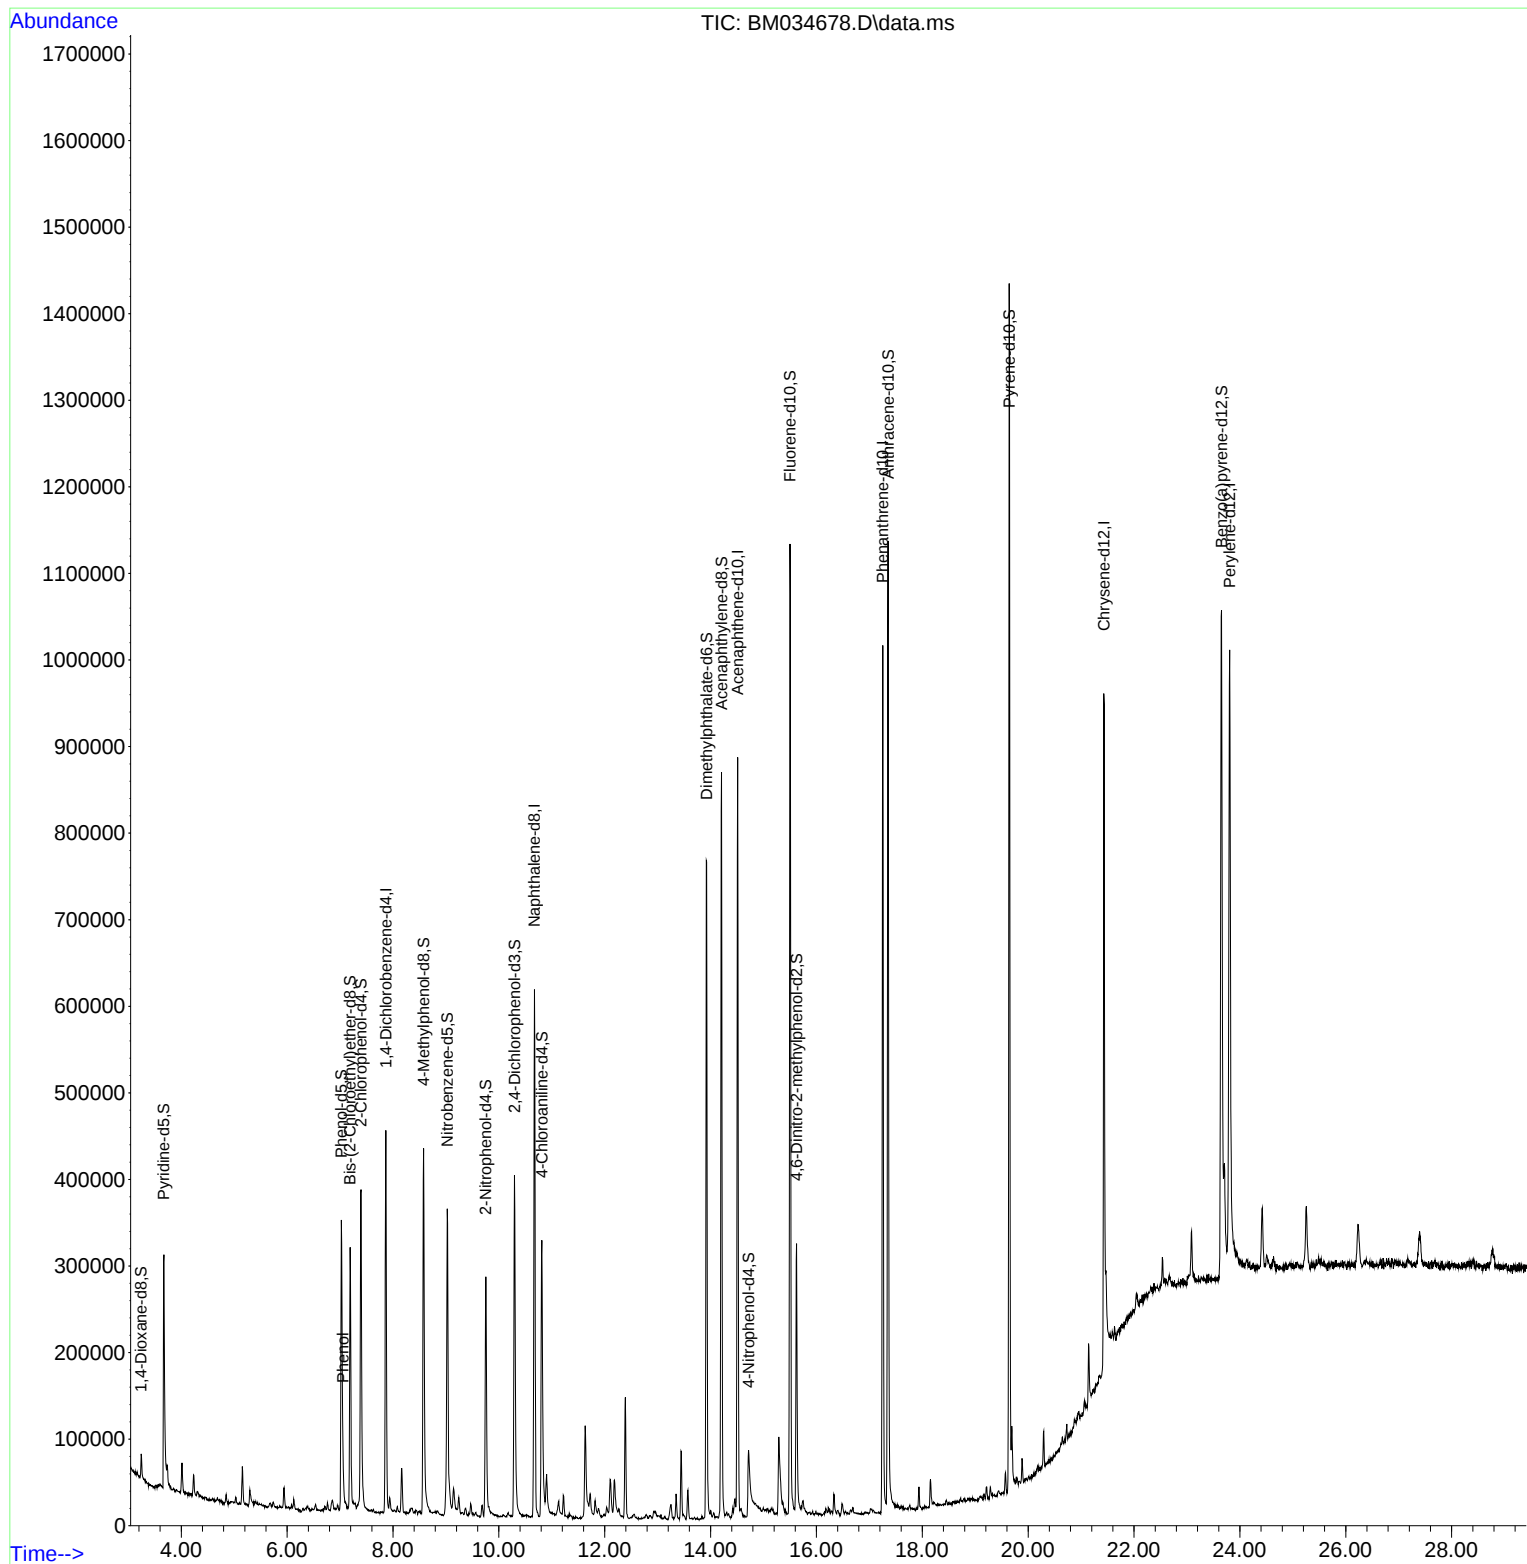

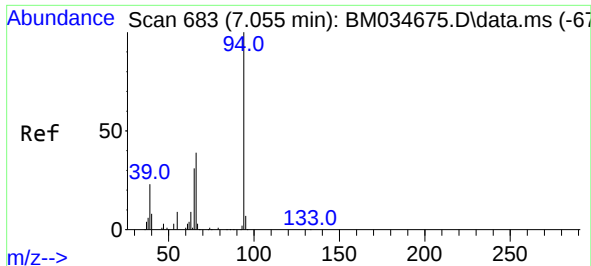

#8
Phenol
Concen: 1.368 ng/ul m
RT: 7.054 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM034678.D
Acq: 14 Apr 2022 21:38

Instrument :
BNA_M
ClientSampleId :
ETNQ3

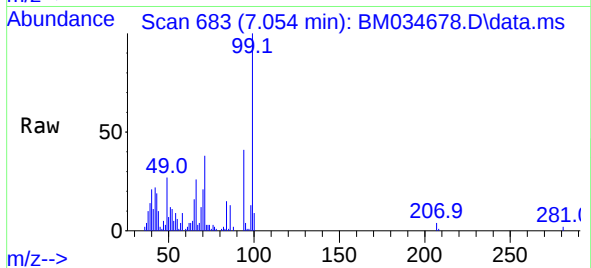

Tgt Ion: 94 Resp: 1298
Ion Ratio Lower Upper
94 100
65 39.0 22.9 34.3
66 64.5 33.7 50.5

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/15/2022
Supervised By :Yogesh Patel 04/23/2022

