

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034662.D
 Acq On : 14 Apr 2022 11:09
 Operator : CG/JU
 Sample : PB144063BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK063

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034662.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.249	33	36	42	rVB	42668	59456	2.34%	0.222%
2	3.672	105	108	124	rBV	421302	683438	26.87%	2.557%
3	4.013	163	166	173	rVB	20359	30729	1.21%	0.115%
4	7.031	673	679	700	rBV	448044	810832	31.88%	3.034%
5	7.195	700	707	720	rVV	411460	690214	27.13%	2.583%
6	7.395	735	741	758	rBV	538727	896223	35.23%	3.353%
7	7.866	815	821	831	rBV	387080	648671	25.50%	2.427%
8	8.578	936	942	959	rBV	561321	1010698	39.73%	3.782%
9	9.031	1012	1019	1032	rBV	476351	836240	32.87%	3.129%
10	9.760	1136	1143	1158	rBV	368845	667289	26.23%	2.497%
11	10.301	1228	1235	1251	rBV	497716	931028	36.60%	3.484%
12	10.678	1292	1299	1314	rVB	535187	913655	35.92%	3.419%
13	10.813	1316	1322	1334	rBV	375238	815646	32.06%	3.052%
14	10.983	1349	1351	1354	rVB4	2990	3443	0.14%	0.013%
15	12.307	1571	1576	1583	rBV6	6003	12334	0.48%	0.046%
16	13.924	1845	1851	1862	rBV	991678	1475773	58.02%	5.522%
17	14.007	1862	1865	1874	rVB4	6149	13323	0.52%	0.050%
18	14.207	1891	1899	1914	rBV	1097414	1683699	66.19%	6.300%
19	14.307	1914	1916	1923	rVV7	6225	13057	0.51%	0.049%
20	14.366	1923	1926	1931	rVB5	2024	4092	0.16%	0.015%
21	14.513	1945	1951	1964	rBV	754889	1132375	44.52%	4.237%
22	14.718	1980	1986	2001	rBV2	74185	256941	10.10%	0.961%
23	15.507	2111	2120	2134	rBV	1482274	2105582	82.78%	7.879%
24	15.624	2134	2140	2157	rVV	379340	650949	25.59%	2.436%
25	15.748	2157	2161	2166	rVB2	14413	23673	0.93%	0.089%
26	16.289	2250	2253	2258	rBV7	4039	6357	0.25%	0.024%
27	16.942	2361	2364	2367	rBV5	2115	3099	0.12%	0.012%
28	17.054	2376	2383	2388	rBV7	3637	9040	0.36%	0.034%
29	17.112	2390	2393	2397	rBV5	2075	2660	0.10%	0.010%
30	17.259	2411	2418	2426	rBV	828341	1238120	48.67%	4.633%
31	17.354	2428	2434	2450	rVV2	1396529	2152641	84.63%	8.055%
32	18.242	2581	2585	2586	rBV4	2724	3513	0.14%	0.013%
33	19.218	2747	2751	2755	rBV3	16479	24338	0.96%	0.091%
34	19.289	2760	2763	2768	rVV2	12083	16342	0.64%	0.061%
35	19.648	2818	2824	2846	rBV	1751390	2543733	100.00%	9.518%
36	21.436	3124	3128	3134	rBV	533665	907384	35.67%	3.395%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034662.D
Acq On : 14 Apr 2022 11:09
Operator : CG/JU
Sample : PB144063BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK063

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Title : SVOA CALIBRATION

37	23.659	3499	3506	3523	rBV	932945	2289407	90.00%	8.566%
38	23.812	3526	3532	3543	rVB2	530506	1159204	45.57%	4.337%




Sum of corrected areas: 26725198

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034662.D
Acq On : 14 Apr 2022 11:09
Operator : CG/JU
Sample : PB144063BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK063

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

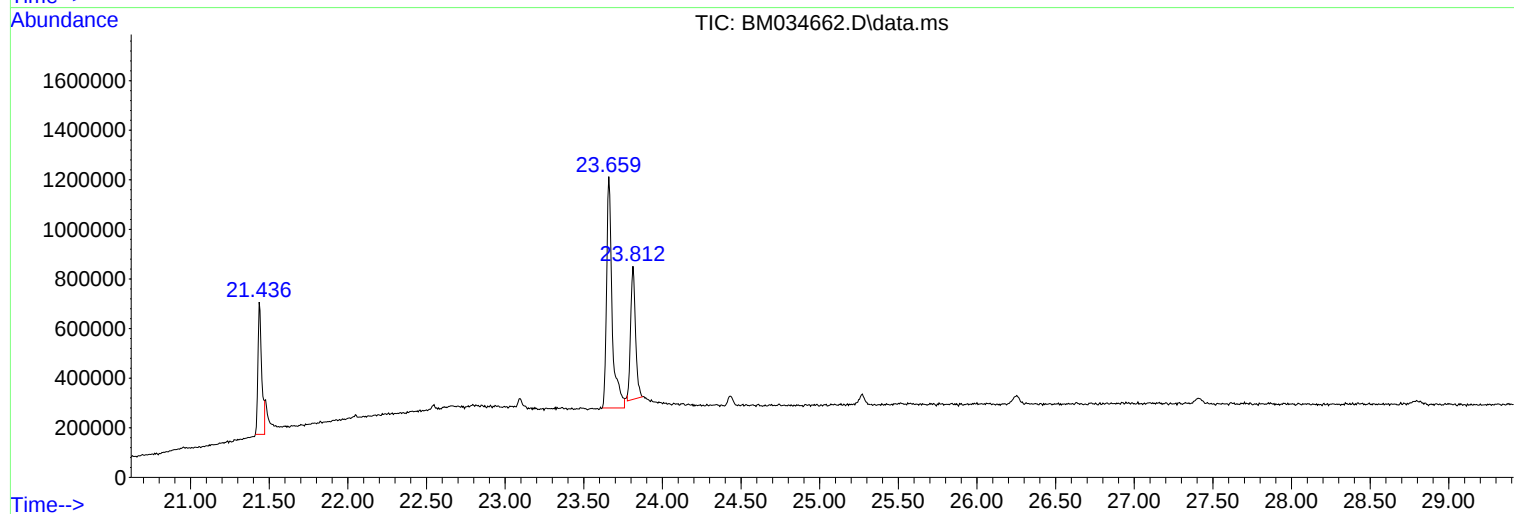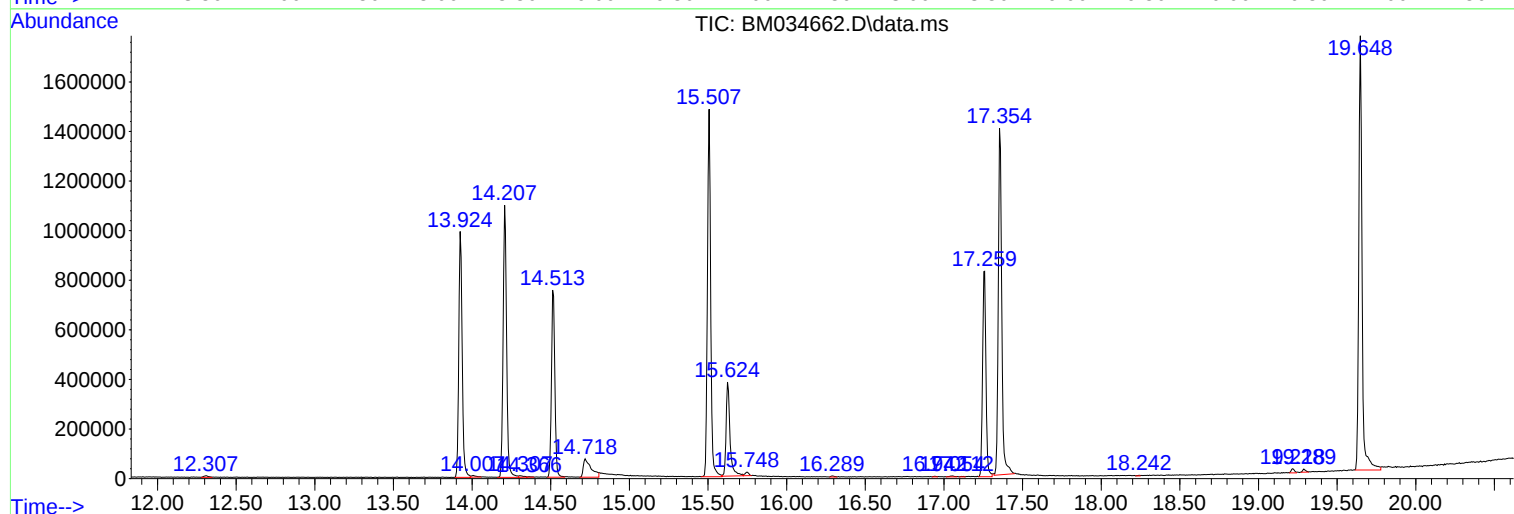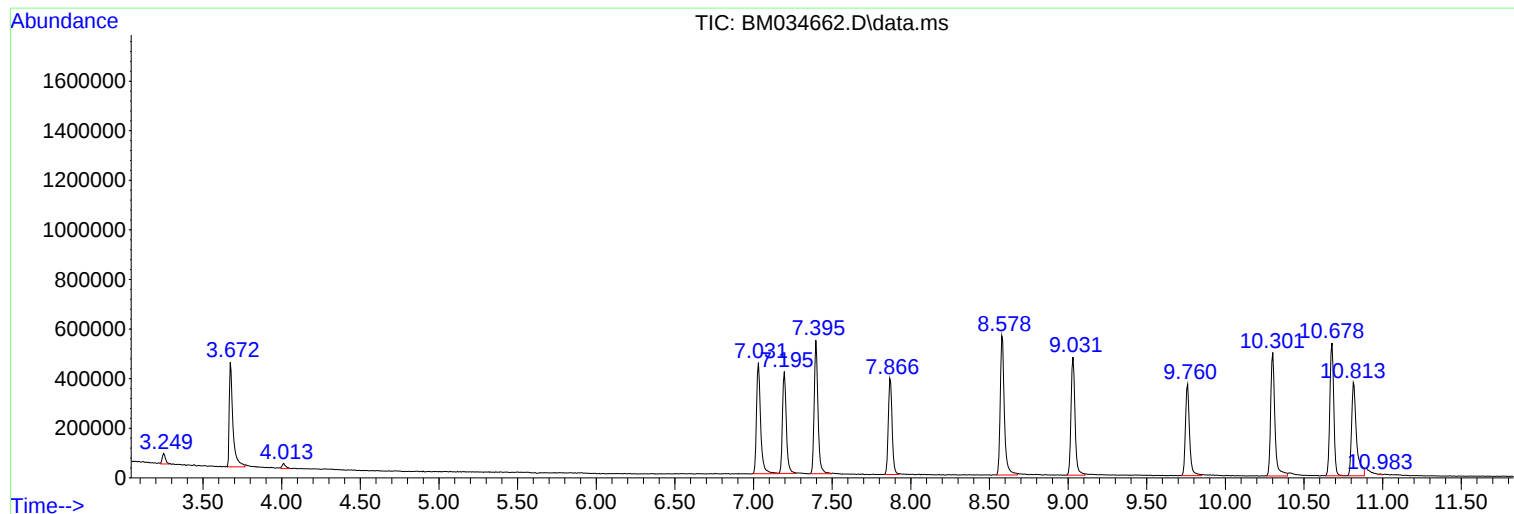

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034662.D
Acq On : 14 Apr 2022 11:09
Operator : CG/JU
Sample : PB144063BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK063

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034662.D
Acq On : 14 Apr 2022 11:09
Operator : CG/JU
Sample : PB144063BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK063

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc