

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034664.D
 Acq On : 14 Apr 2022 12:27
 Operator : CG/JU
 Sample : N2342-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0J09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034664.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.249	33	36	44	rVB2	33381	47670	1.58%	0.169%
2	3.678	106	109	120	rBV	144360	243824	8.10%	0.862%
3	5.160	357	361	367	rBV2	12131	20630	0.69%	0.073%
4	7.031	674	679	692	rBV	89657	182977	6.08%	0.647%
5	7.195	701	707	721	rBV	410750	687140	22.82%	2.430%
6	7.395	735	741	753	rBV	413594	716790	23.80%	2.535%
7	7.866	815	821	832	rBV	450225	766327	25.45%	2.710%
8	7.937	832	833	841	rVB5	7869	12519	0.42%	0.044%
9	8.225	878	882	887	rBV2	7445	12175	0.40%	0.043%
10	8.584	935	943	954	rBV	290785	551292	18.31%	1.950%
11	9.031	1011	1019	1033	rBV	490226	857199	28.47%	3.031%
12	9.478	1090	1095	1100	rVB2	9685	14654	0.49%	0.052%
13	9.760	1136	1143	1155	rBV	356597	656742	21.81%	2.322%
14	10.301	1228	1235	1250	rBV	469876	882606	29.31%	3.121%
15	10.548	1273	1277	1279	rBV5	3798	4689	0.16%	0.017%
16	10.678	1291	1299	1310	rBV	625114	1057683	35.12%	3.740%
17	10.813	1315	1322	1347	rBV	339310	804827	26.73%	2.846%
18	12.136	1543	1547	1551	rBV6	4102	6361	0.21%	0.022%
19	12.230	1562	1563	1568	rBV4	2447	4044	0.13%	0.014%
20	12.301	1571	1575	1580	rVV4	4766	9665	0.32%	0.034%
21	12.930	1677	1682	1689	rVB7	2702	5271	0.18%	0.019%
22	13.354	1748	1754	1763	rVB3	10630	17394	0.58%	0.062%
23	13.924	1845	1851	1863	rBV	1066235	1545381	51.32%	5.465%
24	14.207	1892	1899	1914	rBV	1180197	1752163	58.18%	6.196%
25	14.513	1944	1951	1962	rBV	898509	1312029	43.57%	4.640%
26	14.589	1962	1964	1969	rVB5	1777	3144	0.10%	0.011%
27	14.748	1987	1991	1994	rBV6	6452	10189	0.34%	0.036%
28	14.777	1994	1996	1999	rVB4	2935	3983	0.13%	0.014%
29	14.854	2007	2009	2015	rVB6	1743	3342	0.11%	0.012%
30	15.318	2085	2088	2093	rVB5	1973	3188	0.11%	0.011%
31	15.507	2113	2120	2134	rBV	1542924	2288529	76.00%	8.093%
32	15.624	2134	2140	2157	rVV	461628	745266	24.75%	2.635%
33	15.748	2157	2161	2170	rVB2	17352	31900	1.06%	0.113%
34	16.295	2250	2254	2260	rBV6	4997	7732	0.26%	0.027%
35	17.048	2373	2382	2385	rBV4	4085	8296	0.28%	0.029%
36	17.259	2412	2418	2427	rBV	959756	1413635	46.94%	4.999%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034664.D
 Acq On : 14 Apr 2022 12:27
 Operator : CG/JU
 Sample : N2342-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0J09

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	17.354	2428	2434	2451	rVV2	1676142	2543430	84.46%	8.994%
38	17.942	2531	2534	2538	rBV3	3856	5108	0.17%	0.018%
39	18.159	2566	2571	2578	rBV5	22729	50527	1.68%	0.179%
40	19.218	2747	2751	2755	rBV2	19114	24798	0.82%	0.088%
41	19.289	2759	2763	2767	rBV3	17175	22276	0.74%	0.079%
42	19.648	2818	2824	2837	rBV	2138018	3011396	100.00%	10.649%
43	21.147	3075	3079	3084	rBV2	72552	117534	3.90%	0.416%
44	21.436	3123	3128	3145	rBV	719509	1392392	46.24%	4.924%
45	23.653	3498	3505	3522	rBV2	1242036	2890662	95.99%	10.222%
46	23.806	3525	3531	3545	rVB2	703145	1528895	50.77%	5.407%




Sum of corrected areas: 28278274

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034664.D
Acq On : 14 Apr 2022 12:27
Operator : CG/JU
Sample : N2342-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

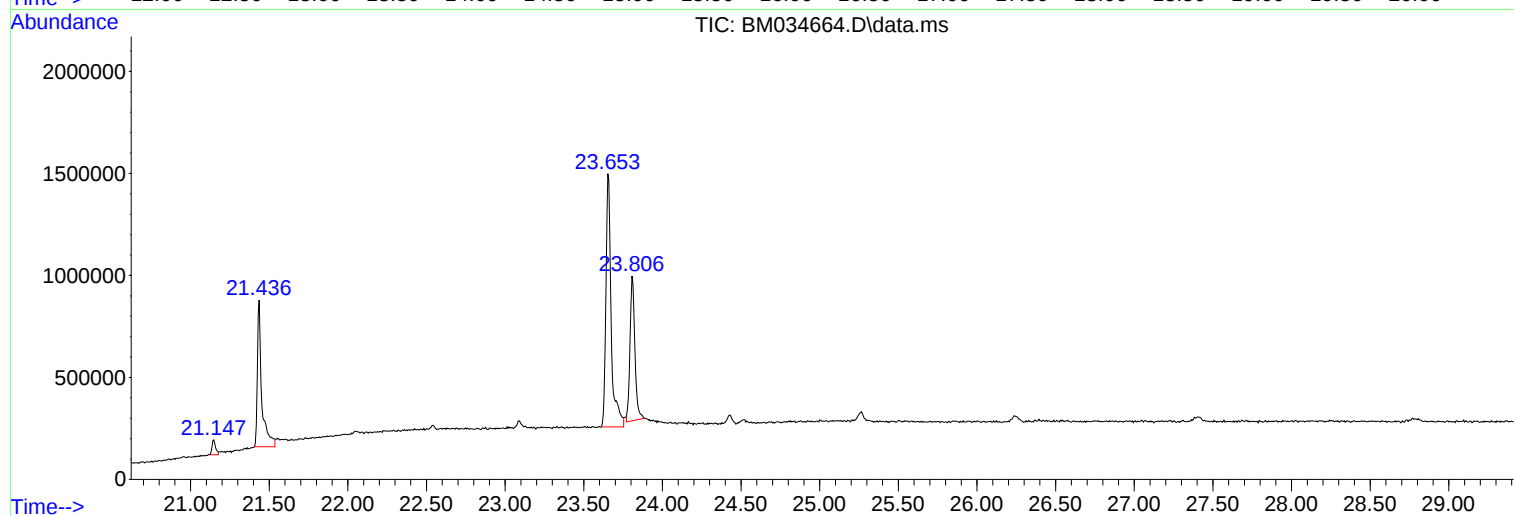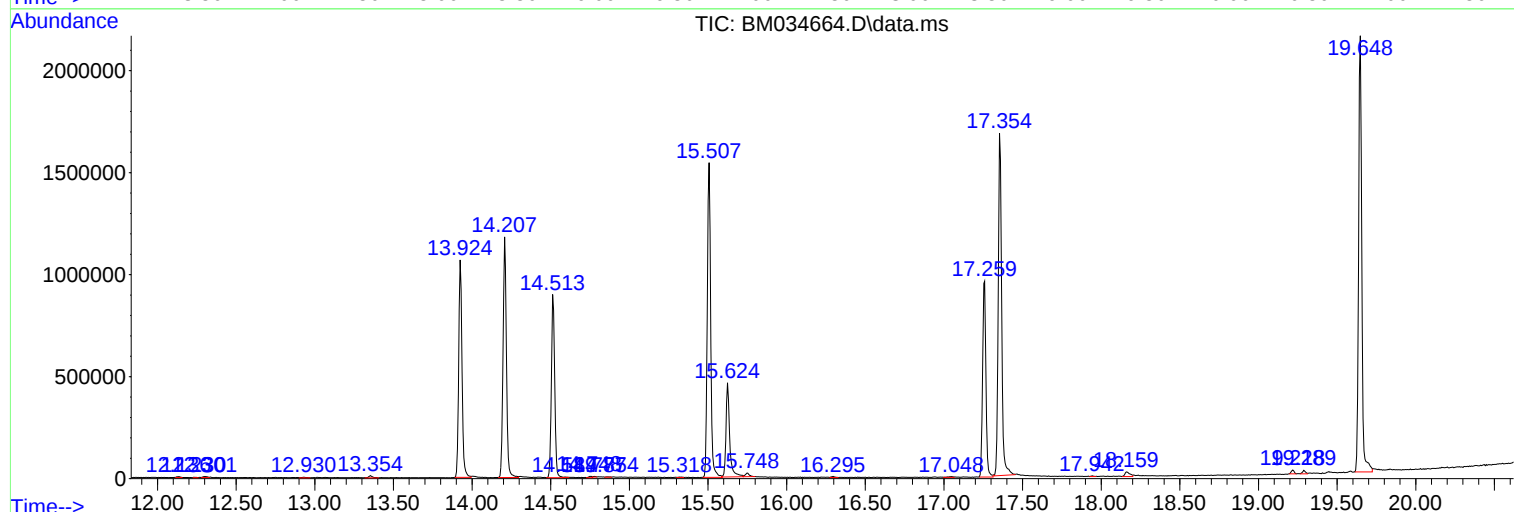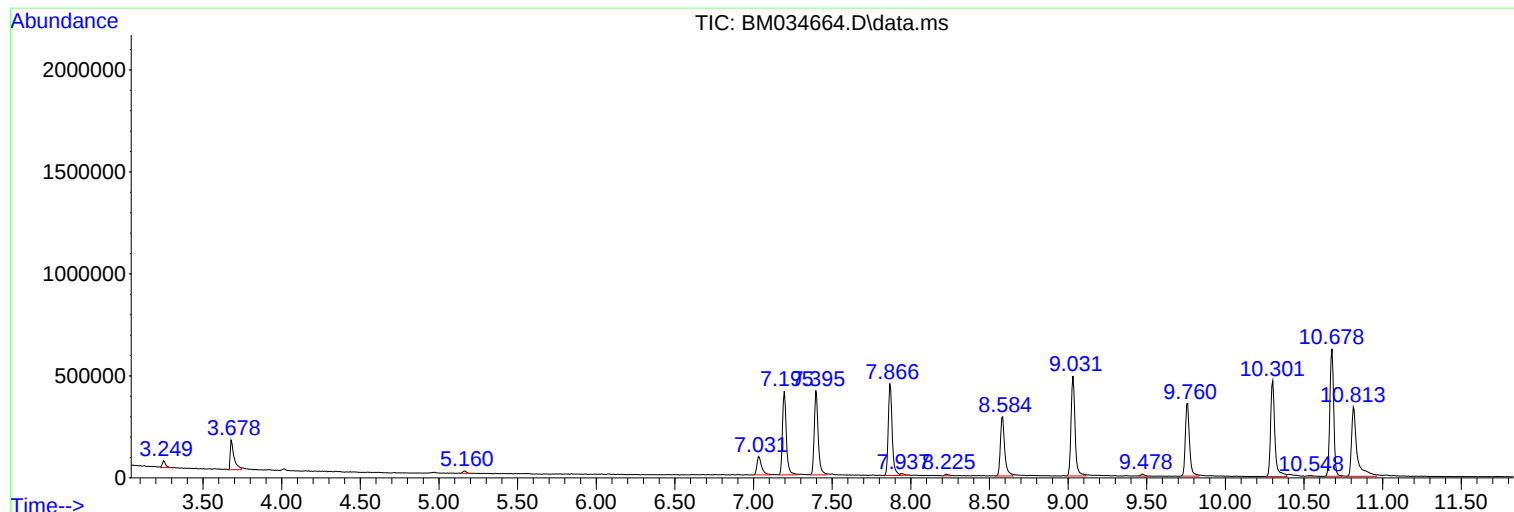

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034664.D
Acq On : 14 Apr 2022 12:27
Operator : CG/JU
Sample : N2342-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034664.D
Acq On : 14 Apr 2022 12:27
Operator : CG/JU
Sample : N2342-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0J09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc