

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034666.D
 Acq On : 14 Apr 2022 13:40
 Operator : CG/JU
 Sample : N2266-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAZ00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034666.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.249	33	36	41	rVB	38624	48759	1.60%	0.170%
2	3.678	107	109	131	rVB	128672	242594	7.94%	0.844%
3	6.860	648	650	658	rVB6	4523	8300	0.27%	0.029%
4	7.031	673	679	691	rBV	92369	189518	6.20%	0.659%
5	7.195	701	707	718	rBV	459019	754831	24.69%	2.625%
6	7.395	735	741	756	rBV	460310	788486	25.79%	2.742%
7	7.866	815	821	832	rBV	404946	672235	21.99%	2.337%
8	7.948	832	835	842	rVB6	5340	11021	0.36%	0.038%
9	8.107	859	862	869	rVB6	7361	12861	0.42%	0.045%
10	8.360	903	905	910	rVB5	2173	3152	0.10%	0.011%
11	8.425	912	916	920	rBV4	4186	6627	0.22%	0.023%
12	8.578	936	942	958	rVV	308234	581908	19.04%	2.023%
13	9.031	1012	1019	1032	rBV	551486	942018	30.82%	3.275%
14	9.472	1089	1094	1103	rVB2	18469	30093	0.98%	0.105%
15	9.760	1135	1143	1158	rBV	404332	745925	24.40%	2.594%
16	10.301	1228	1235	1252	rBV	513959	977688	31.98%	3.400%
17	10.677	1291	1299	1308	rBV	533282	913565	29.89%	3.177%
18	10.813	1316	1322	1349	rBV	360435	855668	27.99%	2.975%
19	11.977	1516	1520	1523	rVB3	3741	5034	0.16%	0.018%
20	12.124	1538	1545	1553	rVB5	7873	15971	0.52%	0.056%
21	12.301	1568	1575	1585	rVB5	6627	16771	0.55%	0.058%
22	12.924	1679	1681	1687	rBV4	2645	4053	0.13%	0.014%
23	13.066	1703	1705	1710	rVB5	2705	3731	0.12%	0.013%
24	13.354	1748	1754	1760	rVB3	13217	21780	0.71%	0.076%
25	13.924	1845	1851	1864	rBV	1203801	1738465	56.87%	6.045%
26	14.007	1864	1865	1878	rVB5	7042	11760	0.38%	0.041%
27	14.207	1890	1899	1913	rBV	1358185	1960255	64.13%	6.816%
28	14.512	1944	1951	1964	rBV	738146	1131383	37.01%	3.934%
29	14.748	1986	1991	1993	rBV4	8599	11570	0.38%	0.040%
30	14.924	2017	2021	2025	rVB6	2062	3666	0.12%	0.013%
31	15.507	2113	2120	2134	rBV	1697009	2516887	82.34%	8.751%
32	15.624	2134	2140	2157	rVV	485505	815989	26.69%	2.837%
33	15.748	2157	2161	2179	rVB	21681	53937	1.76%	0.188%
34	16.289	2250	2253	2259	rVB8	6000	9612	0.31%	0.033%
35	16.942	2361	2364	2369	rVB4	2636	3066	0.10%	0.011%
36	17.054	2379	2383	2385	rBV5	3510	5073	0.17%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034666.D
 Acq On : 14 Apr 2022 13:40
 Operator : CG/JU
 Sample : N2266-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAZ00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	17.253	2411	2417	2427	rBV	833914	1224895	40.07%	4.259%
38	17.353	2428	2434	2459	rVB	1732177	2668491	87.30%	9.279%
39	17.936	2530	2533	2538	rVB6	2981	5171	0.17%	0.018%
40	18.159	2567	2571	2580	rBV4	28945	60323	1.97%	0.210%
41	18.665	2652	2657	2660	rBV7	2440	5233	0.17%	0.018%
42	19.218	2747	2751	2757	rBV2	21197	31100	1.02%	0.108%
43	19.283	2759	2762	2766	rBV	15685	22046	0.72%	0.077%
44	19.436	2786	2788	2790	rBV3	7078	7024	0.23%	0.024%
45	19.577	2810	2812	2816	rVB5	7095	6908	0.23%	0.024%
46	19.647	2818	2824	2831	rBV	2219596	3056763	100.00%	10.629%
47	21.147	3075	3079	3085	rBV3	118095	171016	5.59%	0.595%
48	21.436	3123	3128	3134	rBV	639090	1017881	33.30%	3.539%
49	22.612	3325	3328	3333	rVB2	75712	101607	3.32%	0.353%
50	23.659	3499	3506	3523	rBV2	1254196	2911113	95.24%	10.122%
51	23.812	3526	3532	3546	rVB2	612795	1355718	44.35%	4.714%




Sum of corrected areas: 28759541

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034666.D
Acq On : 14 Apr 2022 13:40
Operator : CG/JU
Sample : N2266-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ00

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

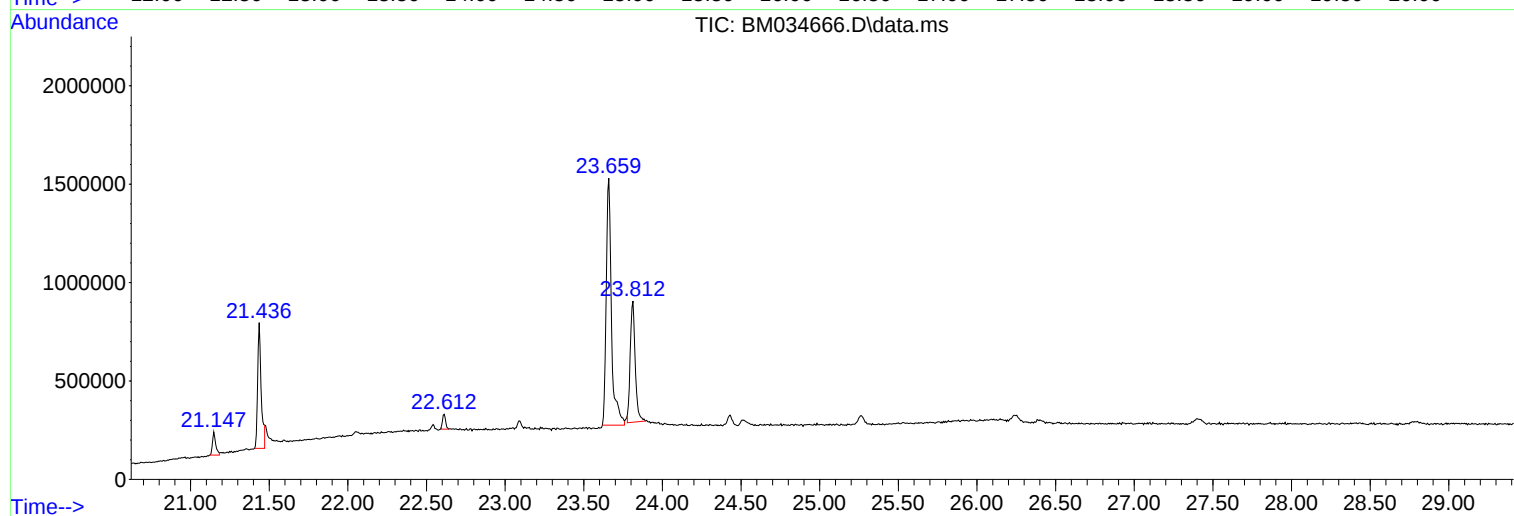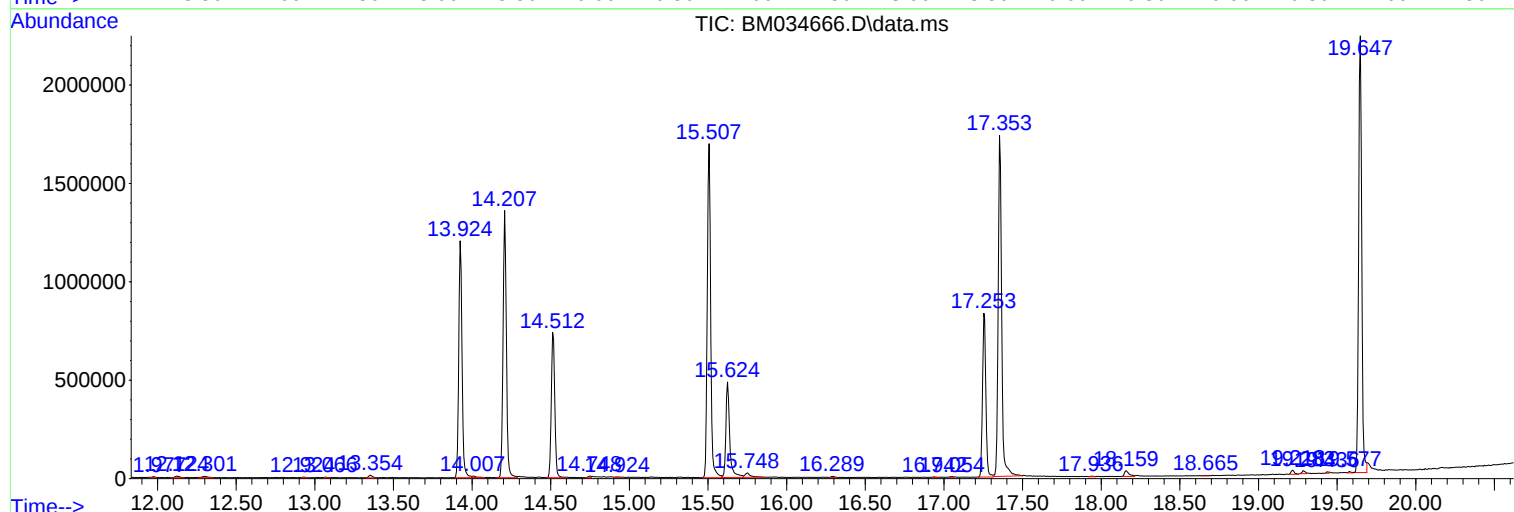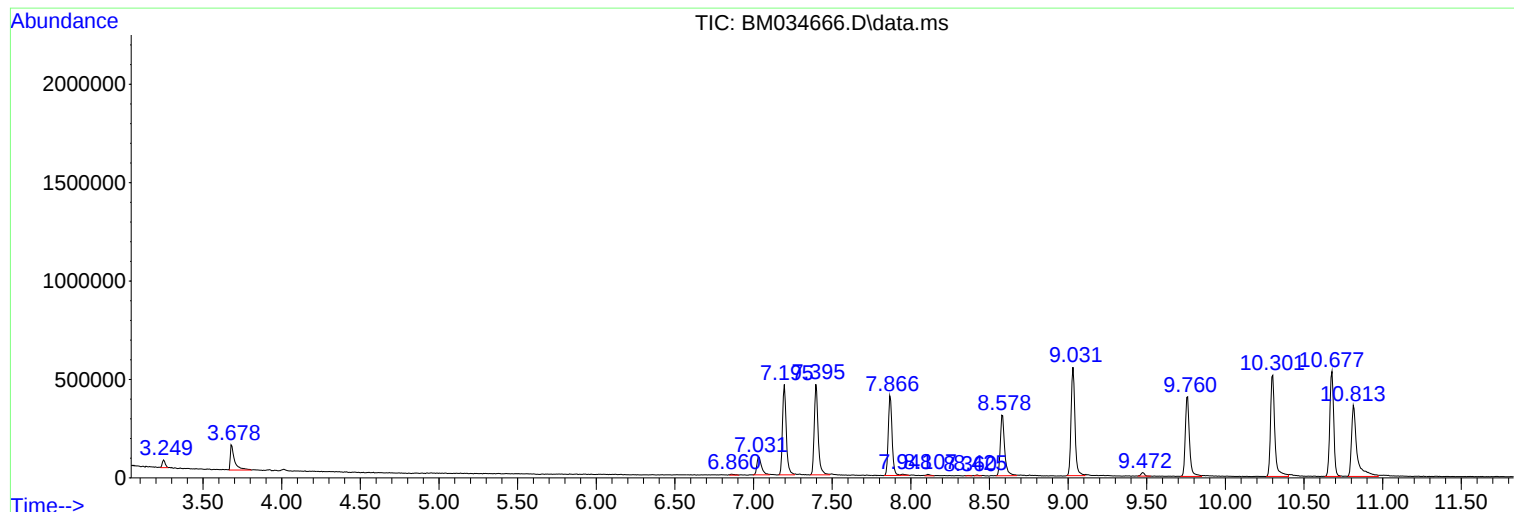

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034666.D
Acq On : 14 Apr 2022 13:40
Operator : CG/JU
Sample : N2266-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ00










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.147 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.147	3.36 ng/ul	171016	Chrysene-d12	21.436

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentadecane	210	C15H30	000295-48-7	95
2			1-Heneicosanol	312	C21H44O	015594-90-8	95
3			Nonacos-1-ene	406	C29H58	018835-35-3	94
4			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
5			Pentacos-1-ene	350	C25H50	016980-85-1	94

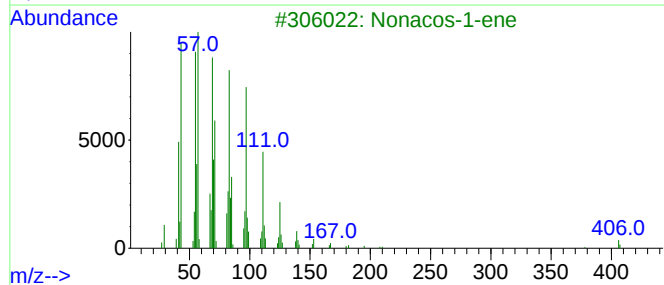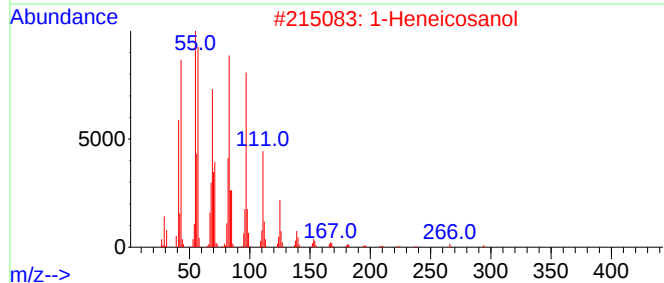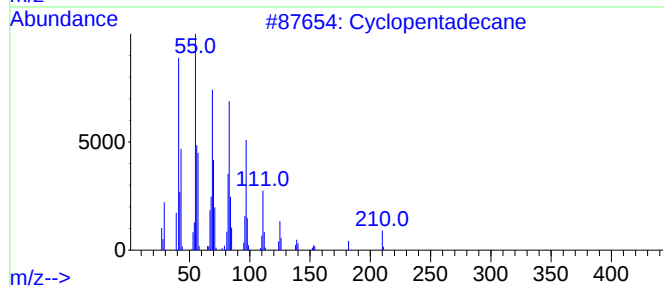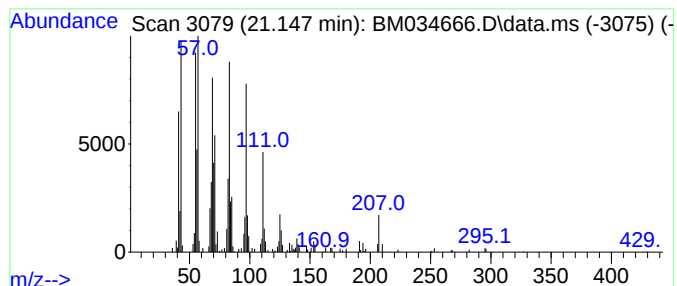

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034666.D
Acq On : 14 Apr 2022 13:40
Operator : CG/JU
Sample : N2266-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAZ00

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	21.147	3.4	ng/ul	171016	5	21.436	1017880	20.0