

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034671.D
 Acq On : 14 Apr 2022 16:44
 Operator : CG/JU
 Sample : N2266-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAYW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.249	32	36	44	rVB	41526	59958	2.11%	0.215%
2	3.678	106	109	122	rBV	120198	203780	7.16%	0.732%
3	4.007	163	165	174	rVB	11388	15078	0.53%	0.054%
4	6.866	646	651	654	rBV6	4254	7034	0.25%	0.025%
5	7.031	674	679	697	rVB	102590	208705	7.33%	0.750%
6	7.195	701	707	719	rBV	419442	700712	24.62%	2.518%
7	7.395	735	741	755	rBV	436020	746690	26.24%	2.683%
8	7.490	755	757	765	rVB6	5582	9736	0.34%	0.035%
9	7.866	815	821	831	rBV	429076	718491	25.25%	2.582%
10	7.942	832	834	839	rVB5	5543	8212	0.29%	0.030%
11	8.107	857	862	869	rVB4	8160	16374	0.58%	0.059%
12	8.419	911	915	919	rVV7	2746	4999	0.18%	0.018%
13	8.578	934	942	963	rBV	318383	618572	21.74%	2.223%
14	9.031	1012	1019	1034	rBV	499641	875825	30.78%	3.148%
15	9.472	1090	1094	1102	rVB	15694	25741	0.90%	0.093%
16	9.760	1135	1143	1160	rBV	367762	698612	24.55%	2.511%
17	10.301	1227	1235	1251	rBV	477842	917804	32.25%	3.298%
18	10.678	1291	1299	1308	rBV	594078	1001380	35.19%	3.599%
19	10.813	1315	1322	1352	rBV	302443	753729	26.49%	2.709%
20	11.978	1514	1520	1527	rVB3	8423	14220	0.50%	0.051%
21	12.119	1535	1544	1551	rBV3	9284	19465	0.68%	0.070%
22	12.289	1569	1573	1578	rBV4	5183	10281	0.36%	0.037%
23	12.748	1646	1651	1655	rBV5	2325	4244	0.15%	0.015%
24	12.795	1655	1659	1665	rVB7	2559	3636	0.13%	0.013%
25	12.930	1677	1682	1684	rVB5	2910	3585	0.13%	0.013%
26	13.013	1692	1696	1702	rBV6	2637	4858	0.17%	0.017%
27	13.066	1702	1705	1708	rVV3	3198	3686	0.13%	0.013%
28	13.354	1748	1754	1762	rVB2	16507	27189	0.96%	0.098%
29	13.807	1828	1831	1836	rVB4	2300	3724	0.13%	0.013%
30	13.924	1845	1851	1863	rVV	1092360	1582526	55.61%	5.687%
31	14.007	1863	1865	1871	rVV3	7825	12632	0.44%	0.045%
32	14.207	1891	1899	1911	rBV	1215982	1785088	62.73%	6.415%
33	14.313	1914	1917	1922	rVB6	3851	6703	0.24%	0.024%
34	14.513	1944	1951	1961	rBV	809441	1224902	43.05%	4.402%
35	14.748	1985	1991	1998	rBV9	10491	29106	1.02%	0.105%
36	15.324	2083	2089	2092	rBV6	3786	7091	0.25%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034671.D
 Acq On : 14 Apr 2022 16:44
 Operator : CG/JU
 Sample : N2266-14
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAYW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	15.507	2113	2120	2134	rBV	1547969	2316774	81.42%	8.326%
38	15.624	2134	2140	2153	rVV	463496	753824	26.49%	2.709%
39	15.748	2156	2161	2170	rVV	22274	47097	1.66%	0.169%
40	15.813	2170	2172	2177	rVB6	2600	3551	0.12%	0.013%
41	16.207	2236	2239	2241	rBV2	2179	2854	0.10%	0.010%
42	16.301	2248	2255	2258	rVB7	5035	7802	0.27%	0.028%
43	16.554	2293	2298	2300	rBV6	2080	3787	0.13%	0.014%
44	16.942	2362	2364	2368	rVB5	2855	2871	0.10%	0.010%
45	17.048	2379	2382	2387	rBV5	2687	4337	0.15%	0.016%
46	17.260	2411	2418	2426	rBV	898262	1336399	46.96%	4.803%
47	17.354	2428	2434	2457	rVB2	1645173	2479350	87.13%	8.910%
48	17.942	2529	2534	2537	rVB7	4243	6587	0.23%	0.024%
49	18.154	2566	2570	2580	rBV5	24050	47764	1.68%	0.172%
50	18.906	2697	2698	2700	rBV2	3152	2895	0.10%	0.010%
51	19.218	2747	2751	2756	rVB3	19351	26150	0.92%	0.094%
52	19.289	2759	2763	2769	rVV	18112	25508	0.90%	0.092%
53	19.442	2784	2789	2795	rBV9	8211	17560	0.62%	0.063%
54	19.648	2818	2824	2831	rBV	2113227	2845577	100.00%	10.227%
55	21.148	3075	3079	3087	rBV3	86596	144908	5.09%	0.521%
56	21.436	3123	3128	3143	rBV	739966	1379437	48.48%	4.957%
57	23.653	3499	3505	3513	rBV2	1151077	2539527	89.24%	9.127%
58	23.812	3525	3532	3546	rVB2	697444	1496565	52.59%	5.378%




Sum of corrected areas: 27825492

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034671.D
Acq On : 14 Apr 2022 16:44
Operator : CG/JU
Sample : N2266-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAYW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

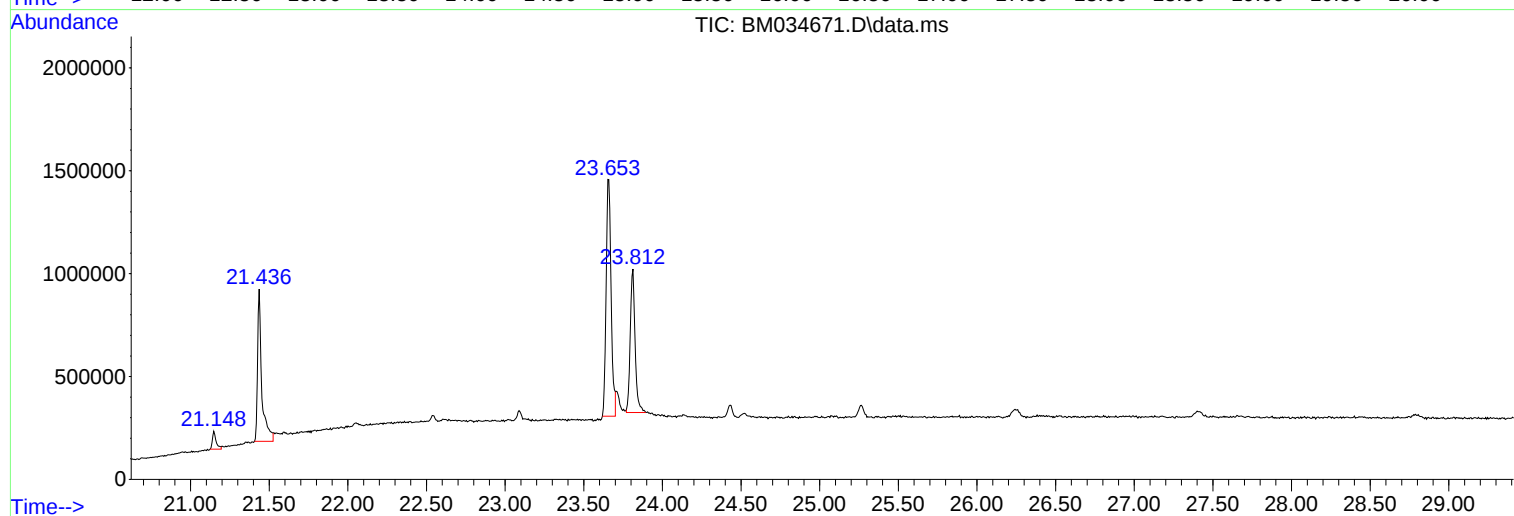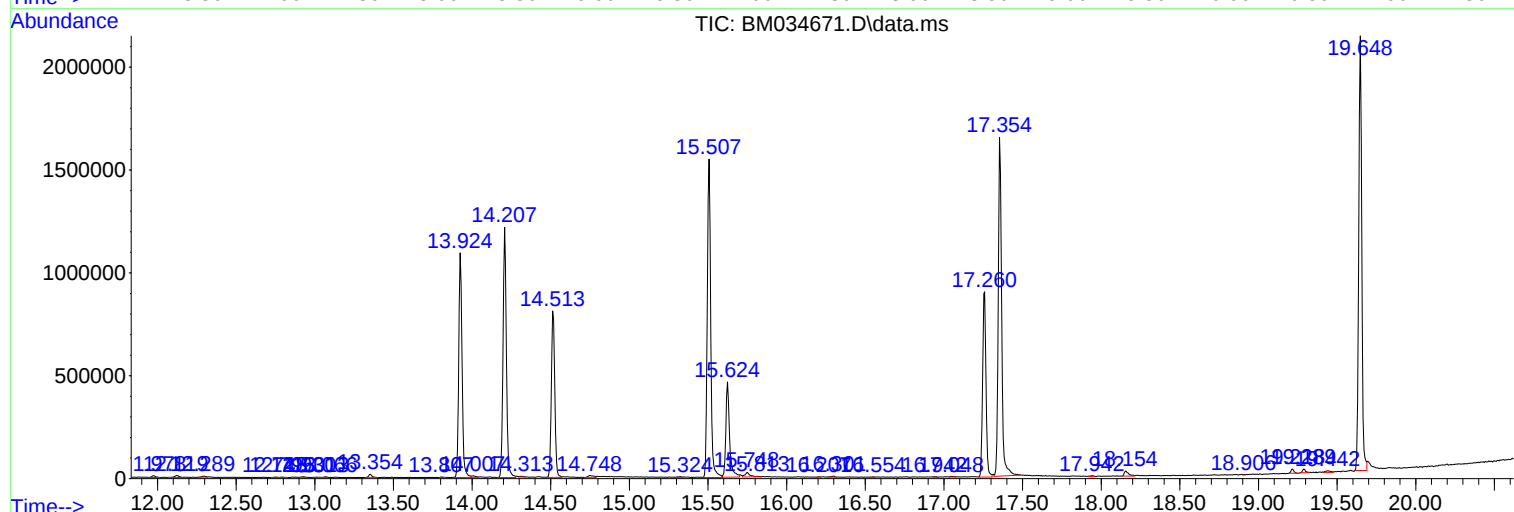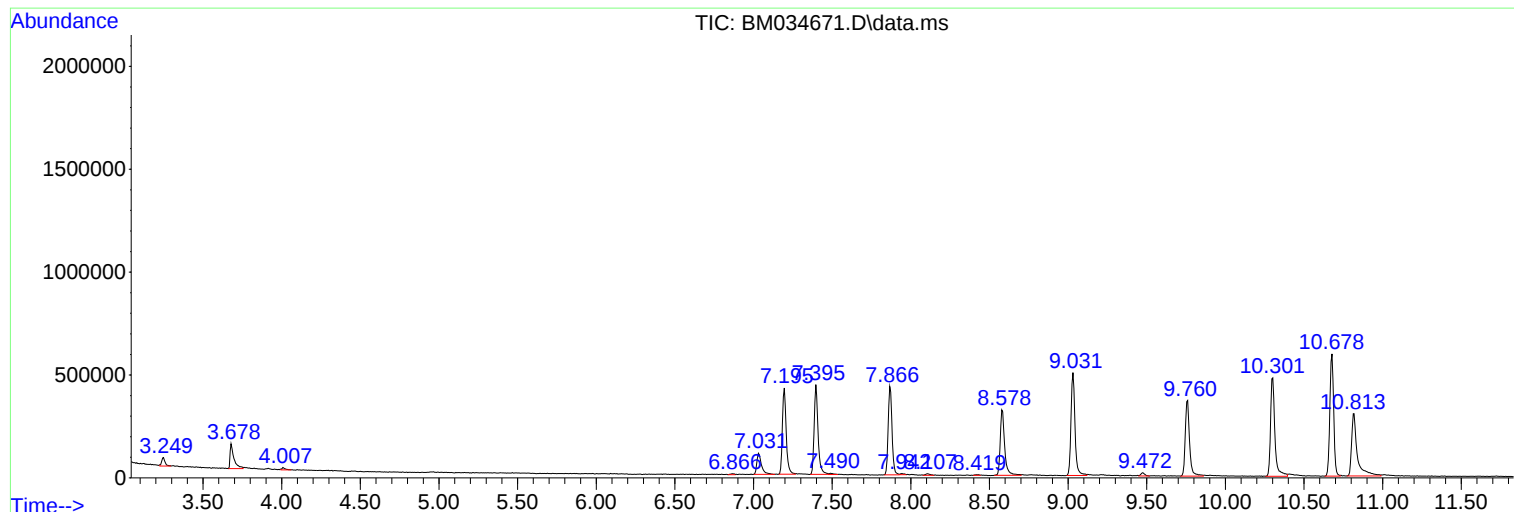

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034671.D
Acq On : 14 Apr 2022 16:44
Operator : CG/JU
Sample : N2266-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAYW6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trichloroacetic acid, hexad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.148	2.10 ng/ul	144908	Chrysene-d12	21.436

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	95
2		n-Tetracosanol-1	354	C24H50O	000506-51-4	94
3		Behenic alcohol	326	C22H46O	000661-19-8	94
4		Cyclotetracosane	336	C24H48	000297-03-0	93
5		1-Heneicosyl formate	340	C22H44O2	077899-03-7	91

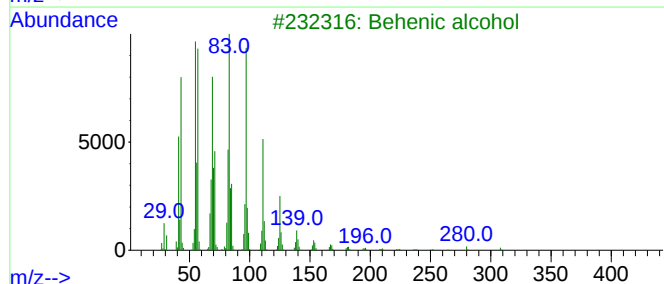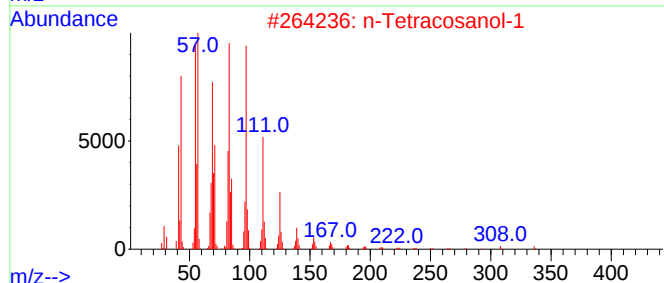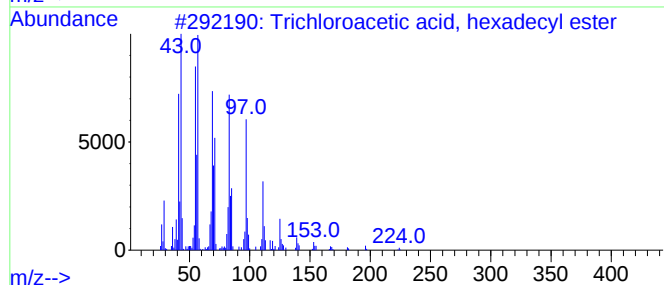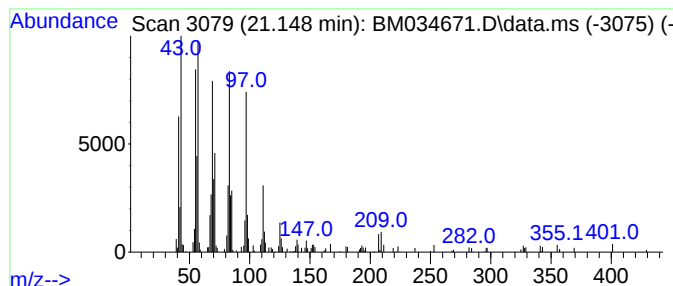

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034671.D
Acq On : 14 Apr 2022 16:44
Operator : CG/JU
Sample : N2266-14
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAYW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trichloroacetic...	21.148	2.1	ng/ul	144908	5	21.436	1379440	20.0