

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034676.D
 Acq On : 14 Apr 2022 20:25
 Operator : CG/JU
 Sample : PB144054BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK054

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034676.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.249	32	36	45	rVB	57882	79538	2.41%	0.216%
2	3.672	105	108	130	rBV	562811	866256	26.24%	2.352%
3	4.013	162	166	173	rVB	26165	37850	1.15%	0.103%
4	7.031	673	679	694	rBV	573024	1020452	30.91%	2.770%
5	7.195	700	707	719	rBV	525216	856129	25.94%	2.324%
6	7.395	735	741	754	rBV	676615	1110647	33.65%	3.015%
7	7.866	815	821	834	rBV	582825	949475	28.76%	2.578%
8	8.578	936	942	964	rBV	731688	1294038	39.20%	3.513%
9	9.031	1012	1019	1036	rBV	609125	1076415	32.61%	2.922%
10	9.754	1135	1142	1157	rBV	481040	874584	26.49%	2.374%
11	10.295	1227	1234	1250	rBV	655602	1205813	36.53%	3.273%
12	10.678	1290	1299	1310	rBV	801368	1376099	41.69%	3.736%
13	10.813	1315	1322	1335	rBV	523548	1087193	32.94%	2.951%
14	12.301	1570	1575	1584	rBV4	7501	15911	0.48%	0.043%
15	13.924	1845	1851	1863	rBV	1308141	1925819	58.34%	5.228%
16	14.207	1892	1899	1914	rBV	1495840	2208419	66.90%	5.995%
17	14.513	1945	1951	1963	rBV	1203528	1745285	52.87%	4.738%
18	14.713	1979	1985	2009	rBV	158741	497859	15.08%	1.352%
19	15.507	2112	2120	2134	rBV	1855900	2742504	83.08%	7.445%
20	15.624	2134	2140	2158	rVV	560698	924001	27.99%	2.508%
21	15.742	2158	2160	2173	rVB5	21938	41783	1.27%	0.113%
22	16.289	2249	2253	2259	rBV7	4459	8325	0.25%	0.023%
23	16.930	2361	2362	2368	rVB5	2581	3497	0.11%	0.009%
24	17.048	2378	2382	2386	rBV3	4690	5648	0.17%	0.015%
25	17.254	2411	2417	2426	rBV	1338832	1931092	58.50%	5.242%
26	17.354	2428	2434	2453	rVB2	1925460	2858427	86.59%	7.760%
27	17.830	2511	2515	2518	rVV5	2030	3543	0.11%	0.010%
28	19.212	2747	2750	2756	rBV	21499	28933	0.88%	0.079%
29	19.283	2759	2762	2768	rVB2	15052	20460	0.62%	0.056%
30	19.648	2818	2824	2839	rBV	2255406	3300941	100.00%	8.961%
31	21.430	3123	3127	3148	rBV	967960	1917883	58.10%	5.206%
32	23.653	3498	3505	3511	rBV2	1348656	2804234	84.95%	7.613%
33	23.806	3525	3531	3546	rVB2	914455	2017385	61.12%	5.477%




Sum of corrected areas: 36836438

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034676.D
Acq On : 14 Apr 2022 20:25
Operator : CG/JU
Sample : PB144054BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

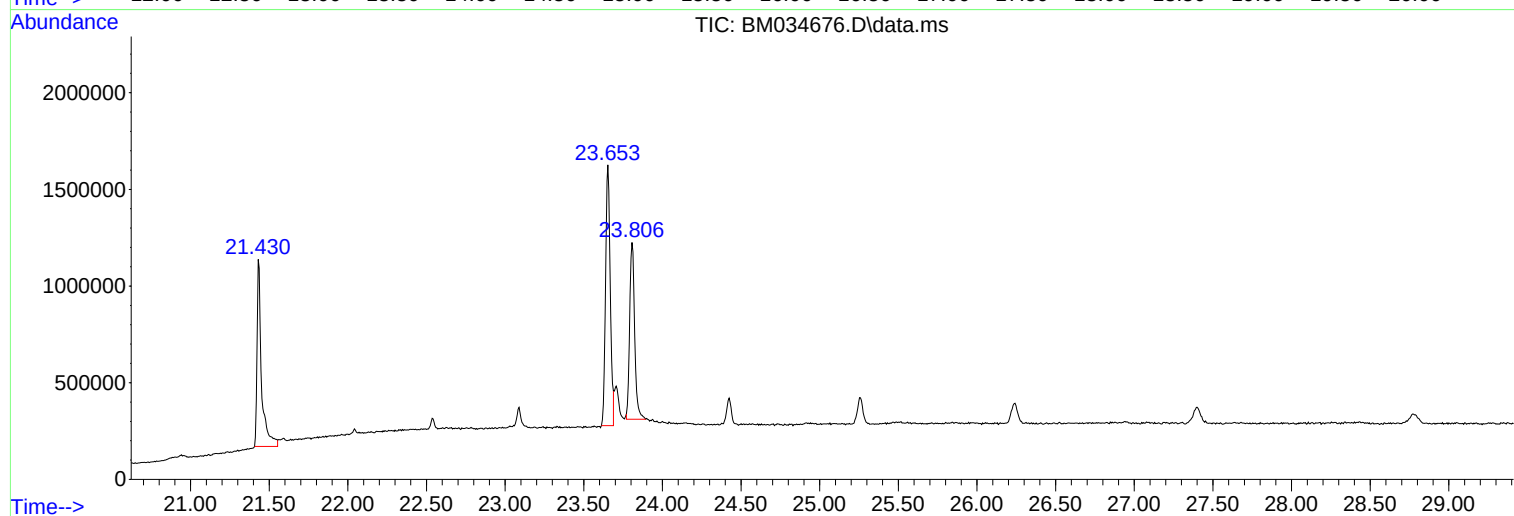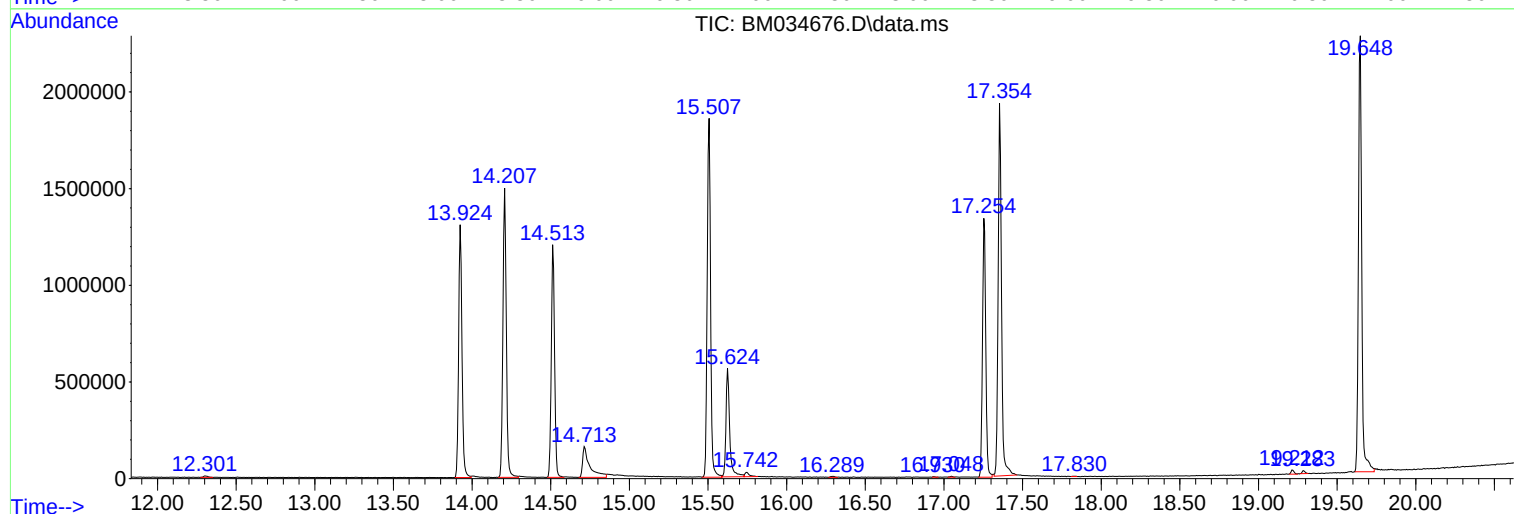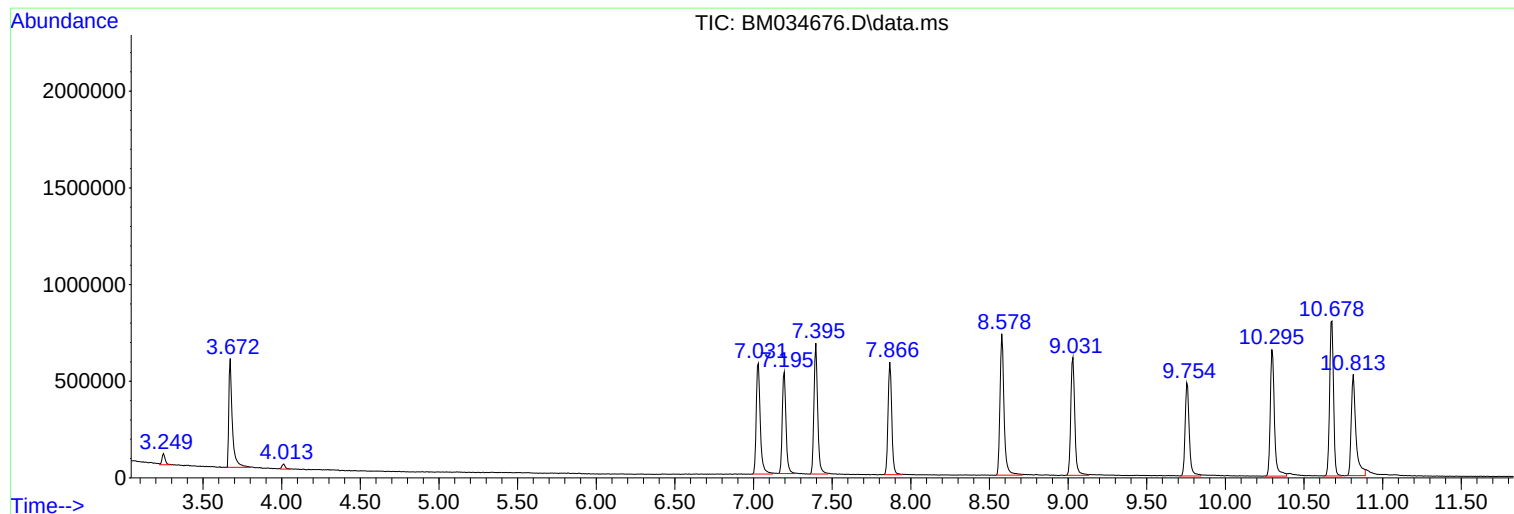

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034676.D
Acq On : 14 Apr 2022 20:25
Operator : CG/JU
Sample : PB144054BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034676.D
Acq On : 14 Apr 2022 20:25
Operator : CG/JU
Sample : PB144054BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------