

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034695.D
 Acq On : 15 Apr 2022 08:27
 Operator : CG/JU
 Sample : N2316-20
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETNR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034695.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.243	32	35	39	rBV	31693	37667	1.62%	0.132%
2	3.678	106	109	122	rBV	200654	408466	17.62%	1.434%
3	5.014	334	336	338	rVB2	3203	2379	0.10%	0.008%
4	5.155	354	360	366	rBV	37249	59232	2.55%	0.208%
5	7.031	672	679	694	rBV	373590	747448	32.24%	2.624%
6	7.190	700	706	719	rBV	363198	603258	26.02%	2.118%
7	7.390	734	740	753	rBV	457503	788028	33.99%	2.766%
8	7.860	814	820	831	rVV	452164	756234	32.62%	2.655%
9	7.937	831	833	840	rVB5	10878	17509	0.76%	0.061%
10	8.225	878	882	886	rBV7	2110	3310	0.14%	0.012%
11	8.413	912	914	917	rVB3	3047	2709	0.12%	0.010%
12	8.578	935	942	958	rBV	481375	901684	38.89%	3.165%
13	9.025	1011	1018	1032	rBV	424195	757787	32.68%	2.660%
14	9.366	1071	1076	1083	rBV8	7328	12922	0.56%	0.045%
15	9.466	1088	1093	1104	rVB	20201	36899	1.59%	0.130%
16	9.584	1110	1113	1115	rBV5	2022	2363	0.10%	0.008%
17	9.678	1126	1129	1130	rBV3	2992	3514	0.15%	0.012%
18	9.754	1135	1142	1157	rBV	304539	566612	24.44%	1.989%
19	10.043	1189	1191	1194	rVB3	2366	2894	0.12%	0.010%
20	10.066	1194	1195	1198	rBV3	2673	3339	0.14%	0.012%
21	10.149	1205	1209	1212	rBV6	1711	2447	0.11%	0.009%
22	10.296	1227	1234	1252	rBV	397303	863610	37.25%	3.031%
23	10.525	1272	1273	1278	rVB5	2426	2921	0.13%	0.010%
24	10.566	1278	1280	1285	rVB4	2963	3190	0.14%	0.011%
25	10.672	1291	1298	1314	rBV	621538	1073063	46.28%	3.767%
26	10.819	1316	1323	1349	rBV	159582	578645	24.96%	2.031%
27	11.225	1390	1392	1396	rVB5	2189	3075	0.13%	0.011%
28	11.713	1471	1475	1478	rVB6	2421	3243	0.14%	0.011%
29	11.819	1489	1493	1495	rVB4	1951	2530	0.11%	0.009%
30	11.966	1516	1518	1523	rVB5	2488	4162	0.18%	0.015%
31	12.107	1537	1542	1543	rBV5	9338	10949	0.47%	0.038%
32	12.195	1554	1557	1560	rVB5	1992	2627	0.11%	0.009%
33	12.237	1560	1564	1566	rBV5	2732	3491	0.15%	0.012%
34	12.290	1571	1573	1577	rVB5	4992	5560	0.24%	0.020%
35	12.401	1587	1592	1596	rVB6	5430	9335	0.40%	0.033%
36	12.742	1647	1650	1652	rBV4	3109	3631	0.16%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034695.D
 Acq On : 15 Apr 2022 08:27
 Operator : CG/JU
 Sample : N2316-20
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETNR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	12.784	1656	1657	1665	rVB8	3199	3902	0.17%	0.014%
38	12.919	1675	1680	1684	rVB7	4379	6785	0.29%	0.024%
39	13.060	1700	1704	1710	rBV5	5167	8765	0.38%	0.031%
40	13.131	1714	1716	1721	rVB6	2909	3396	0.15%	0.012%
41	13.342	1746	1752	1761	rVB2	25510	39656	1.71%	0.139%
42	13.448	1763	1770	1777	rBV	73908	115514	4.98%	0.405%
43	13.742	1814	1820	1822	rBV5	2085	3540	0.15%	0.012%
44	13.813	1826	1832	1834	rBV7	2779	5008	0.22%	0.018%
45	13.919	1844	1850	1862	rBV	897713	1396876	60.25%	4.903%
46	14.001	1862	1864	1868	rVB4	8575	10688	0.46%	0.038%
47	14.201	1889	1898	1913	rBV	1047929	1638280	70.66%	5.751%
48	14.295	1913	1914	1920	rVB5	9128	12982	0.56%	0.046%
49	14.419	1930	1935	1939	rBV3	10907	16330	0.70%	0.057%
50	14.466	1939	1943	1944	rBV3	2462	3118	0.13%	0.011%
51	14.513	1944	1951	1960	rVV	863155	1302492	56.18%	4.572%
52	14.642	1968	1973	1977	rVB6	6193	9344	0.40%	0.033%
53	14.748	1985	1991	1999	rBV2	32134	103560	4.47%	0.364%
54	15.307	2083	2086	2087	rBV3	2594	2855	0.12%	0.010%
55	15.366	2092	2096	2100	rVB5	6023	10362	0.45%	0.036%
56	15.419	2103	2105	2110	rVB5	2936	3312	0.14%	0.012%
57	15.501	2112	2119	2135	rBV	1308293	2063359	89.00%	7.243%
58	15.625	2135	2140	2156	rVV	129066	252578	10.89%	0.887%
59	15.748	2158	2161	2169	rVB4	15644	27899	1.20%	0.098%
60	15.925	2190	2191	2197	rVB6	4051	4778	0.21%	0.017%
61	16.189	2232	2236	2237	rBV4	3513	3876	0.17%	0.014%
62	16.225	2237	2242	2250	rVV10	5510	12247	0.53%	0.043%
63	16.289	2250	2253	2259	rVB8	5742	7362	0.32%	0.026%
64	16.407	2269	2273	2274	rBV4	3263	3902	0.17%	0.014%
65	16.495	2284	2288	2291	rVB5	5249	6581	0.28%	0.023%
66	16.648	2307	2314	2319	rVB8	6460	11166	0.48%	0.039%
67	16.719	2323	2326	2328	rVV4	2311	2890	0.12%	0.010%
68	16.748	2328	2331	2334	rVV4	3124	4259	0.18%	0.015%
69	16.936	2360	2363	2366	rBV5	2877	5088	0.22%	0.018%
70	17.254	2411	2417	2427	rBV	1005892	1480438	63.85%	5.197%
71	17.354	2427	2434	2451	rVV	1228229	2107298	90.89%	7.397%
72	17.477	2451	2455	2464	rVB9	17390	46390	2.00%	0.163%
73	17.936	2531	2533	2538	rVB5	5242	6639	0.29%	0.023%
74	18.154	2566	2570	2578	rBV6	26226	53493	2.31%	0.188%
75	18.589	2642	2644	2648	rBV5	3418	5318	0.23%	0.019%
76	19.213	2746	2750	2754	rBV6	14401	23573	1.02%	0.083%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
 Data File : BM034695.D
 Acq On : 15 Apr 2022 08:27
 Operator : CG/JU
 Sample : N2316-20
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETNR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

77	19.283	2759	2762	2765	rBV	10774	14309	0.62%	0.050%
78	19.442	2785	2789	2790	rBV3	5688	7590	0.33%	0.027%
79	19.642	2817	2823	2827	rBV	1706888	2318511	100.00%	8.138%
80	19.689	2827	2831	2845	rVB	793357	1233486	53.20%	4.330%
81	20.342	2940	2942	2947	rVB5	16853	17005	0.73%	0.060%
82	20.730	3005	3008	3011	rVB	40341	41480	1.79%	0.146%
83	21.148	3075	3079	3084	rBV2	81720	121557	5.24%	0.427%
84	21.430	3123	3127	3138	rBV	667150	1398317	60.31%	4.908%
85	21.712	3173	3175	3192	rVB	587314	1402427	60.49%	4.923%
86	23.654	3498	3505	3511	rBV2	649466	1519099	65.52%	5.332%
87	23.806	3525	3531	3548	rVB2	543106	1301969	56.16%	4.570%



Sum of corrected areas: 28488382

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034695.D
Acq On : 15 Apr 2022 08:27
Operator : CG/JU
Sample : N2316-20
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETNR8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

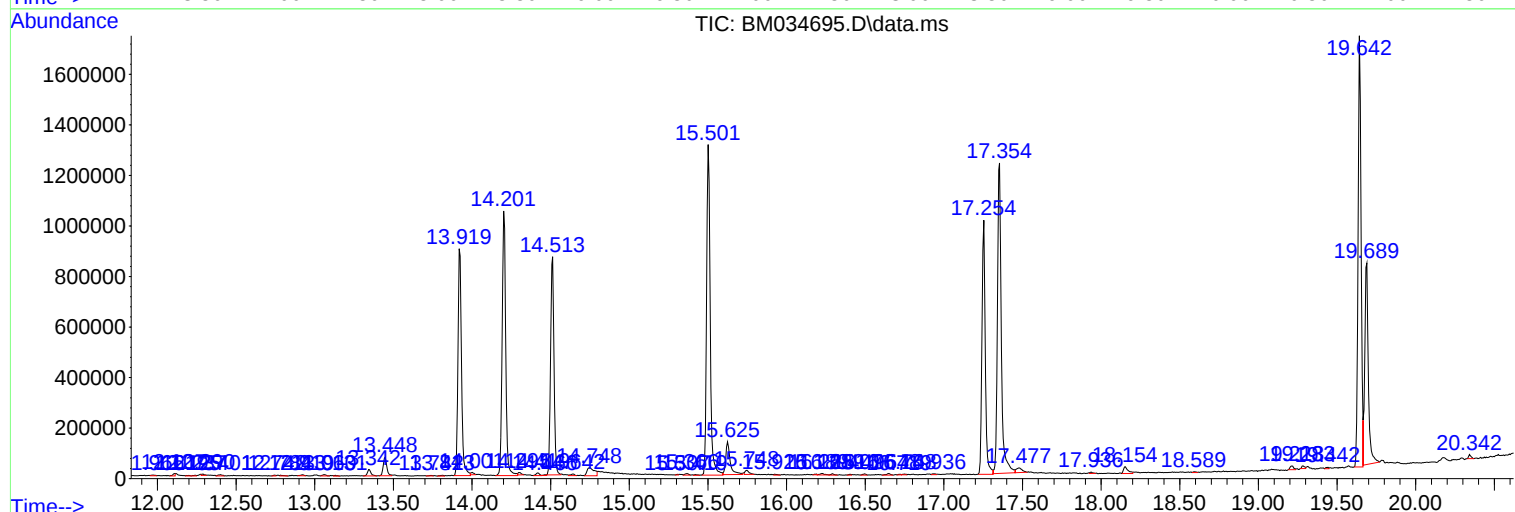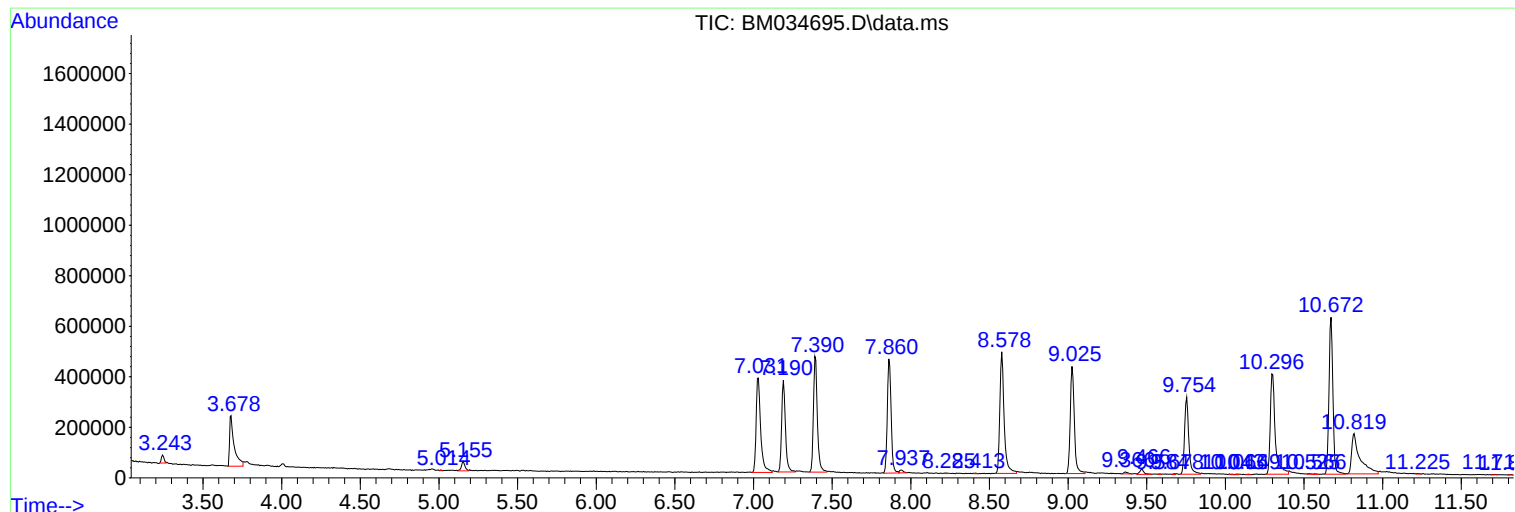

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034695.D
Acq On : 15 Apr 2022 08:27
Operator : CG/JU
Sample : N2316-20
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETNR8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 1,2,3-tribromo- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.712	20.06 ng/ul	1402430	Chrysene-d12	21.436

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 1,2,3-tribromo-	278	C3H5Br3	000096-11-7	50
2			Propane, 1,2,3-tribromo-	278	C3H5Br3	000096-11-7	40
3			Propane, 1,2,2-tribromo-	278	C3H5Br3	014476-30-3	28
4			2(3H)-Benzothiazolethione, 5-chl...	201	C7H4ClNS2	005331-91-9	17
5			N-t-Butyl 2-bromo-5-fluorobenzamide	273	C11H13BrFNO	941294-23-1	10

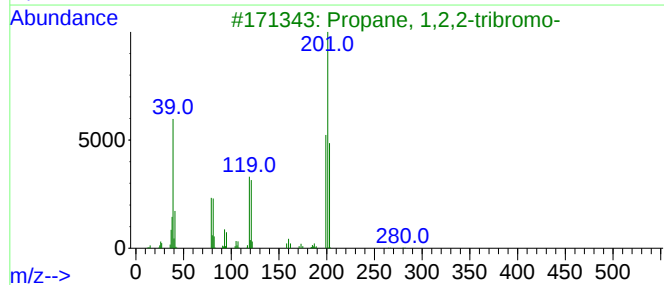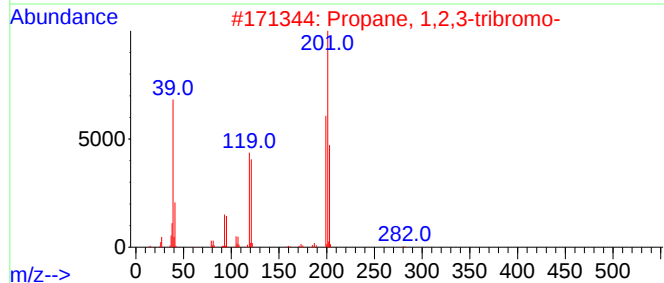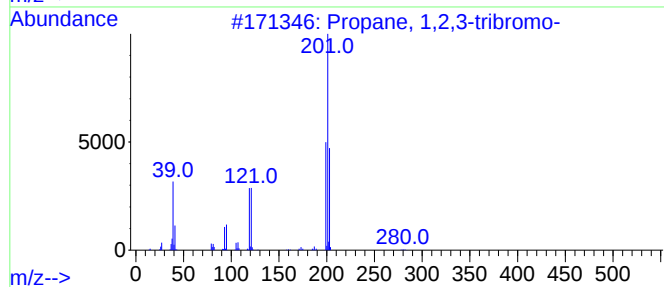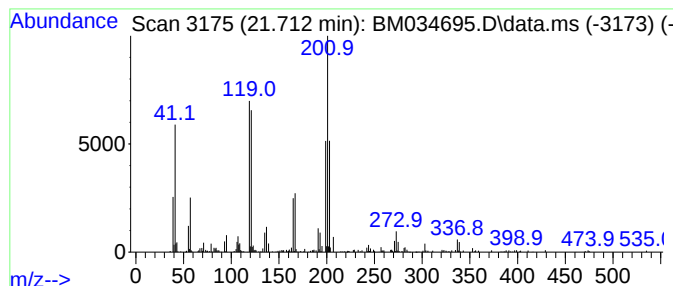

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041422\
Data File : BM034695.D
Acq On : 15 Apr 2022 08:27
Operator : CG/JU
Sample : N2316-20
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETNR8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 1,2,3-...	21.712	20.1	ng/ul	1402430	5	21.436	1398320	20.0