




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041515\SOM01.2\
Data File : BM001011.D
Acq On : 15 Apr 2015 15:53
Operator : TP/IZ
Sample : SSTD04024
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD04024

Manual Integrations
APPROVED

apatel
4/16/2015 3:24:40 PM

Quant Time: Apr 16 05:44:40 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041515.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 05:31:08 2015
Response via : Initial Calibration

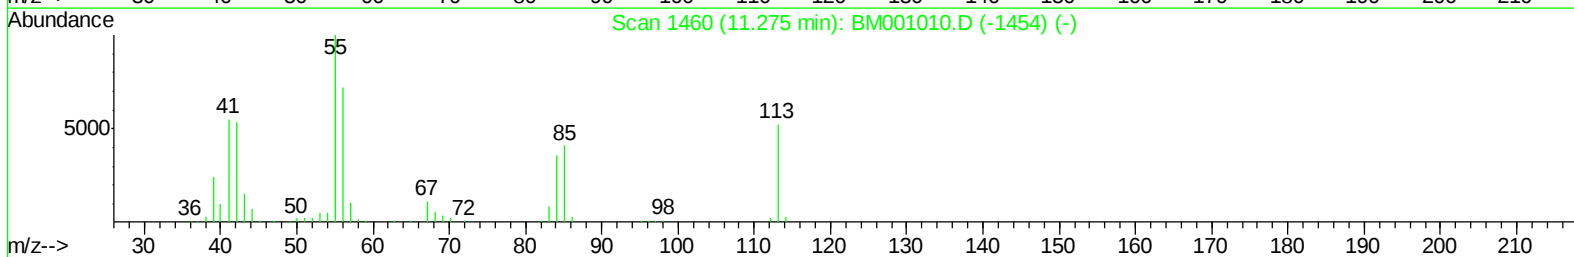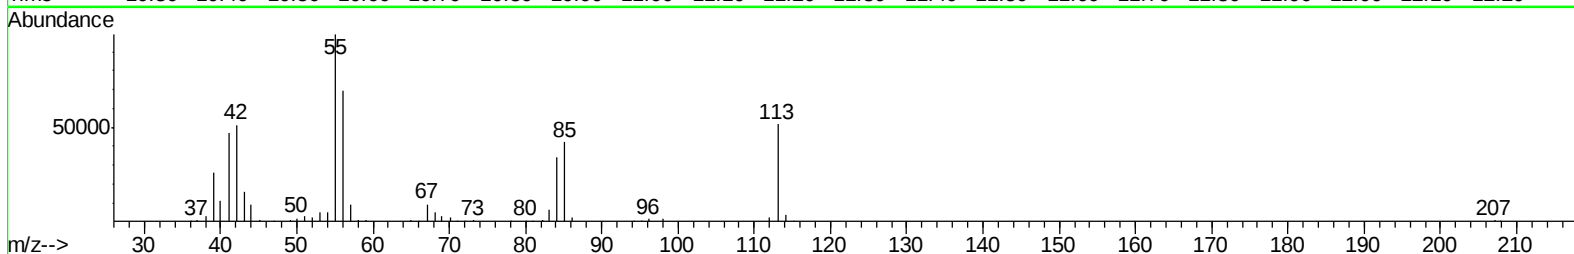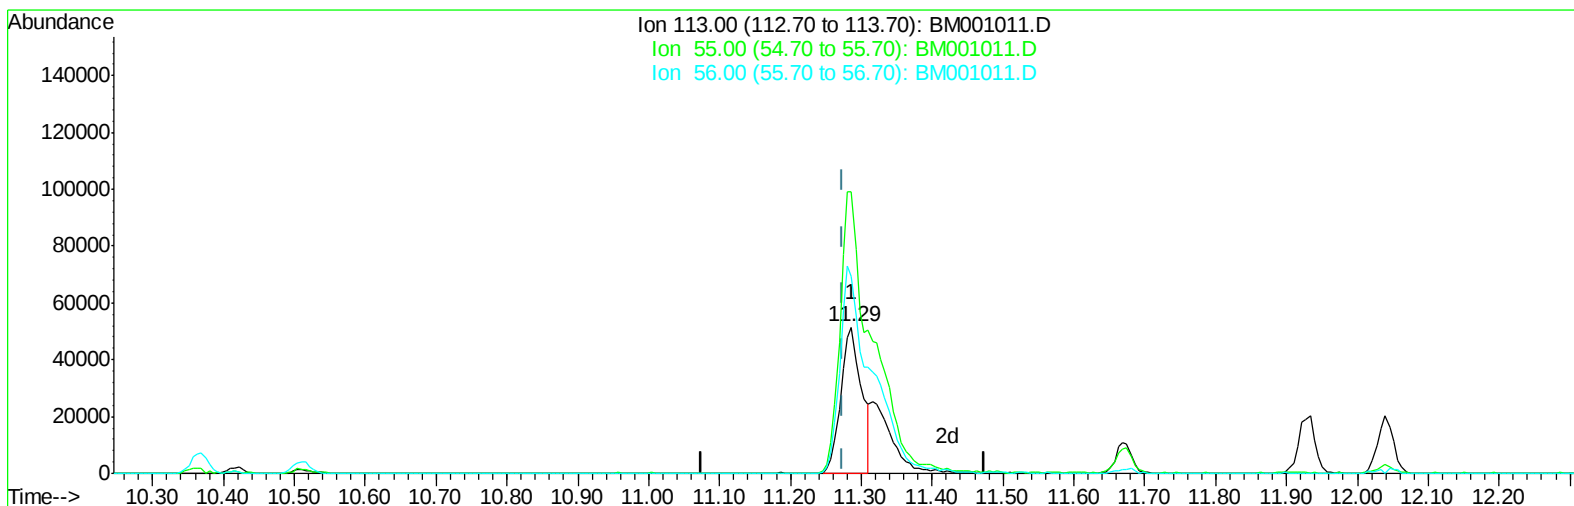

TIC: BM001011.D

(32) Caprolactam

11.286min (+0.012) 29.93ng/ul

response 105378

Ion	Exp%	Act%
113.00	100	100
55.00	192.90	192.48
56.00	139.50	134.33
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041515\SOM01.2\
Data File : BM001011.D
Acq On : 15 Apr 2015 15:53
Operator : TP/IZ
Sample : SSTD04024
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD04024

Manual Integrations
APPROVED

apatel
4/16/2015 3:24:40 PM

Quant Time: Apr 16 05:44:40 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041515.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 05:31:08 2015
Response via : Initial Calibration

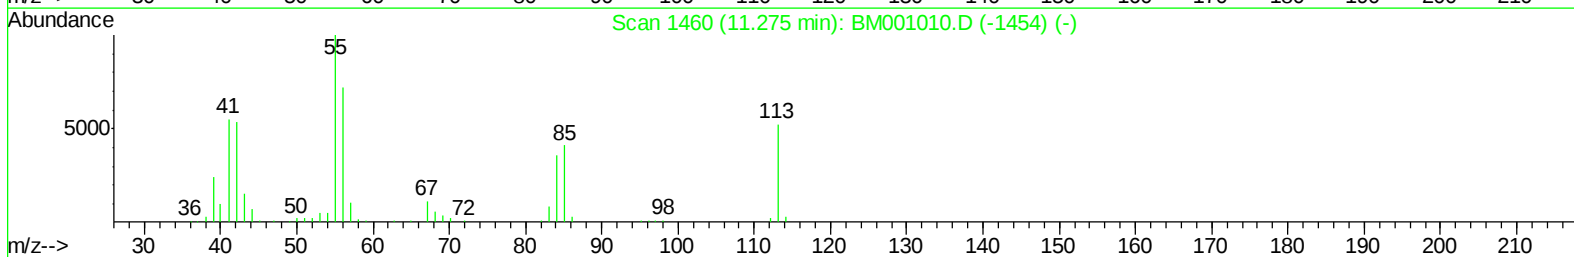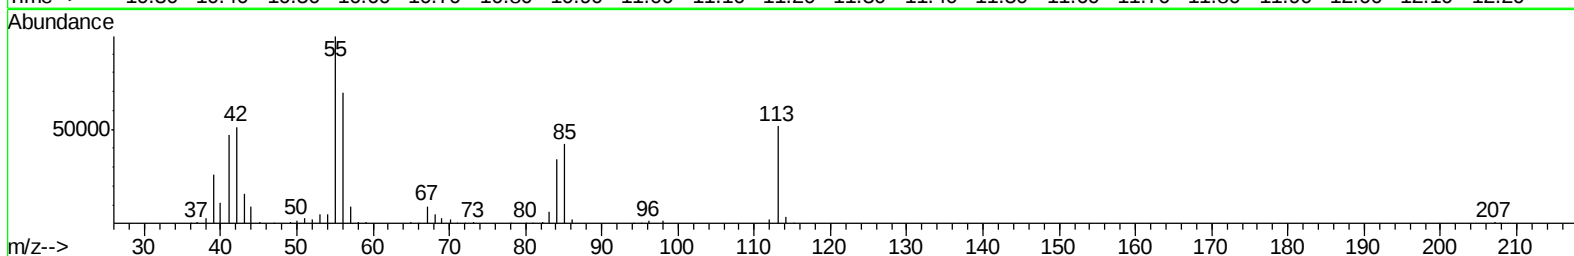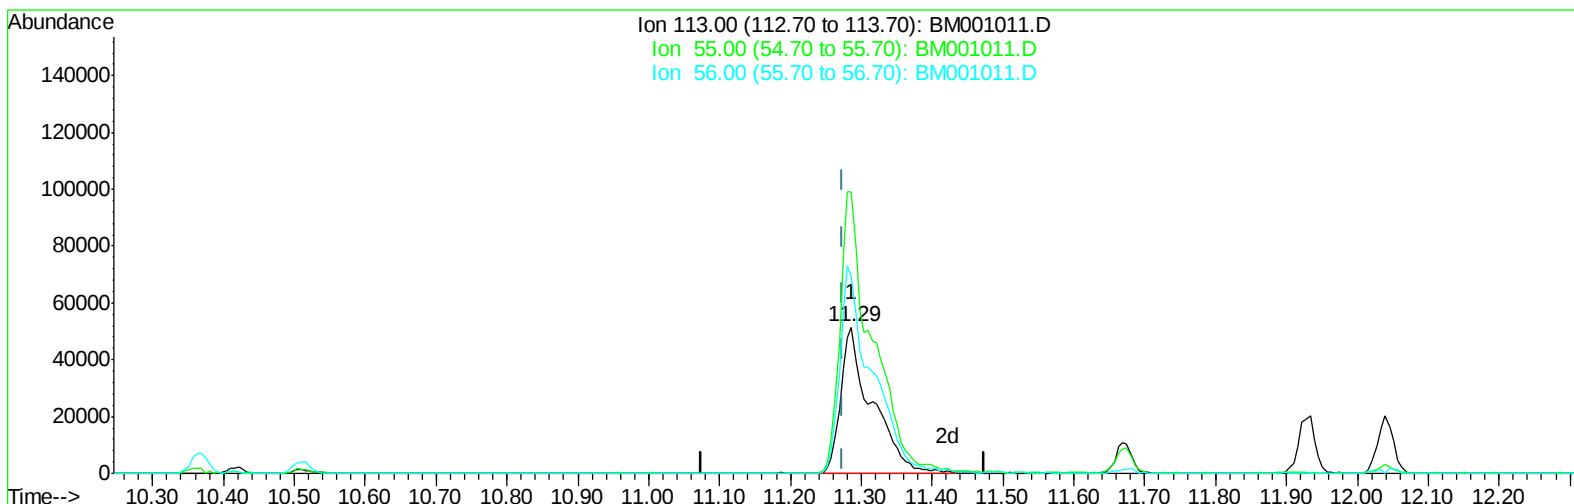

TIC: BM001011.D

(32) Caprolactam

11.286min (+0.012) 45.08ng/ul m

response 158721

Ion	Exp%	Act%
113.00	100	100
55.00	192.90	192.48
56.00	139.50	134.33
0.00	0.00	0.00