




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041515\SOM01.2\
Data File : BM001012.D
Acq On : 15 Apr 2015 16:29
Operator : TP/IZ
Sample : SSTD08025
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD08025

Manual Integrations
APPROVED

apatel
4/16/2015 3:24:44 PM

Quant Time: Apr 16 05:45:13 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041515.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 05:31:08 2015
Response via : Initial Calibration

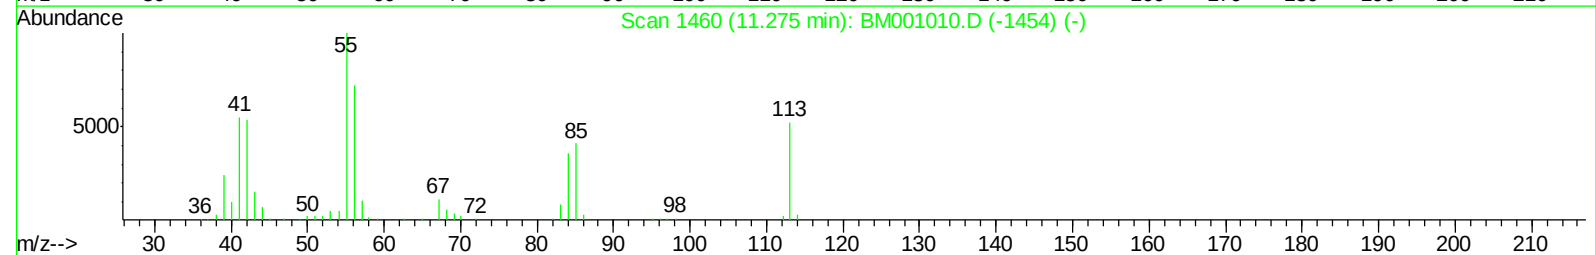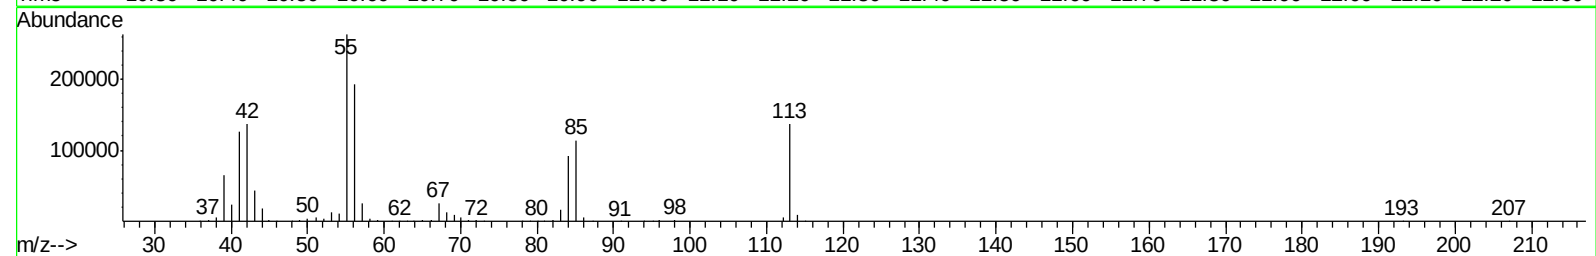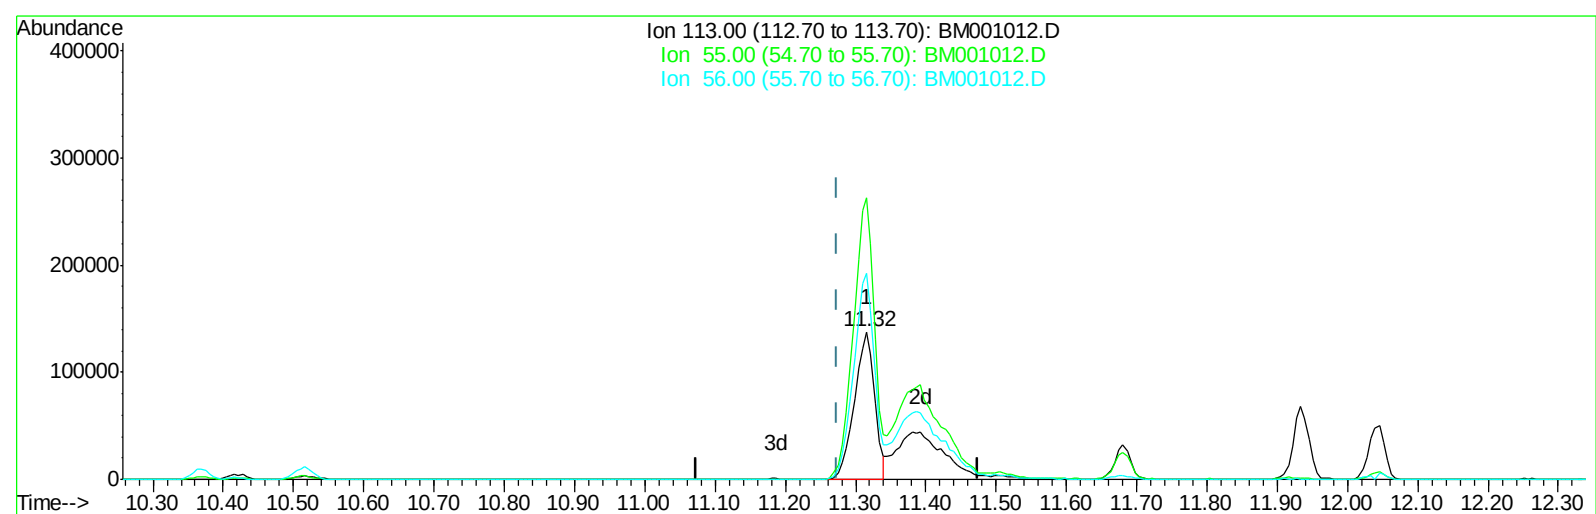

TIC: BM001012.D

(32) Caprolactam

11.316min (+0.041) 61.05ng/ul

response 275710

Ion	Exp%	Act%
113.00	100	100
55.00	192.90	191.11
56.00	139.50	139.94
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041515\SOM01.2\
Data File : BM001012.D
Acq On : 15 Apr 2015 16:29
Operator : TP/IZ
Sample : SSTD08025
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD08025

Manual Integrations
APPROVED

apatel
4/16/2015 3:24:44 PM

Quant Time: Apr 16 05:45:13 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM041515.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 16 05:31:08 2015
Response via : Initial Calibration

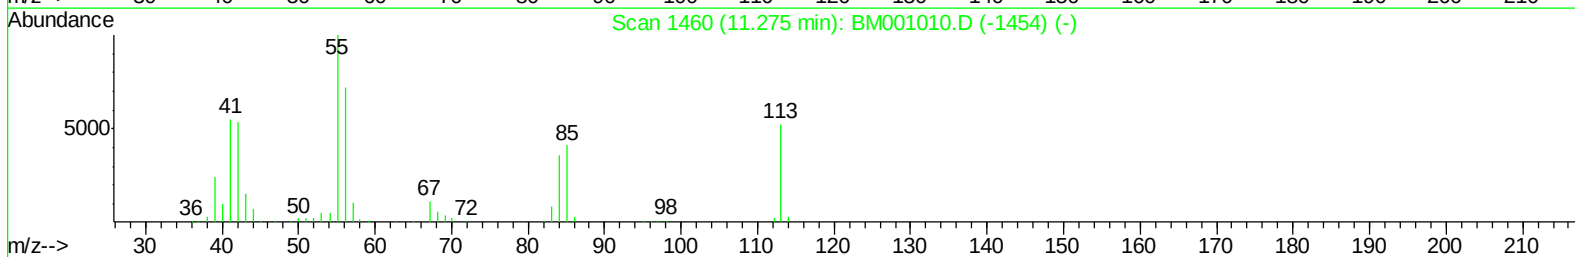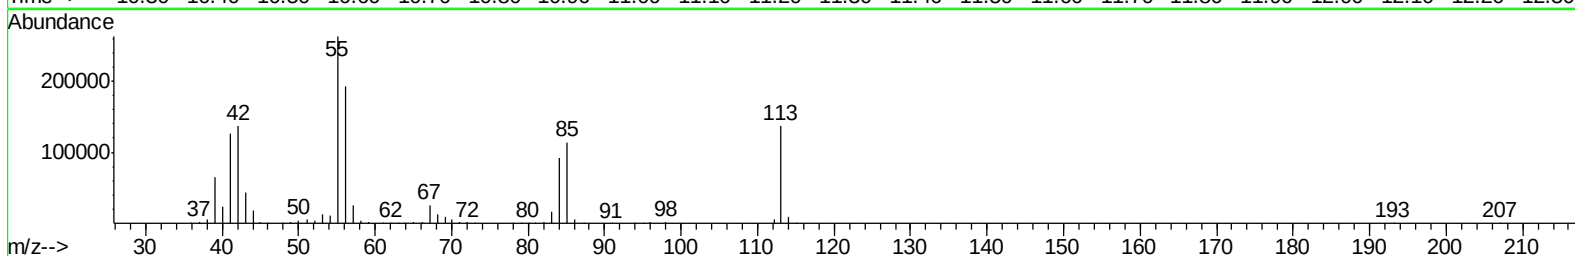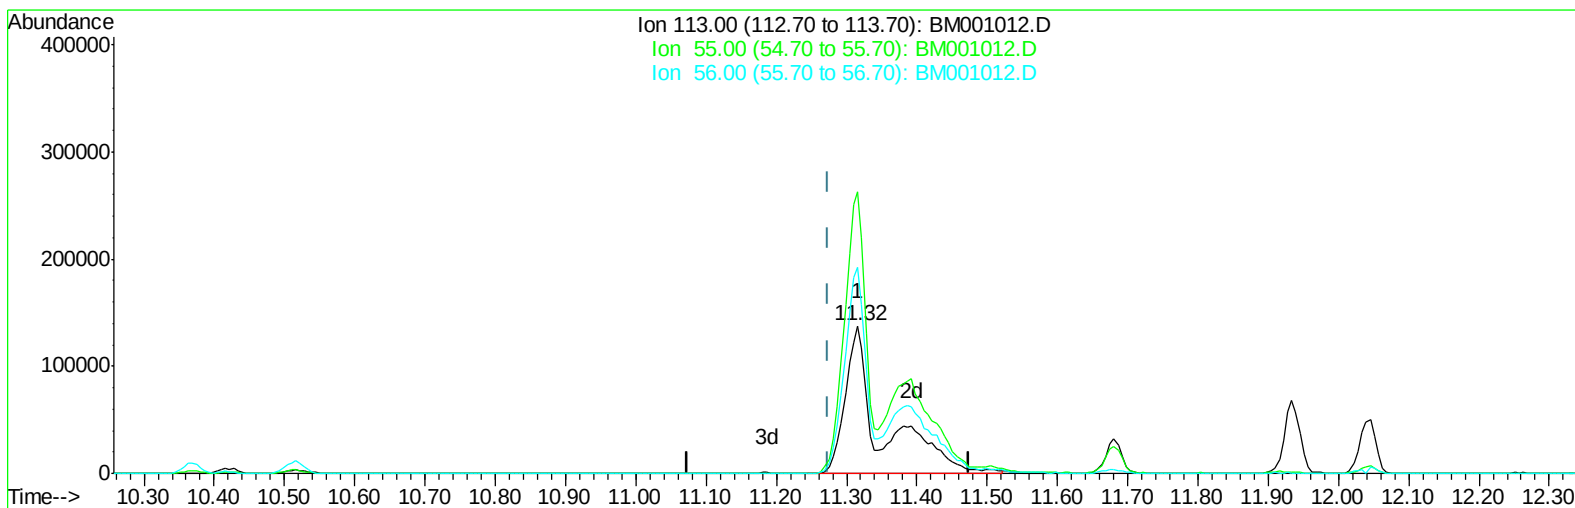

TIC: BM001012.D

(32) Caprolactam

11.316min (+0.041) 108.59ng/ul m

response 490380

Ion	Exp%	Act%
113.00	100	100
55.00	192.90	191.11
56.00	139.50	139.94
0.00	0.00	0.00