

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041516\
 Data File : BM004956.D
 Acq On : 15 Apr 2016 12:30
 Operator : UM/SJ
 Sample : H2298-09
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T92

Quant Time: Apr 15 23:03:08 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 15 22:59:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	50609	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	234455	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	142289	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	302782	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	295454	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	286065	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	1421	1.50	ng/uL	0.00
5) Phenol-d5	6.97	99	28203	7.81	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	88943	42.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	95029	31.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	47037	15.76	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	61969	39.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	69985	40.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	110766	34.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	1143	0.32	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	401396	41.47	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	485596	40.91	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	6773	4.10	ng/ul	0.00
57) Fluorene-d10	15.44	176	345575	41.33	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	44320	33.84	ng/ul	0.00
70) Anthracene-d10	17.29	188	405505	33.70	ng/ul	0.00
76) Pyrene-d10	19.59	212	452343	36.74	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	451210	40.96	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) 2,6-Dinitrotoluene	13.86	165	2776	1.45	ng/ul#	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041516\
Data File : BM004956.D
Acq On : 15 Apr 2016 12:30
Operator : UM/SJ
Sample : H2298-09
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9T92

Quant Time: Apr 15 23:03:08 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 15 22:59:24 2016
Response via : Initial Calibration

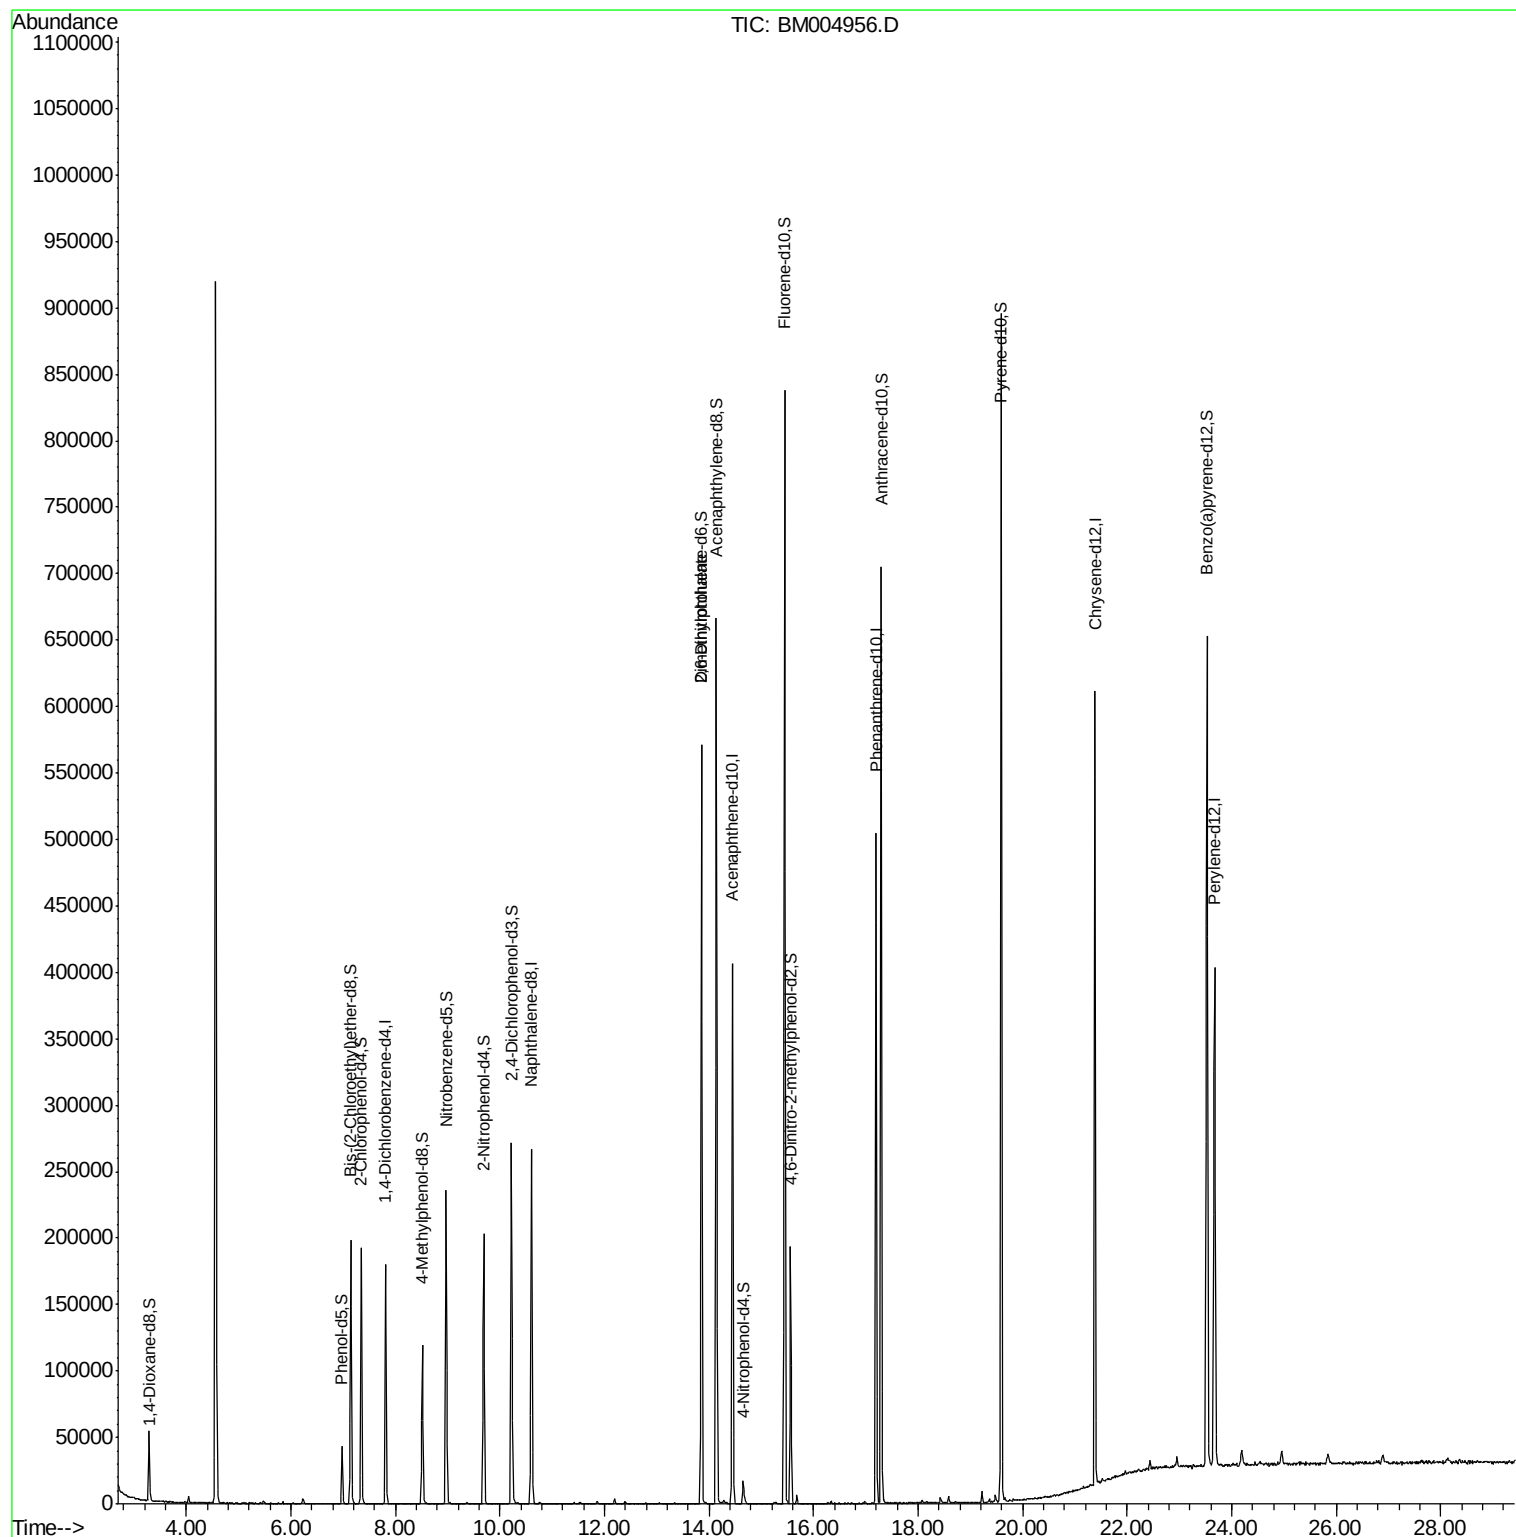

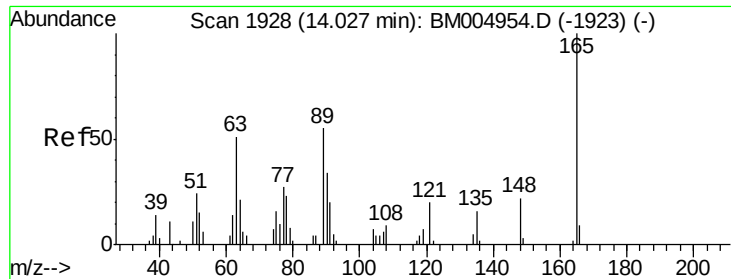

#45
 2,6-Dinitrotoluene
 Concen: 1.45 ng/ul
 RT: 13.86 min Scan# 1899
 Delta R.T. -0.17 min
 Lab File: BM004956.D
 Acq: 15 Apr 2016 12:30

Instrument :
 BNA_M
 ClientSampleId :
 D9T92

Tgt Ion:165 Resp: 2776
 Ion Ratio Lower Upper
 165 100
 89 0.0 43.1 64.7#
 121 28.6 16.0 24.0#

