

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041516\
 Data File : BM004959.D
 Acq On : 15 Apr 2016 15:30
 Operator : UM/SJ
 Sample : H2298-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9T99

Quant Time: Apr 15 23:03:32 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 15 22:59:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	59790	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	272269	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	173636	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	395258	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	370845	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	307460	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	1441	1.29	ng/uL	0.00
5) Phenol-d5	6.97	99	27216	6.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	84493	34.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	90583	25.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	57568	16.33	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	60718	33.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	67815	33.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	110261	29.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	3563	0.86	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	449799	38.08	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	515735	35.60	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	7591	3.77	ng/ul	0.00
57) Fluorene-d10	15.44	176	376704	36.92	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	52423	30.66	ng/ul	0.00
70) Anthracene-d10	17.29	188	569424	36.26	ng/ul	0.00
76) Pyrene-d10	19.59	212	617396	39.95	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	457021	38.60	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) 2,6-Dinitrotoluene	13.86	165	3187	1.36	ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041516\
Data File : BM004959.D
Acq On : 15 Apr 2016 15:30
Operator : UM/SJ
Sample : H2298-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9T99

Quant Time: Apr 15 23:03:32 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 15 22:59:24 2016
Response via : Initial Calibration

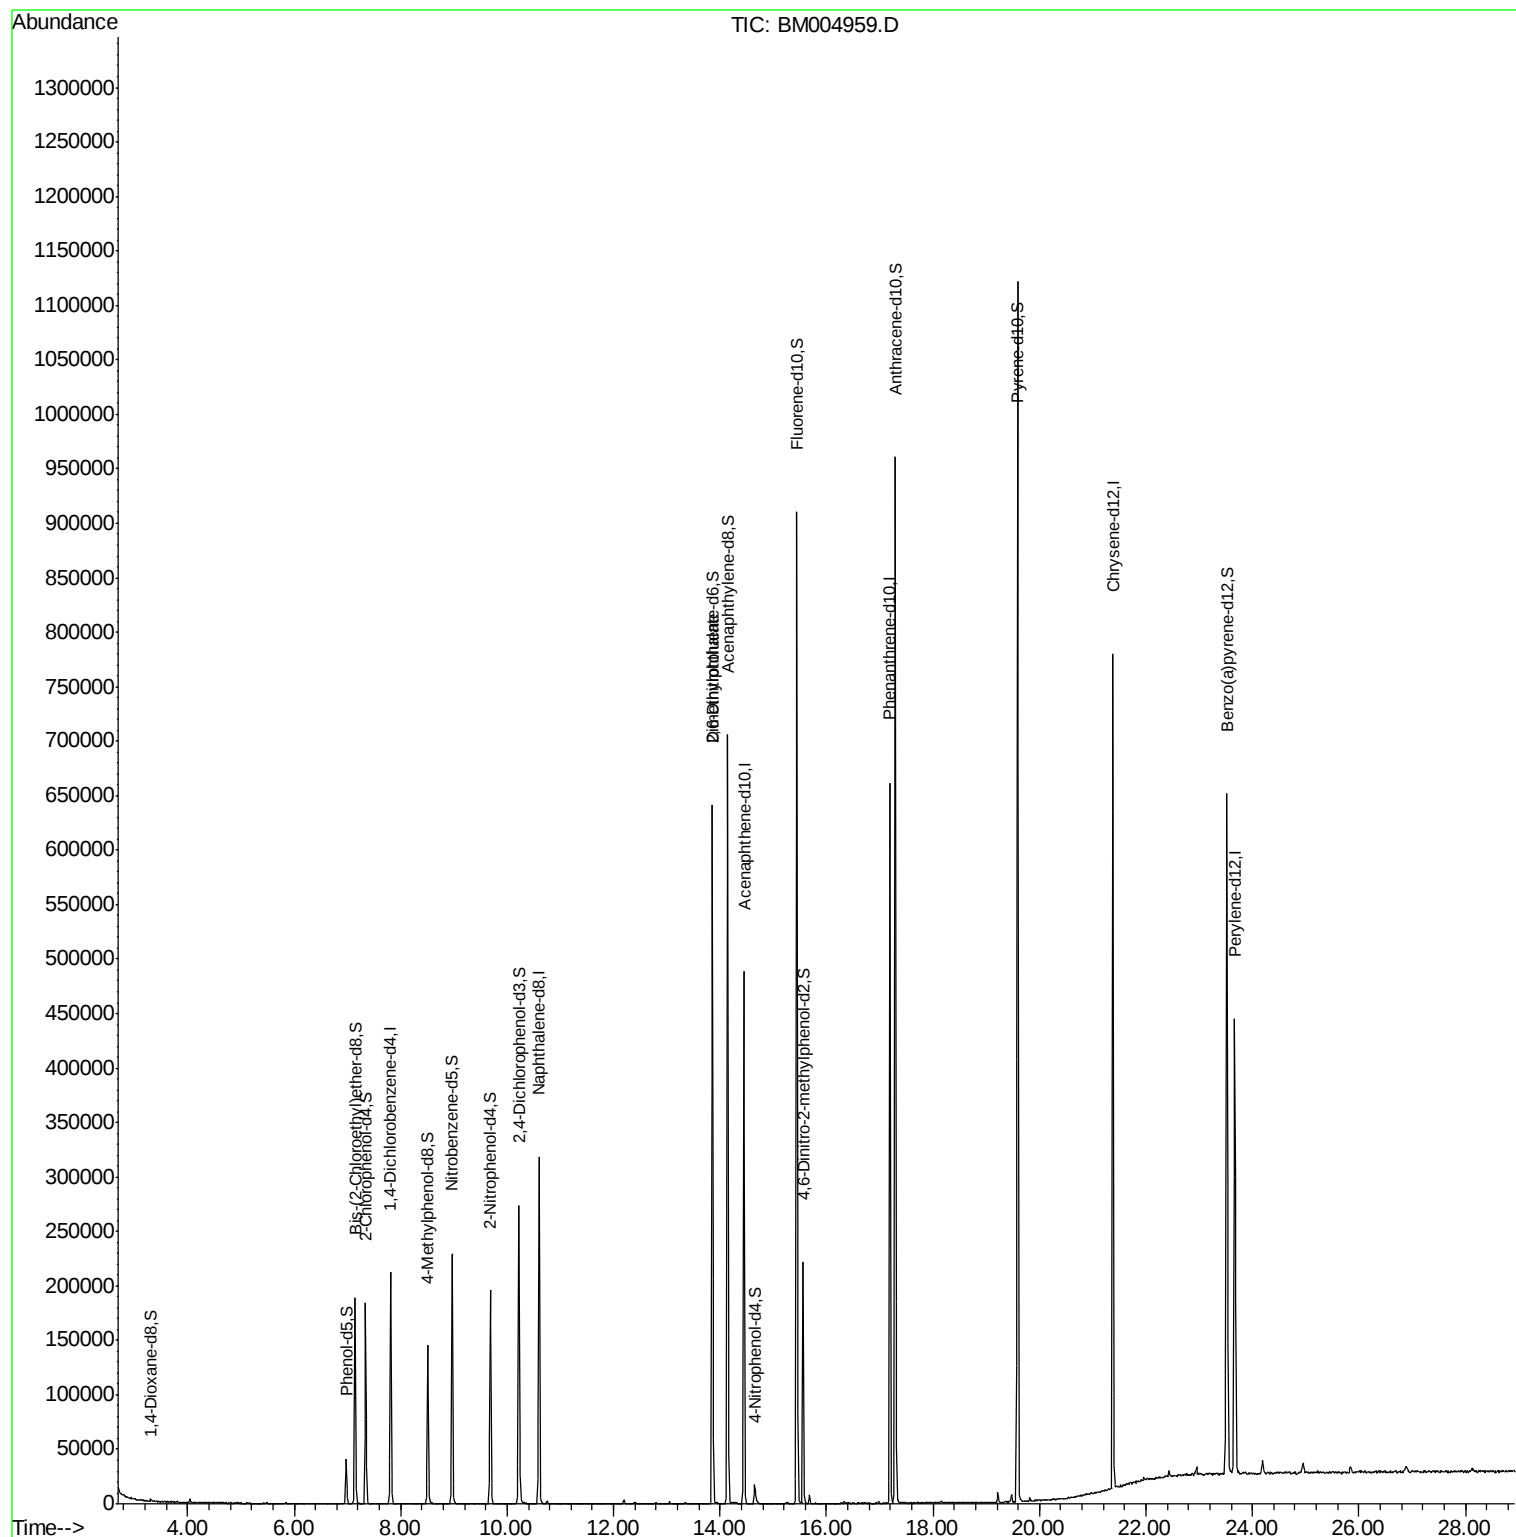

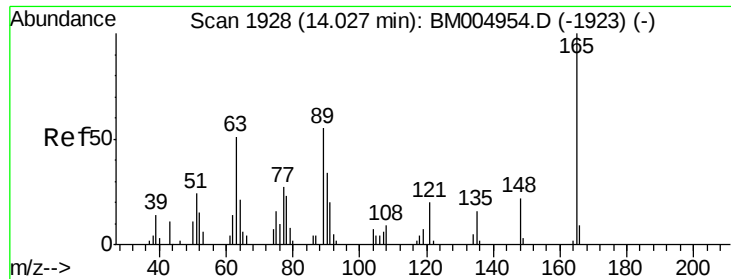

#45

2,6-Dinitrotoluene

Concen: 1.36 ng/ul

RT: 13.86 min Scan# 1899

Delta R.T. -0.17 min

Lab File: BM004959.D


Acq: 15 Apr 2016 15:30

Instrument :

BNA_M

ClientSampleId :

D9T99

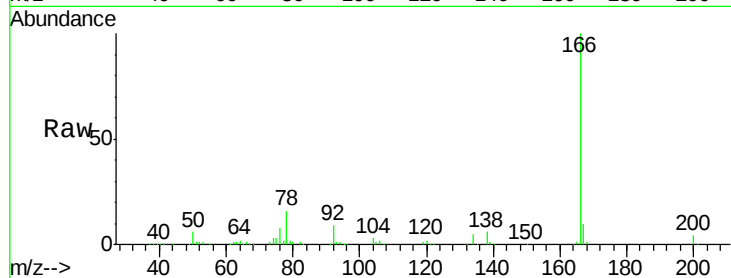

Tgt Ion:	165	Resp:	3187
Ion Ratio	Lower	Upper	
165	100		
89	0.0	43.1	64.7#
121	31.3	16.0	24.0#

