

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041516\
 Data File : BM004965.D
 Acq On : 15 Apr 2016 19:34
 Operator : UM/SJ
 Sample : PB89717BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK17

Quant Time: Apr 15 23:05:03 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 15 22:59:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	65068	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	295452	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.45	164	185537	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	433312	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	452929	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	372236	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.31	96	8053	6.63	ng/uL	0.00
5) Phenol-d5	6.98	99	144907	31.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	89819	33.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	118561	30.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.51	113	122247	31.86	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	61001	31.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	68984	31.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.22	165	118489	29.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	181570	40.29	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	485216	38.45	ng/ul	0.00
46) Acenaphthylene-d8	14.14	160	520845	33.65	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	67040	31.13	ng/ul	0.00
57) Fluorene-d10	15.44	176	392693	36.02	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	58791	31.37	ng/ul	0.00
70) Anthracene-d10	17.29	188	651506	37.84	ng/ul	0.00
76) Pyrene-d10	19.59	212	736155	39.00	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.53	264	593708	41.42	ng/ul	0.00


Target Compounds					Qvalue
45) 2,6-Dinitrotoluene	13.86	165	3350	1.34 ng/ul#	40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM041516\
Data File : BM004965.D
Acq On : 15 Apr 2016 19:34
Operator : UM/SJ
Sample : PB89717BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK17

Quant Time: Apr 15 23:05:03 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM041416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 15 22:59:24 2016
Response via : Initial Calibration

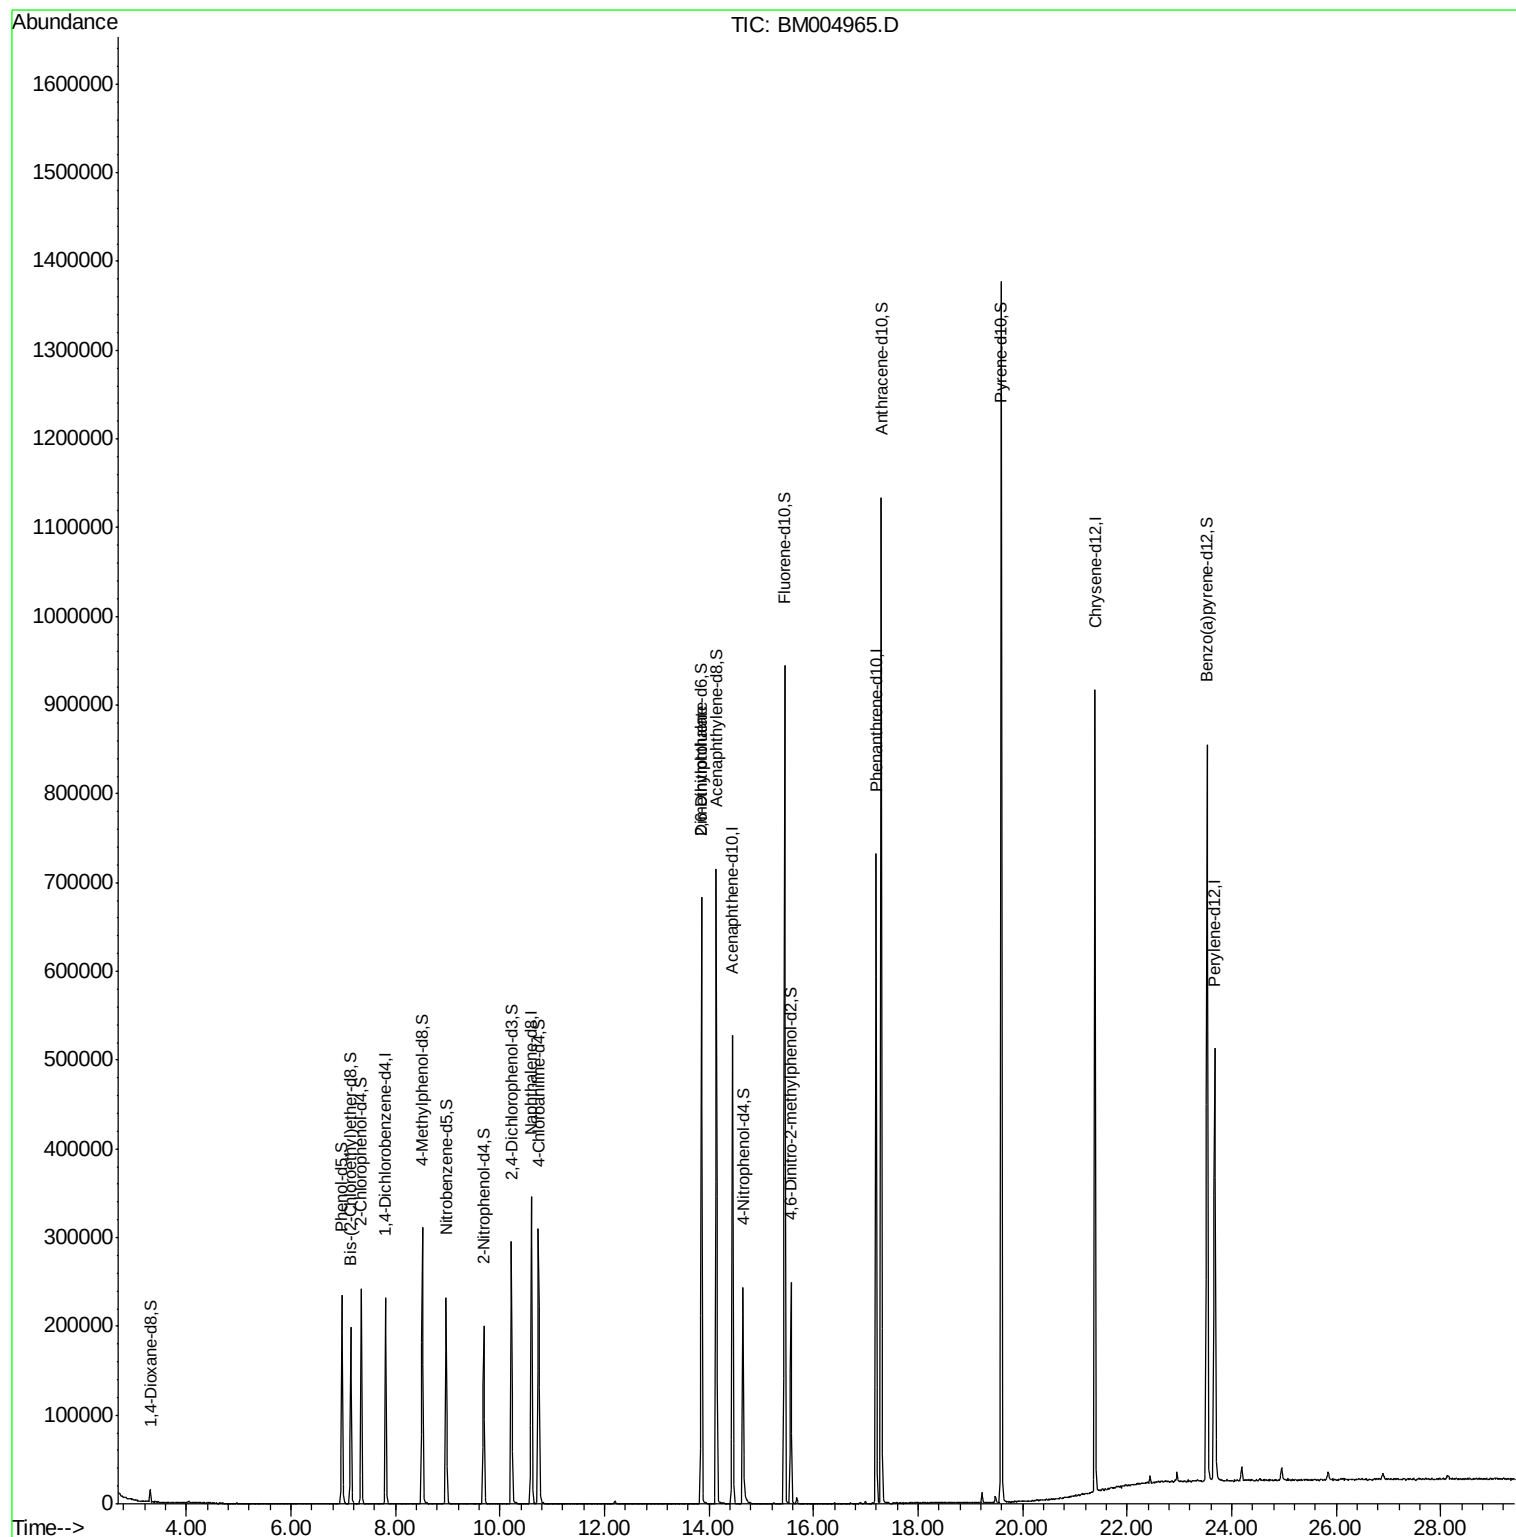

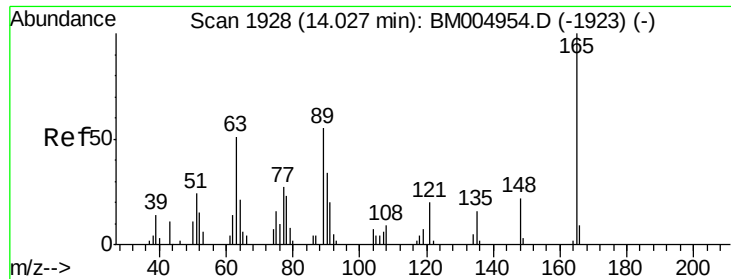

#45

2,6-Dinitrotoluene

Concen: 1.34 ng/ul

RT: 13.86 min Scan# 1899

Delta R.T. -0.17 min

Lab File: BM004965.D


Acq: 15 Apr 2016 19:34

Instrument :

BNA_M

ClientSampleId :

SBLK17

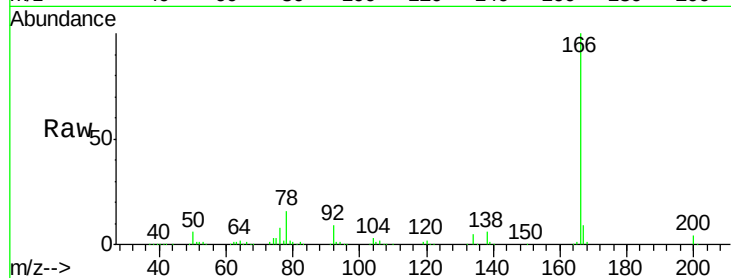

Tgt Ion:	165	Resp:	3350
Ion Ratio	Lower	Upper	
165	100		
89	0.0	43.1	64.7#
121	29.2	16.0	24.0#

