




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
 Data File : BM034703.D
 Acq On : 15 Apr 2022 15:49
 Operator : CG/JU
 Sample : N2290-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFFC8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 06:45:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 05:39:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

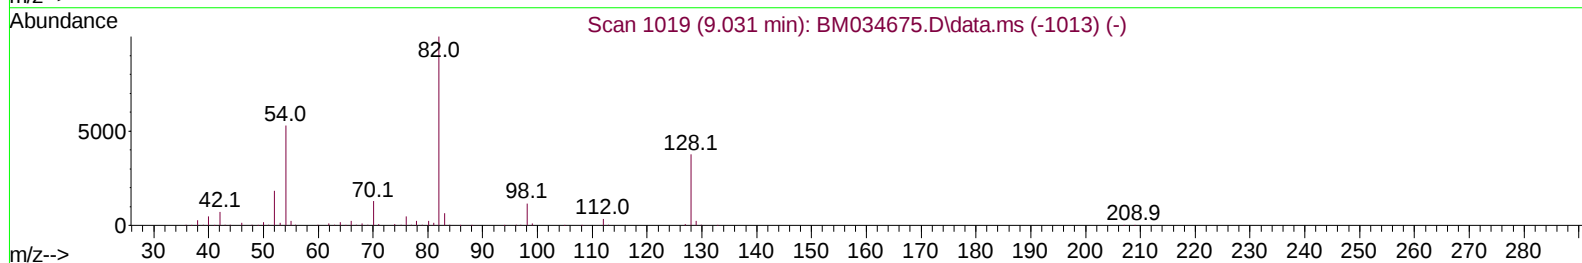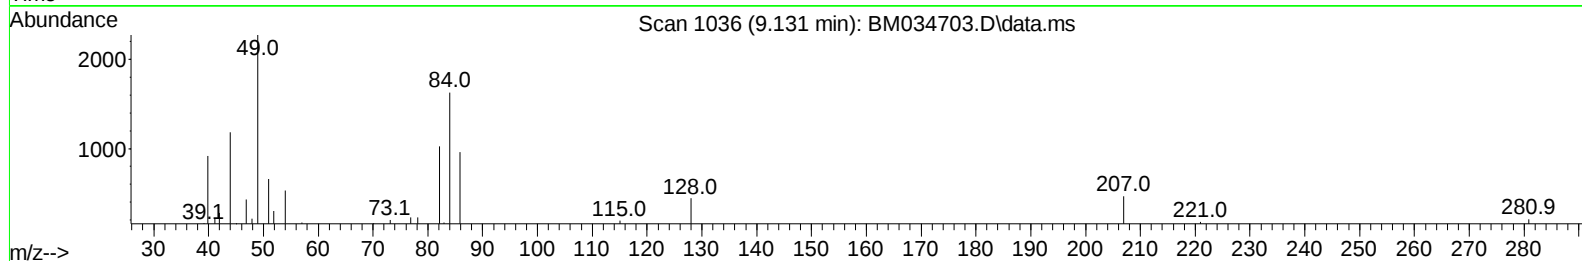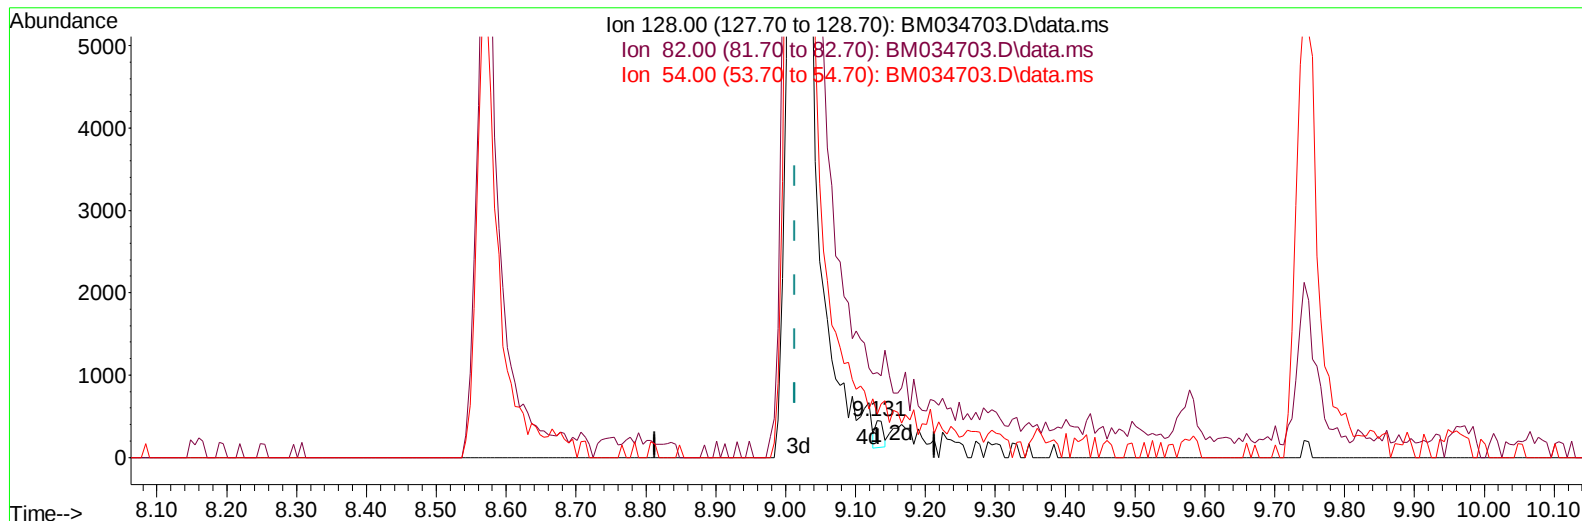

TIC: BM034703.D\data.ms

(21) Nitrobenzene-d5 (S)

9.131min (+ 0.118) 0.09 ng/u1

response 255

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	228.00	231.24
54.00	100.50	118.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
 Data File : BM034703.D
 Acq On : 15 Apr 2022 15:49
 Operator : CG/JU
 Sample : N2290-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFFC8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 06:45:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 05:39:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

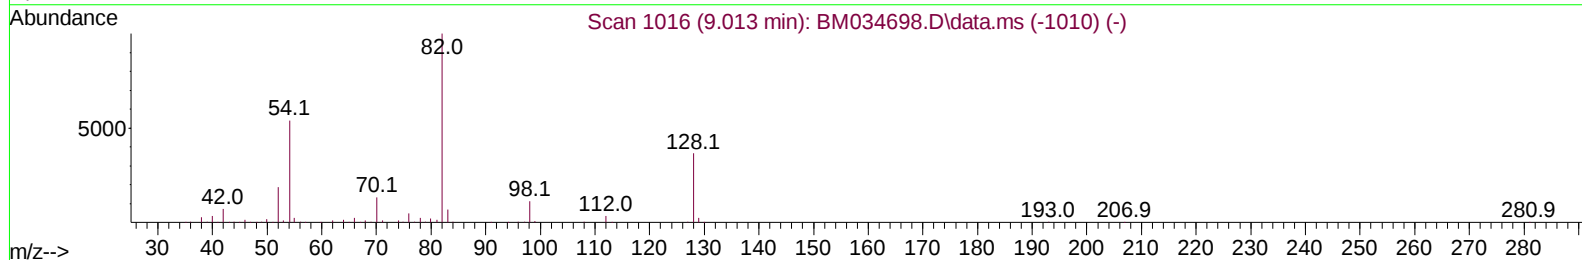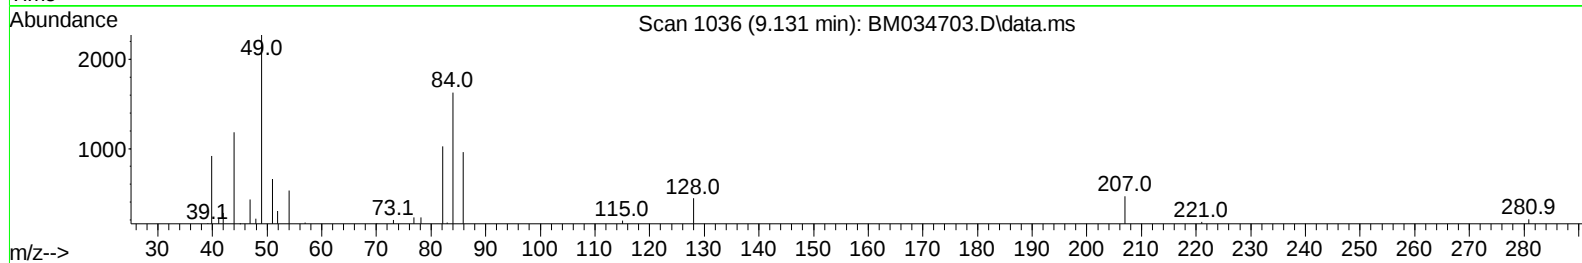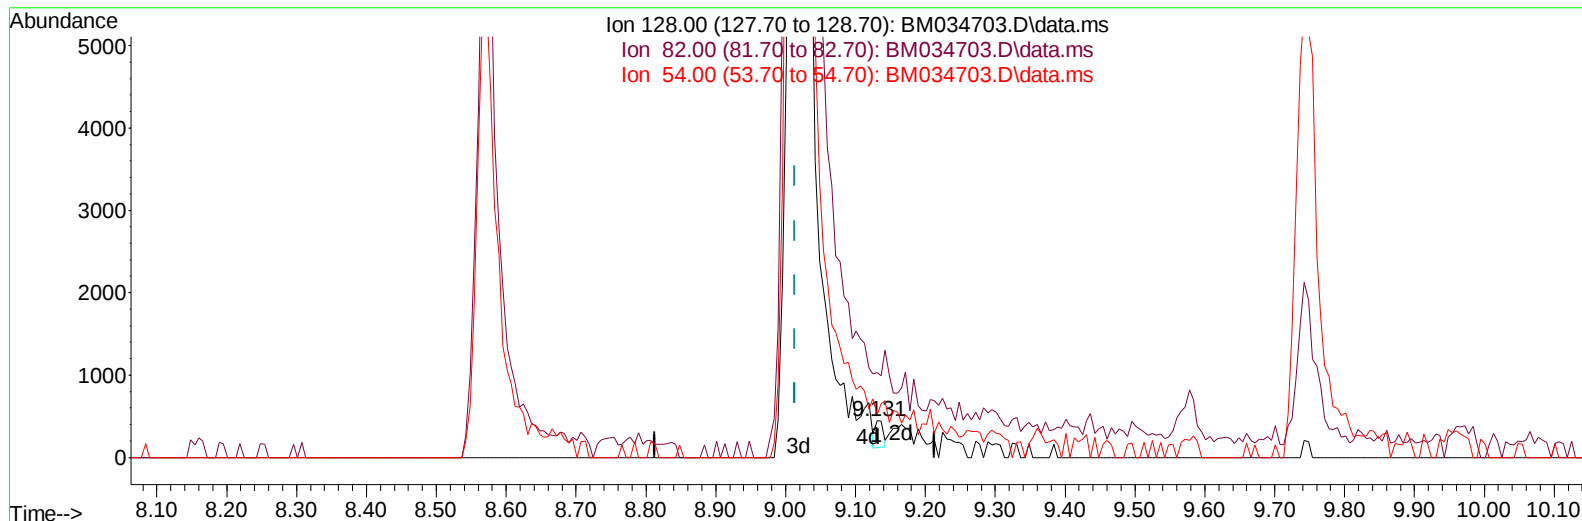

TIC: BM034703.D\data.ms

(21) Nitrobenzene-d5 (S)

9.131min (+ 0.118) 0.09 ng/u1

response 255

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	228.00	231.24
54.00	100.50	118.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
 Data File : BM034703.D
 Acq On : 15 Apr 2022 15:49
 Operator : CG/JU
 Sample : N2290-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFFC8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 06:45:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 05:39:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

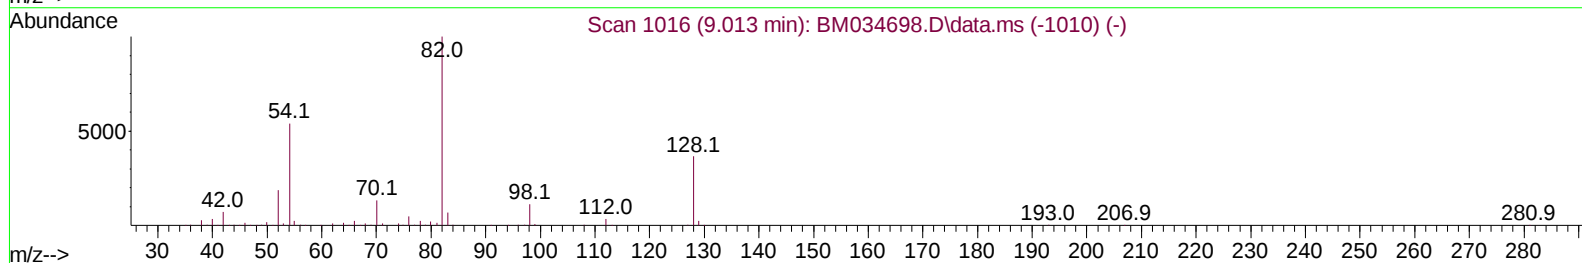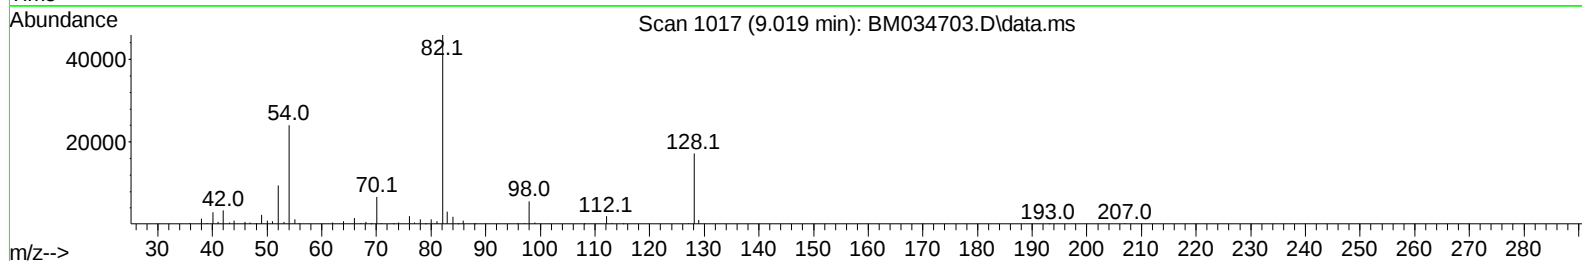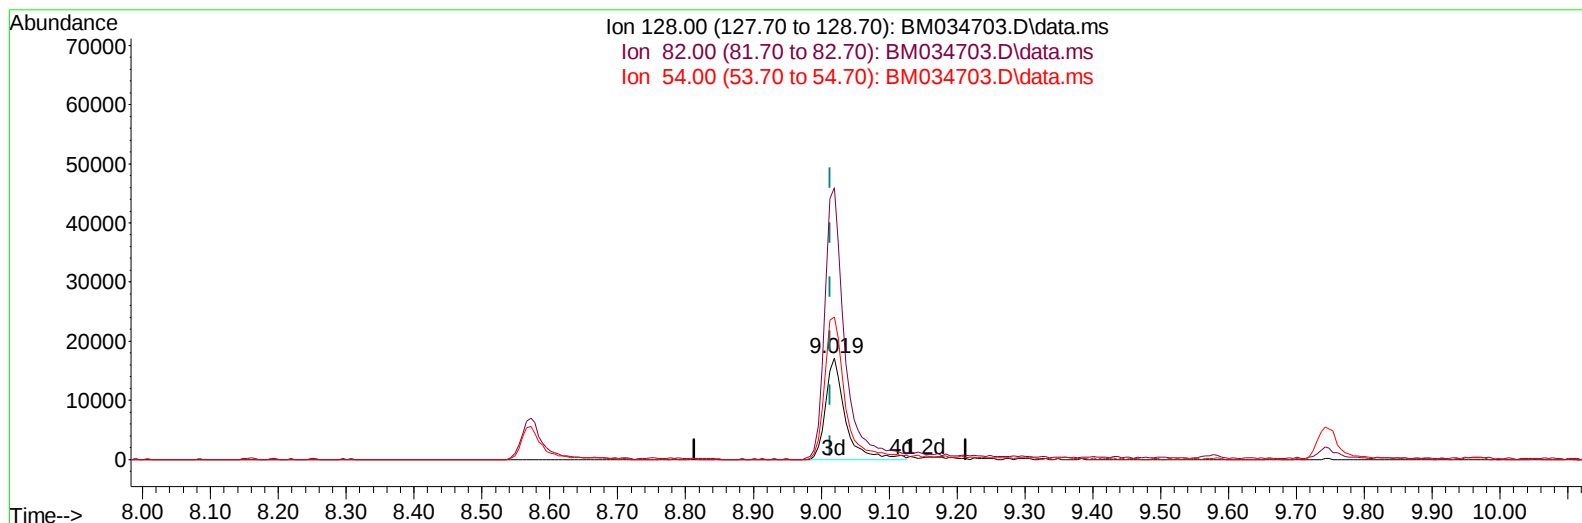

TIC: BM034703.D\data.ms

(21) Nitrobenzene-d5 (S)

9.019min (+ 0.006) 12.67 ng/ul m

response 34320

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	228.00	266.81
54.00	100.50	139.75#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
Data File : BM034703.D
Acq On : 15 Apr 2022 15:49
Operator : CG/JU
Sample : N2290-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFFC8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 06:45:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 05:39:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

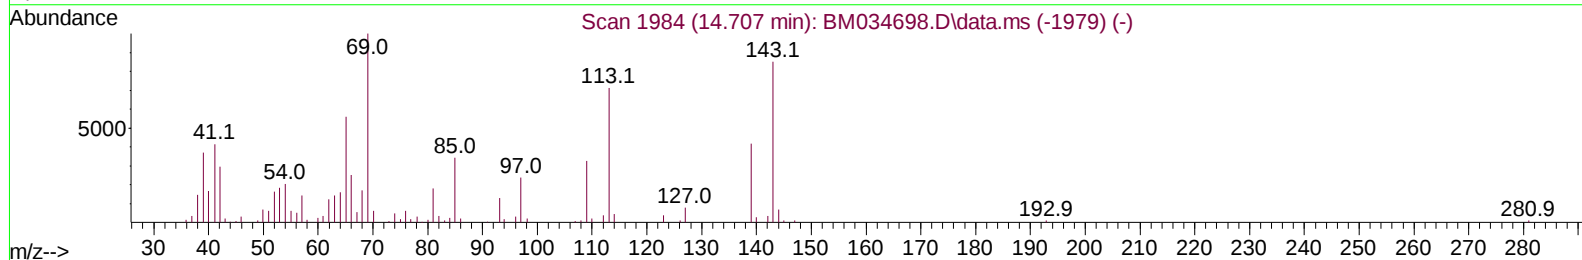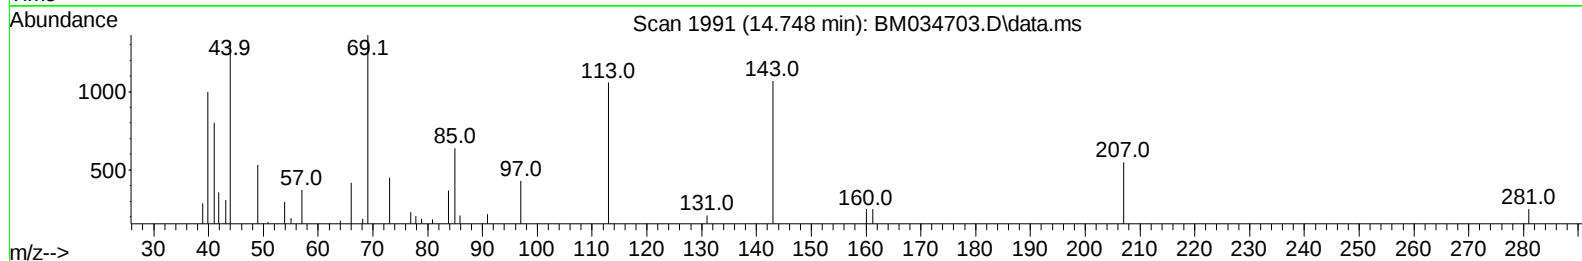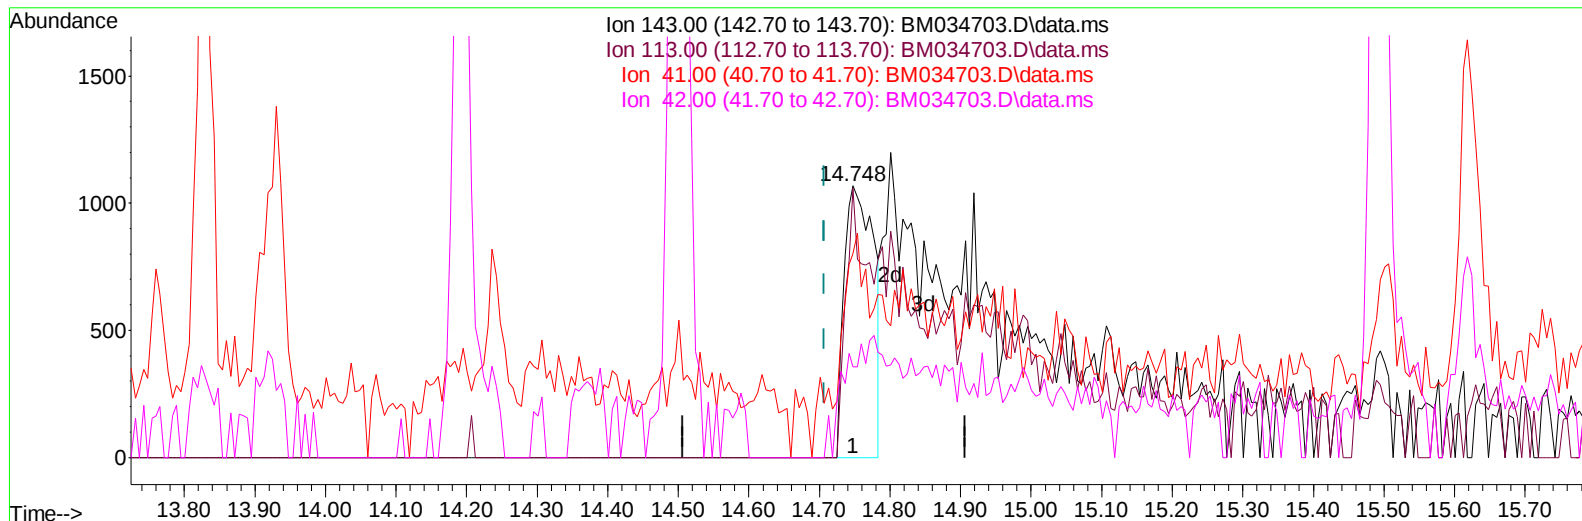

TIC: BM034703.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.748min (+ 0.041) 1.34 ng/ul

response 3108

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	99.06#
41.00	31.90	75.19#
42.00	19.10	33.33#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
Data File : BM034703.D
Acq On : 15 Apr 2022 15:49
Operator : CG/JU
Sample : N2290-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFFC8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 06:45:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 05:39:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

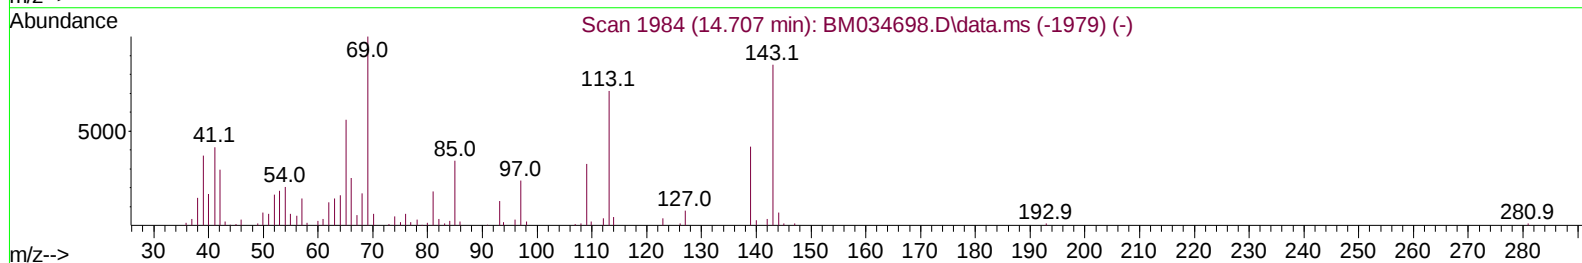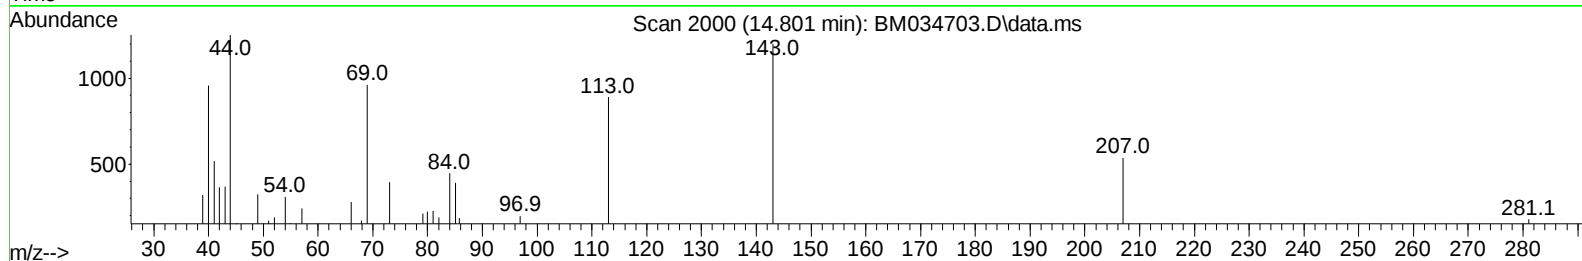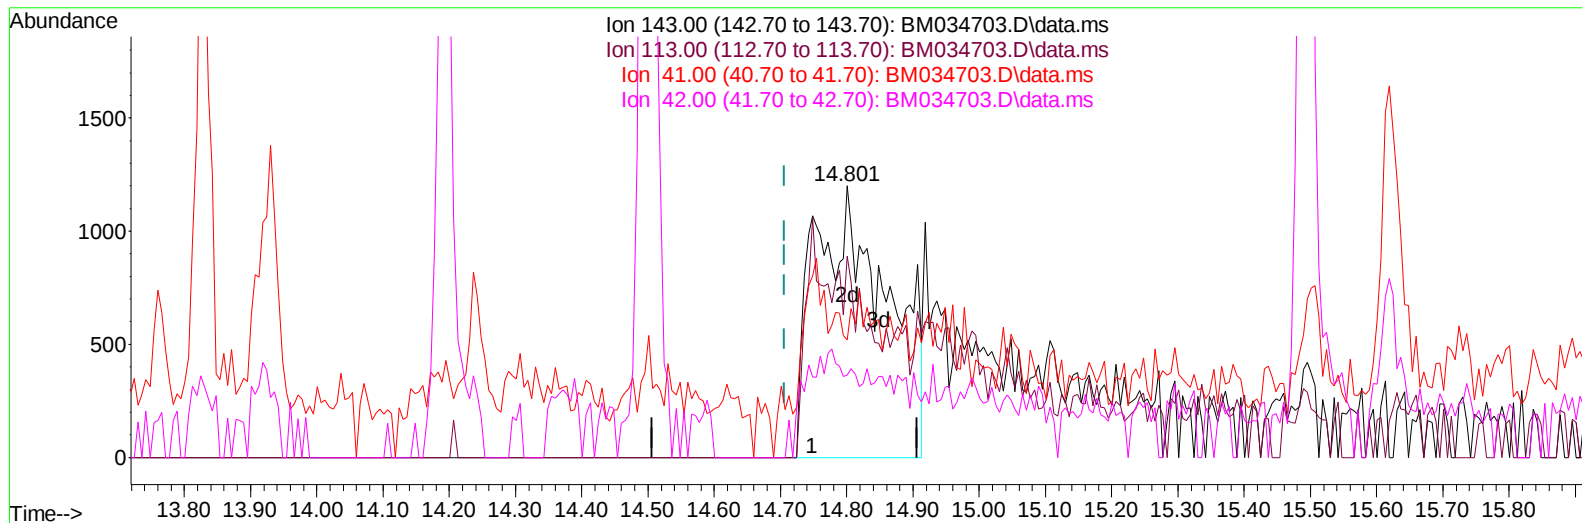

TIC: BM034703.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.801min (+ 0.094) 3.93 ng/ul m

response 9154

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	77.80	74.08
41.00	31.90	43.17#
42.00	19.10	30.25#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
 Data File : BM034703.D
 Acq On : 15 Apr 2022 15:49
 Operator : CG/JU
 Sample : N2290-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFFC8

Manual IntegrationsAPPROVED

Quant Time: Apr 18 06:45:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 05:39:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/18/2022
 Supervised By :Yogesh Patel 04/18/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.854	152		93296	20.000	ng/ul	0.00
20) Naphthalene-d8	10.660	136		368575	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.501	164		211145	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.242	188		397057	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.424	240		378801	20.000	ng/ul	# 0.00
88) Perylene-d12	23.794	264		417286	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.231	96		6323	2.417	ng/uL	0.00
4) Pyridine-d5	3.672	84		29327	4.645	ng/ul	0.01
7) Phenol-d5	7.019	99		79198	10.199	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.178	67		66837	12.917	ng/ul	0.00
11) 2-Chlorophenol-d4	7.384	132		79758	13.287	ng/ul	0.00
15) 4-Methylphenol-d8	8.572	113		71126	11.726	ng/ul	0.00
21) Nitrobenzene-d5	9.019	128		34320m	12.670	ng/ul	0.00
24) 2-Nitrophenol-d4	9.748	143		34428	12.208	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.289	165		59625	11.228	ng/ul	0.00
31) 4-Chloroaniline-d4	10.813	131		63849	8.715	ng/ul	0.01
46) Dimethylphthalate-d6	13.913	166		248079	16.260	ng/ul	0.00
49) Acenaphthylene-d8	14.195	160		278684	14.212	ng/ul	0.00
54) 4-Nitrophenol-d4	14.801	143		9154m	3.935	ng/ul	0.09
60) Fluorene-d10	15.495	176		213644	16.204	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.618	200		19897	8.209	ng/ul	0.00
73) Anthracene-d10	17.342	188		321632	16.990	ng/ul	0.00
81) Pyrene-d10	19.636	212		397835	19.243	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.641	264		382891	18.241	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
Data File : BM034703.D
Acq On : 15 Apr 2022 15:49
Operator : CG/JU
Sample : N2290-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFFC8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/18/2022
Supervised By :Yogesh Patel 04/18/2022

Quant Time: Apr 18 06:45:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 05:39:41 2022
Response via : Initial Calibration

