

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
 Data File : BM034706.D
 Acq On : 15 Apr 2022 17:37
 Operator : CG/JU
 Sample : N2358-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETNS1

Quant Time: Apr 18 07:56:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 18 05:39:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.854	152	102463	20.000	ng/ul	0.00
20) Naphthalene-d8	10.660	136	417873	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.501	164	246519	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.242	188	474174	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.424	240	425581	20.000	ng/ul	# 0.00
88) Perylene-d12	23.794	264	450363	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.237	96	5944	2.069	ng/uL	0.00
4) Pyridine-d5	3.672	84	26513	3.823	ng/ul	0.01
7) Phenol-d5	7.019	99	88685	10.399	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.178	67	61157	10.762	ng/ul	0.00
11) 2-Chlorophenol-d4	7.384	132	71010	10.771	ng/ul	0.00
15) 4-Methylphenol-d8	8.566	113	93598	14.050	ng/ul	0.00
21) Nitrobenzene-d5	9.019	128	38232	12.449	ng/ul	0.00
24) 2-Nitrophenol-d4	9.742	143	43984	13.756	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.284	165	91512	15.199	ng/ul	0.00
31) 4-Chloroaniline-d4	10.801	131	116138	13.982	ng/ul	0.00
46) Dimethylphthalate-d6	13.913	166	421331	23.653	ng/ul	0.00
49) Acenaphthylene-d8	14.195	160	438933	19.172	ng/ul	0.00
54) 4-Nitrophenol-d4	14.713	143	28528	10.503	ng/ul	0.00
60) Fluorene-d10	15.489	176	351664	22.845	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.613	200	56820	19.629	ng/ul	0.00
73) Anthracene-d10	17.342	188	606065	26.809	ng/ul	0.00
81) Pyrene-d10	19.636	212	783021	33.710	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.642	264	697962	30.809	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.684	105	11961	1.150	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
Data File : BM034706.D
Acq On : 15 Apr 2022 17:37
Operator : CG/JU
Sample : N2358-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETNS1


Quant Time: Apr 18 07:56:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 18 05:39:41 2022
Response via : Initial Calibration

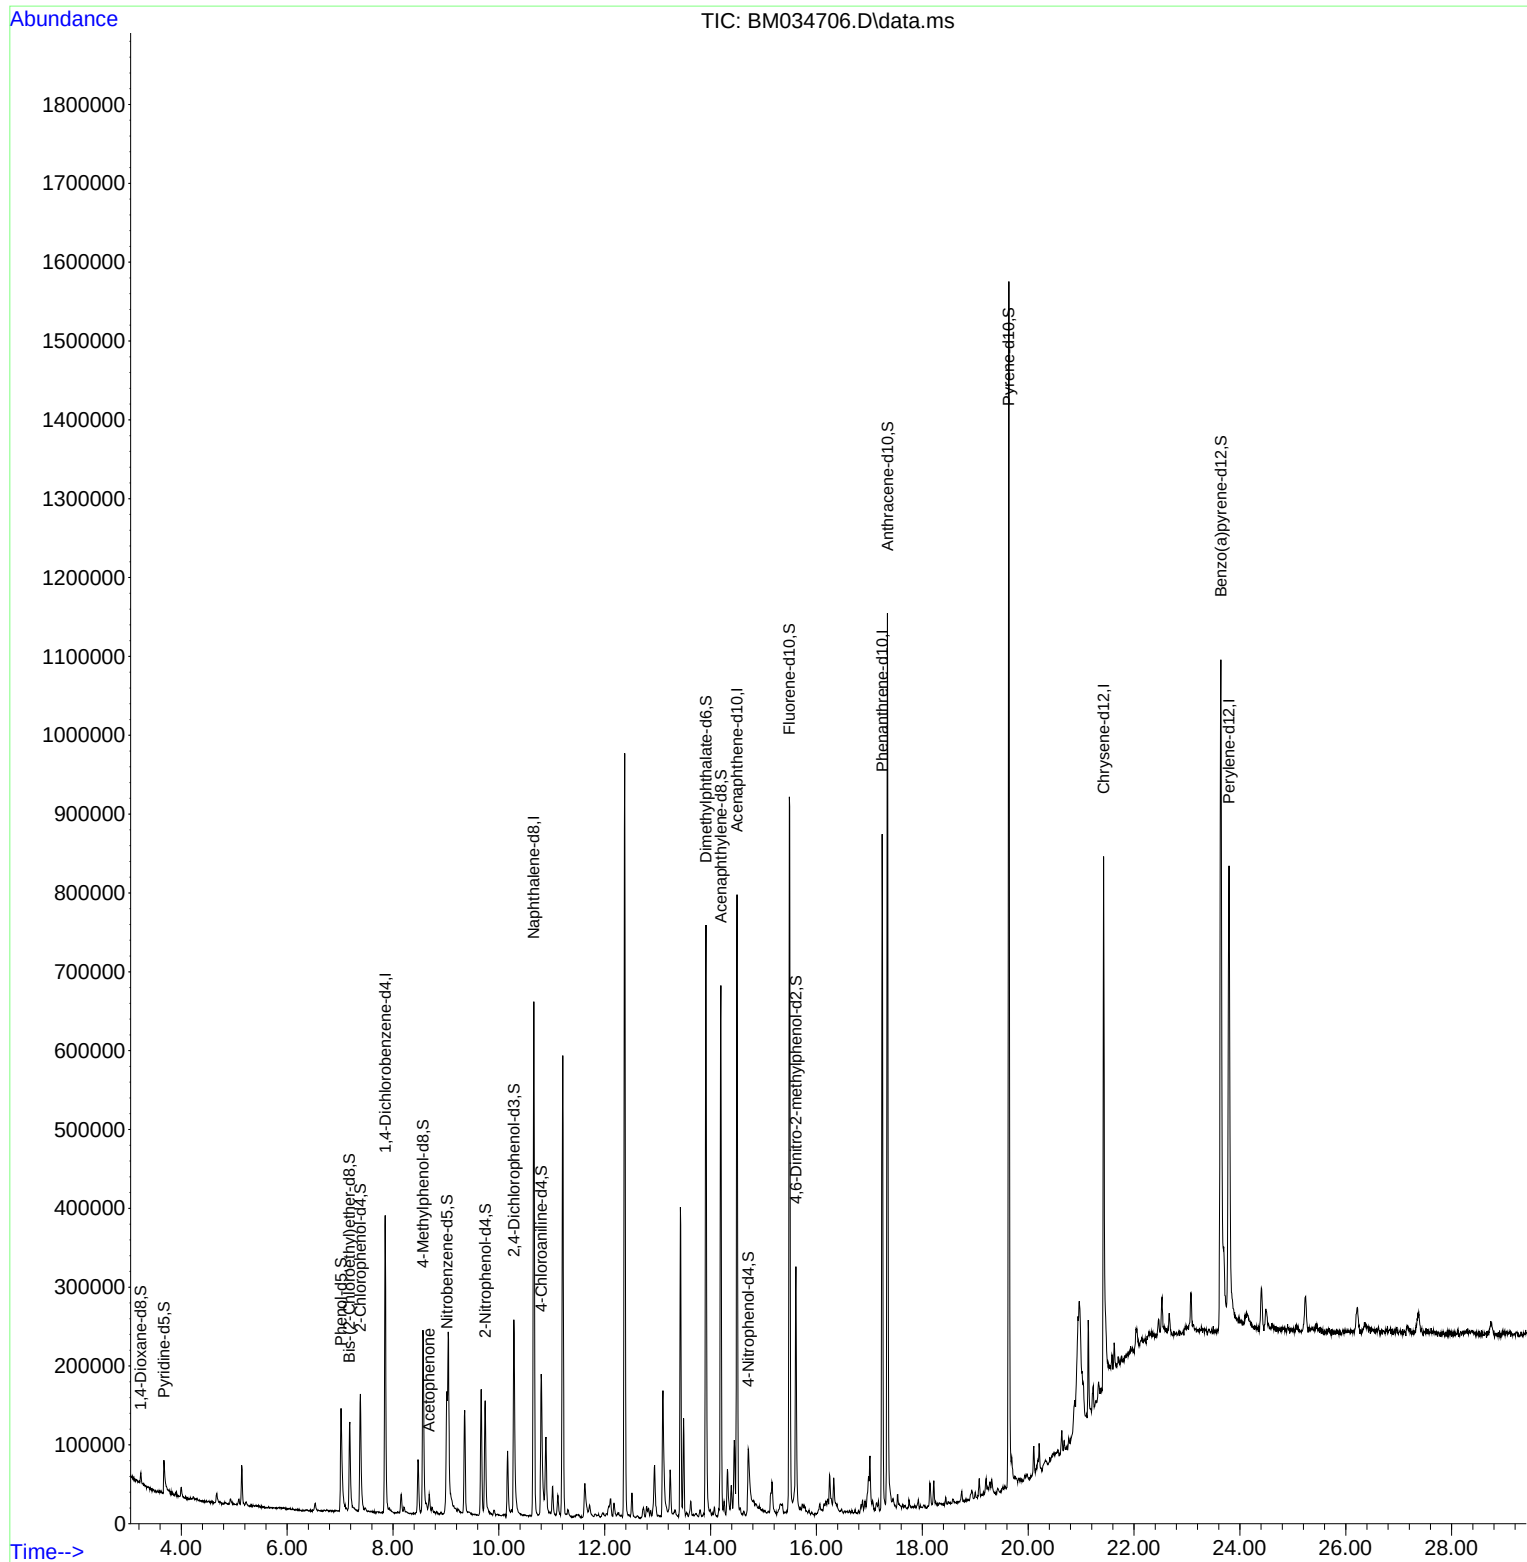

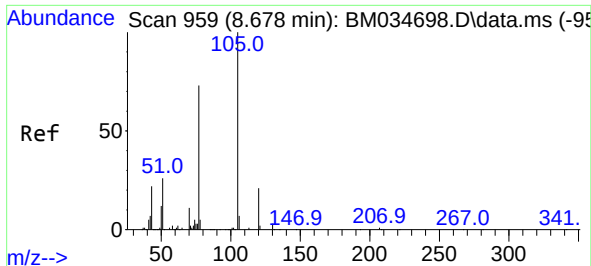

#16
 Acetophenone
 Concen: 1.150 ng/ul
 RT: 8.684 min Scan# 916
 Delta R.T. 0.006 min
 Lab File: BM034706.D
 Acq: 15 Apr 2022 17:37

Instrument :
 BNA_M
 ClientSampleId :
 ETNS1

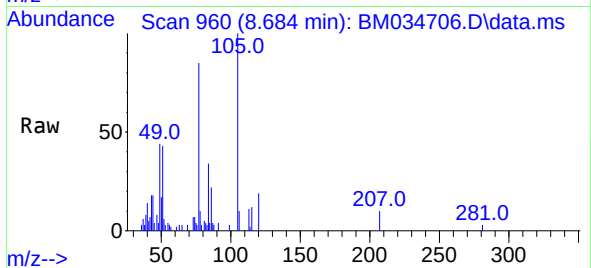

Tgt Ion:105 Resp: 11961
 Ion Ratio Lower Upper
 105 100
 77 84.8 59.4 89.2
 51 42.5 19.3 28.9#

