

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
 Data File : BM034701.D
 Acq On : 15 Apr 2022 14:37
 Operator : CG/JU
 Sample : N2280-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFFC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034701.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.672	106	108	115	rBV	38595	61703	6.98%	0.656%
2	4.925	319	321	327	rVB2	6816	8735	0.99%	0.093%
3	7.019	672	677	694	rBV	75578	185840	21.02%	1.975%
4	7.178	699	704	716	rBV	77915	154904	17.52%	1.646%
5	7.384	733	739	751	rBV	113230	216439	24.48%	2.300%
6	7.690	788	791	792	rVB3	1866	1724	0.19%	0.018%
7	7.701	792	793	796	rBV3	1742	2016	0.23%	0.021%
8	7.854	812	819	836	rBV	268263	491404	55.58%	5.223%
9	8.166	870	872	875	rVB3	1946	1635	0.18%	0.017%
10	8.495	926	928	933	rVB4	1627	1595	0.18%	0.017%
11	8.572	936	941	956	rVV2	80394	190479	21.54%	2.024%
12	8.695	957	962	974	rVB4	8823	22418	2.54%	0.238%
13	8.884	992	994	998	rBV4	1900	2245	0.25%	0.024%
14	8.948	1003	1005	1008	rVB3	2213	1904	0.22%	0.020%
15	9.019	1011	1017	1031	rBV	84609	185612	20.99%	1.973%
16	9.436	1084	1088	1089	rBV4	1867	2236	0.25%	0.024%
17	9.454	1089	1091	1097	rVB6	3936	4938	0.56%	0.052%
18	9.748	1134	1141	1150	rBV2	66135	140726	15.92%	1.496%
19	9.895	1165	1166	1170	rVB4	2265	2145	0.24%	0.023%
20	10.042	1189	1191	1193	rBV3	1513	1380	0.16%	0.015%
21	10.295	1228	1234	1244	rBV	61934	158641	17.94%	1.686%
22	10.495	1266	1268	1270	rVB2	2121	1822	0.21%	0.019%
23	10.560	1276	1279	1281	rBV3	2121	2182	0.25%	0.023%
24	10.601	1281	1286	1287	rBV5	1332	1886	0.21%	0.020%
25	10.660	1289	1296	1311	rBV	381481	669007	75.67%	7.110%
26	10.819	1317	1323	1342	rBV3	27850	122046	13.80%	1.297%
27	11.007	1354	1355	1358	rVB3	1671	1300	0.15%	0.014%
28	11.272	1397	1400	1402	rVB4	1479	1464	0.17%	0.016%
29	11.366	1414	1416	1420	rVB5	1297	1427	0.16%	0.015%
30	11.407	1420	1423	1426	rVB5	1687	1614	0.18%	0.017%
31	11.807	1487	1491	1494	rBV4	1579	1949	0.22%	0.021%
32	11.889	1503	1505	1508	rVB3	1957	1456	0.16%	0.015%
33	12.036	1527	1530	1534	rBV3	1897	3651	0.41%	0.039%
34	12.301	1573	1575	1579	rVV4	1650	1998	0.23%	0.021%
35	12.395	1586	1591	1593	rVB6	1226	1900	0.21%	0.020%
36	12.760	1652	1653	1657	rVB3	1384	1422	0.16%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
 Data File : BM034701.D
 Acq On : 15 Apr 2022 14:37
 Operator : CG/JU
 Sample : N2280-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFFC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	12.866	1667	1671	1672	rBV3	2201	2386	0.27%	0.025%
38	12.877	1672	1673	1676	rVB3	1970	1405	0.16%	0.015%
39	13.113	1709	1713	1714	rBV2	1871	1982	0.22%	0.021%
40	13.130	1714	1716	1719	rVB4	2777	3098	0.35%	0.033%

41	13.154	1719	1720	1722	rBV2	1536	1360	0.15%	0.014%
42	13.242	1734	1735	1739	rVB4	1431	1402	0.16%	0.015%
43	13.342	1749	1752	1758	rVB4	2522	3697	0.42%	0.039%
44	13.736	1818	1819	1822	rBV3	1594	1545	0.17%	0.016%
45	13.795	1826	1829	1831	rBV2	1668	1621	0.18%	0.017%

46	13.824	1831	1834	1840	rVB7	3924	6384	0.72%	0.068%
47	13.913	1843	1849	1860	rBV	190840	348816	39.45%	3.707%
48	14.077	1875	1877	1881	rVB5	1487	1426	0.16%	0.015%
49	14.113	1881	1883	1887	rBV3	1056	1543	0.17%	0.016%
50	14.195	1890	1897	1912	rBV	243926	400559	45.31%	4.257%

51	14.289	1912	1913	1920	rVB5	3042	4111	0.46%	0.044%
52	14.354	1923	1924	1931	rBV5	2579	4677	0.53%	0.050%
53	14.407	1931	1933	1938	rVB5	2192	2962	0.34%	0.031%
54	14.501	1942	1949	1959	rBV	544771	819764	92.72%	8.712%
55	14.713	1984	1985	1990	rVB4	1254	1512	0.17%	0.016%

56	14.766	1990	1994	1996	rBV4	2954	4669	0.53%	0.050%
57	14.842	2004	2007	2008	rBV3	1912	1302	0.15%	0.014%
58	14.930	2020	2022	2026	rBV5	1258	1422	0.16%	0.015%
59	15.124	2053	2055	2059	rVB4	1528	1579	0.18%	0.017%
60	15.313	2083	2087	2088	rVV3	3432	4026	0.46%	0.043%

61	15.495	2112	2118	2131	rBV	289950	519404	58.75%	5.520%
62	15.624	2134	2140	2149	rVV2	37667	75556	8.55%	0.803%
63	15.742	2158	2160	2165	rVB5	4078	5139	0.58%	0.055%
64	15.818	2171	2173	2175	rBV3	1588	1292	0.15%	0.014%
65	15.913	2187	2189	2190	rBV2	2003	1406	0.16%	0.015%

66	15.989	2199	2202	2204	rVB4	1169	1473	0.17%	0.016%
67	16.077	2215	2217	2223	rVB5	1549	1998	0.23%	0.021%
68	16.277	2249	2251	2252	rBV2	2628	1738	0.20%	0.018%
69	16.377	2264	2268	2269	rBV4	1563	1708	0.19%	0.018%
70	16.395	2269	2271	2273	rVV3	2487	1899	0.21%	0.020%

71	16.448	2277	2280	2281	rVV2	1856	2018	0.23%	0.021%
72	16.654	2312	2315	2321	rBV8	2685	5515	0.62%	0.059%
73	16.807	2339	2341	2343	rVB2	2425	1886	0.21%	0.020%
74	16.948	2362	2365	2366	rBV3	1533	1380	0.16%	0.015%
75	16.989	2371	2372	2376	rBV3	1962	1908	0.22%	0.020%

76	17.042	2380	2381	2385	rVB4	2201	1418	0.16%	0.015%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
 Data File : BM034701.D
 Acq On : 15 Apr 2022 14:37
 Operator : CG/JU
 Sample : N2280-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFFC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

77	17.112	2391	2393	2395	rBV3	1545	1300	0.15%	0.014%
78	17.165	2400	2402	2404	rBV3	1428	1565	0.18%	0.017%
79	17.183	2404	2405	2409	rVB4	2203	1903	0.22%	0.020%
80	17.242	2409	2415	2427	rBV	563614	884136	100.00%	9.397%
81	17.348	2427	2433	2451	rVB	263145	500927	56.66%	5.324%
82	17.512	2459	2461	2463	rVB3	2057	1328	0.15%	0.014%
83	17.718	2495	2496	2498	rBV2	2074	2036	0.23%	0.022%
84	17.777	2504	2506	2508	rVB3	2495	1614	0.18%	0.017%
85	17.865	2519	2521	2526	rVB6	2603	3035	0.34%	0.032%
86	17.930	2530	2532	2535	rVB4	3813	2868	0.32%	0.030%
87	18.148	2564	2569	2575	rBV7	12337	23235	2.63%	0.247%
88	18.212	2579	2580	2584	rVB4	3429	3385	0.38%	0.036%
89	18.601	2643	2646	2647	rBV3	1668	1778	0.20%	0.019%
90	18.677	2657	2659	2663	rBV4	2379	3736	0.42%	0.040%
91	18.724	2665	2667	2671	rVV5	5263	6906	0.78%	0.073%
92	18.865	2690	2691	2693	rBV2	2797	1967	0.22%	0.021%
93	19.206	2746	2749	2752	rVB4	5227	6375	0.72%	0.068%
94	19.283	2759	2762	2764	rBV4	4038	5359	0.61%	0.057%
95	19.636	2816	2822	2835	rBV	462341	744881	84.25%	7.917%
96	20.512	2969	2971	2975	rBV5	16385	18750	2.12%	0.199%
97	21.142	3075	3078	3083	rVB4	30343	37758	4.27%	0.401%
98	21.424	3122	3126	3141	rBV	406978	871111	98.53%	9.258%
99	23.641	3497	3503	3509	rBV2	236781	520749	58.90%	5.535%
100	23.794	3523	3529	3541	rVB2	386571	859561	97.22%	9.135%


Sum of corrected areas: 9409092

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
Data File : BM034701.D
Acq On : 15 Apr 2022 14:37
Operator : CG/JU
Sample : N2280-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFFC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

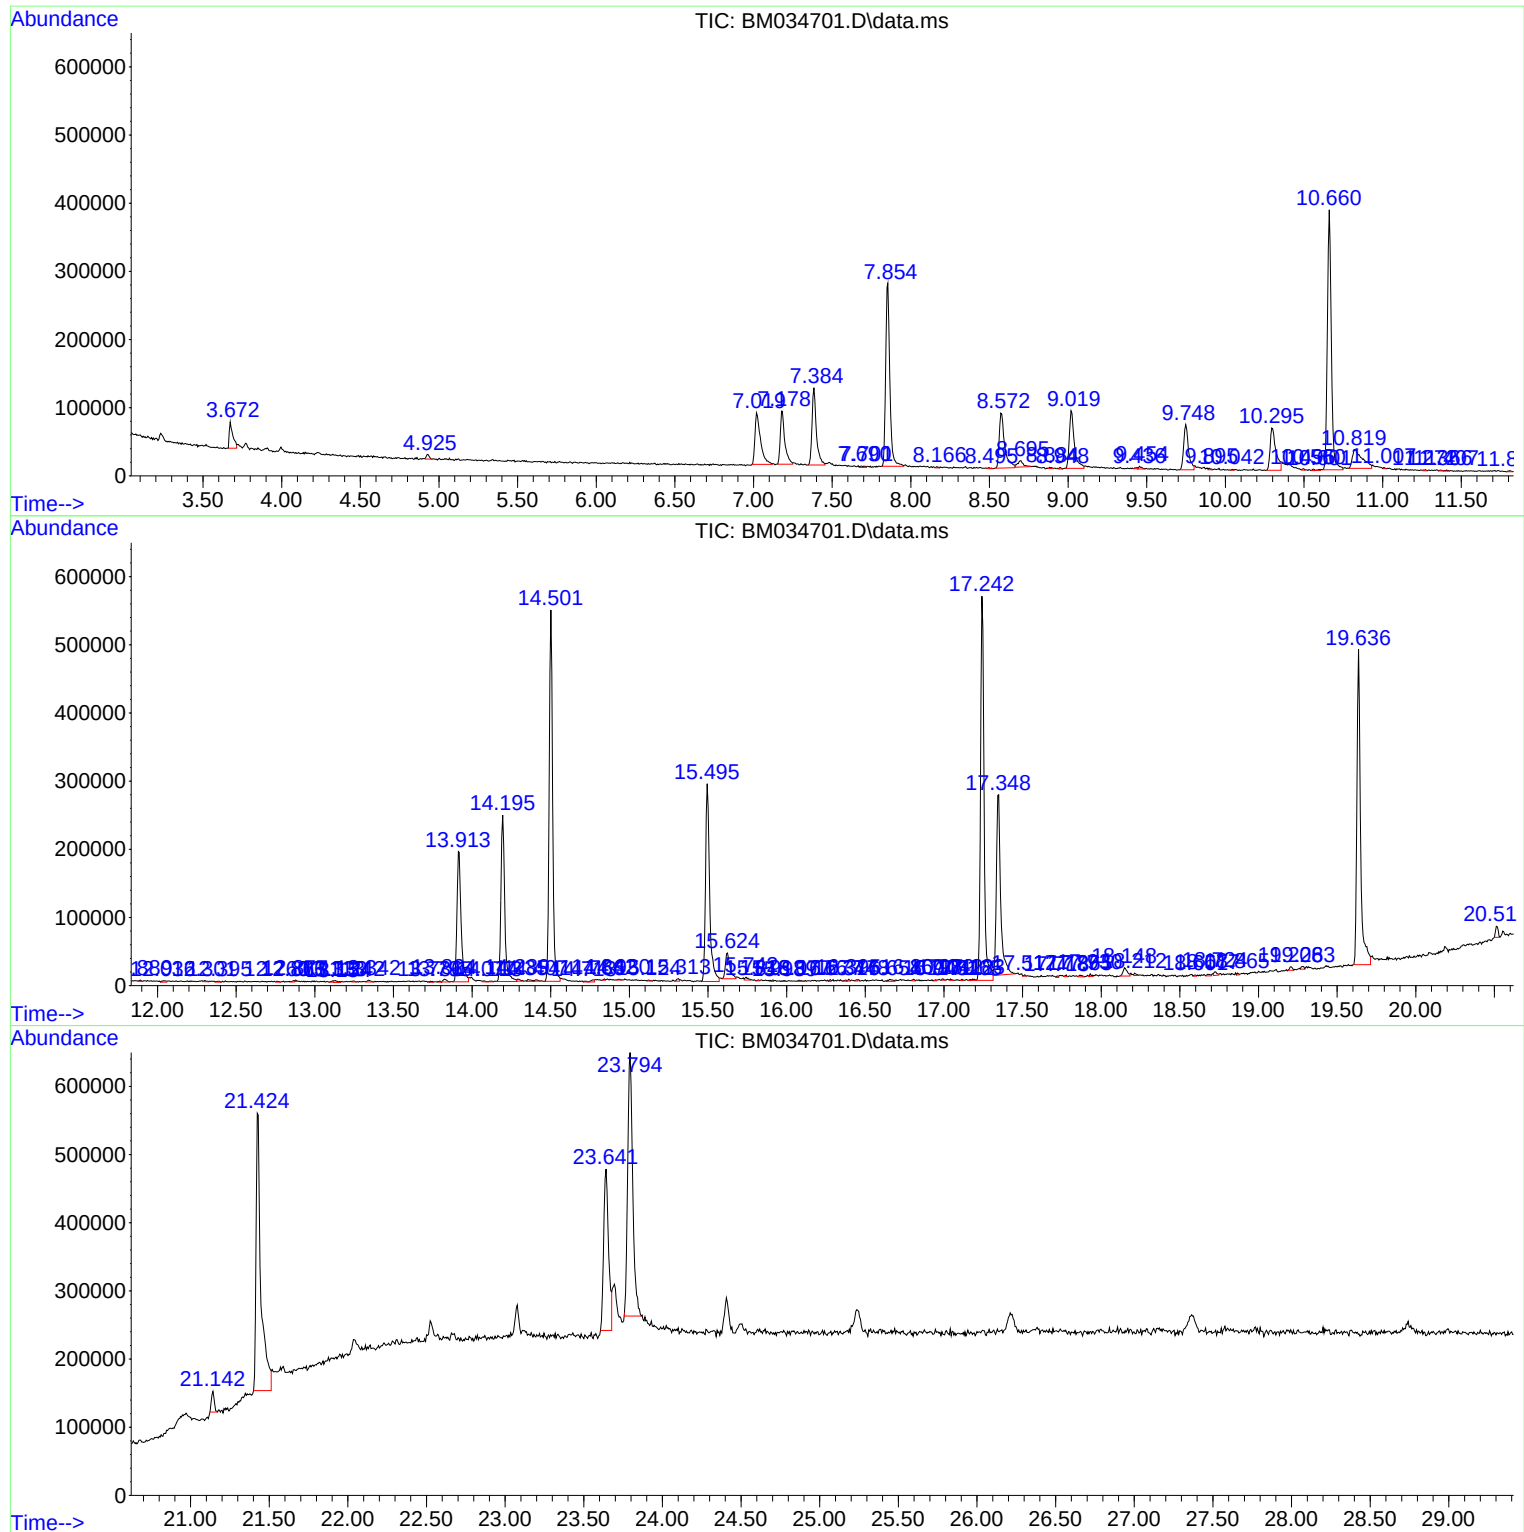

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
Data File : BM034701.D
Acq On : 15 Apr 2022 14:37
Operator : CG/JU
Sample : N2280-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFFC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
Data File : BM034701.D
Acq On : 15 Apr 2022 14:37
Operator : CG/JU
Sample : N2280-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFFC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------