

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
 Data File : BM034711.D
 Acq On : 15 Apr 2022 20:39
 Operator : CG/JU
 Sample : PB144121BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK121

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

Signal : TIC: BM034711.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.231	30	33	39	rVB	35107	44068	2.23%	0.253%
2	3.666	105	107	131	rBV	167475	394287	19.98%	2.266%
3	3.996	159	163	173	rVB	21911	35240	1.79%	0.202%
4	7.025	672	678	697	rBV	276712	599949	30.40%	3.447%
5	7.178	699	704	721	rVB	280739	506200	25.65%	2.909%
6	7.384	733	739	752	rBV	389125	684408	34.68%	3.933%
7	7.607	775	777	781	rVB5	2535	2828	0.14%	0.016%
8	7.854	812	819	836	rBV	338245	582684	29.53%	3.348%
9	8.407	911	913	916	rVB3	2799	2237	0.11%	0.013%
10	8.572	935	941	963	rBV	333672	719936	36.48%	4.137%
11	9.019	1010	1017	1029	rBV	307085	588380	29.81%	3.381%
12	9.183	1043	1045	1053	rVB8	2038	3634	0.18%	0.021%
13	9.342	1071	1072	1077	rVB5	1657	2230	0.11%	0.013%
14	9.748	1134	1141	1153	rBV	224243	455501	23.08%	2.617%
15	10.301	1228	1235	1259	rBV	222102	637340	32.30%	3.662%
16	10.660	1289	1296	1312	rBV	413924	755274	38.27%	4.340%
17	10.830	1318	1325	1351	rBV	63016	361066	18.30%	2.075%
18	11.613	1455	1458	1462	rVB6	1842	2464	0.12%	0.014%
19	11.848	1495	1498	1500	rVB4	2197	2167	0.11%	0.012%
20	11.883	1500	1504	1507	rBV5	2530	4456	0.23%	0.026%
21	12.024	1524	1528	1531	rBV6	1682	3007	0.15%	0.017%
22	12.101	1540	1541	1546	rVB5	1943	2534	0.13%	0.015%
23	12.219	1557	1561	1564	rBV5	1525	2202	0.11%	0.013%
24	12.289	1570	1573	1574	rBV3	4164	4637	0.23%	0.027%
25	12.871	1670	1672	1676	rVB5	2329	2081	0.11%	0.012%
26	13.183	1720	1725	1728	rBV6	1688	2982	0.15%	0.017%
27	13.289	1739	1743	1744	rBV4	1879	2240	0.11%	0.013%
28	13.454	1768	1771	1772	rVV3	2454	2189	0.11%	0.013%
29	13.918	1843	1850	1874	rBV	614306	1087561	55.11%	6.249%
30	14.195	1886	1897	1912	rBV	780148	1258439	63.77%	7.231%
31	14.501	1942	1949	1970	rBV	609739	961250	48.71%	5.524%
32	14.789	1991	1998	2000	rBV4	14031	31552	1.60%	0.181%
33	15.207	2064	2069	2071	rBV5	2540	3883	0.20%	0.022%
34	15.312	2085	2087	2090	rVB3	2649	2830	0.14%	0.016%
35	15.495	2111	2118	2135	rBV	844090	1558427	78.97%	8.955%
36	15.630	2136	2141	2151	rVB2	81295	156646	7.94%	0.900%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
 Data File : BM034711.D
 Acq On : 15 Apr 2022 20:39
 Operator : CG/JU
 Sample : PB144121BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK121

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
 Title : SVOA CALIBRATION

37	15.748	2156	2161	2167	rVB6	9371	20339	1.03%	0.117%
38	16.001	2202	2204	2208	rVB4	3200	3381	0.17%	0.019%
39	16.742	2328	2330	2334	rVV5	1476	2585	0.13%	0.015%
40	17.248	2410	2416	2427	rBV	656661	1055377	53.48%	6.065%
41	17.348	2427	2433	2449	rVV	857748	1544940	78.29%	8.878%
42	17.548	2465	2467	2468	rVB2	3294	2062	0.10%	0.012%
43	17.818	2511	2513	2518	rVB6	2905	3508	0.18%	0.020%
44	18.653	2651	2655	2657	rVV5	2522	3070	0.16%	0.018%
45	19.212	2746	2750	2753	rBV5	11182	15758	0.80%	0.091%
46	19.283	2758	2762	2766	rBV4	9790	17945	0.91%	0.103%
47	19.642	2817	2823	2843	rBV	1099882	1973479	100.00%	11.340%
48	21.441	3124	3129	3145	rBV	248697	882664	44.73%	5.072%
49	23.659	3502	3506	3524	rBV2	114318	410556	20.80%	2.359%




Sum of corrected areas: 17402473

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
Data File : BM034711.D
Acq On : 15 Apr 2022 20:39
Operator : CG/JU
Sample : PB144121BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

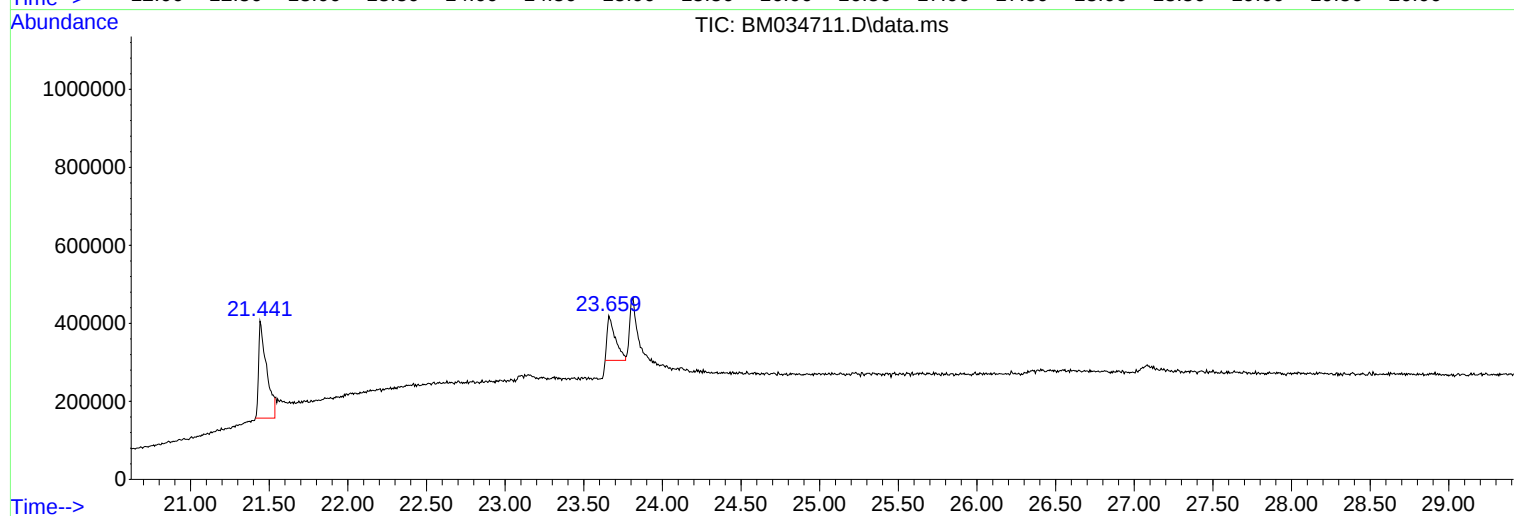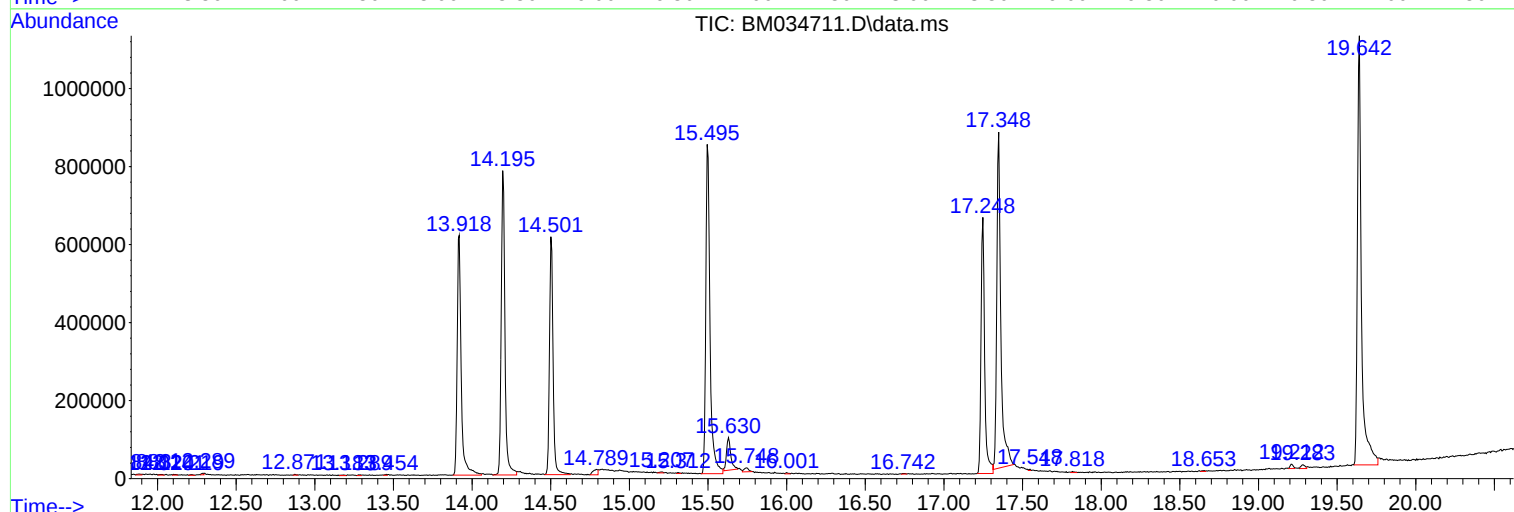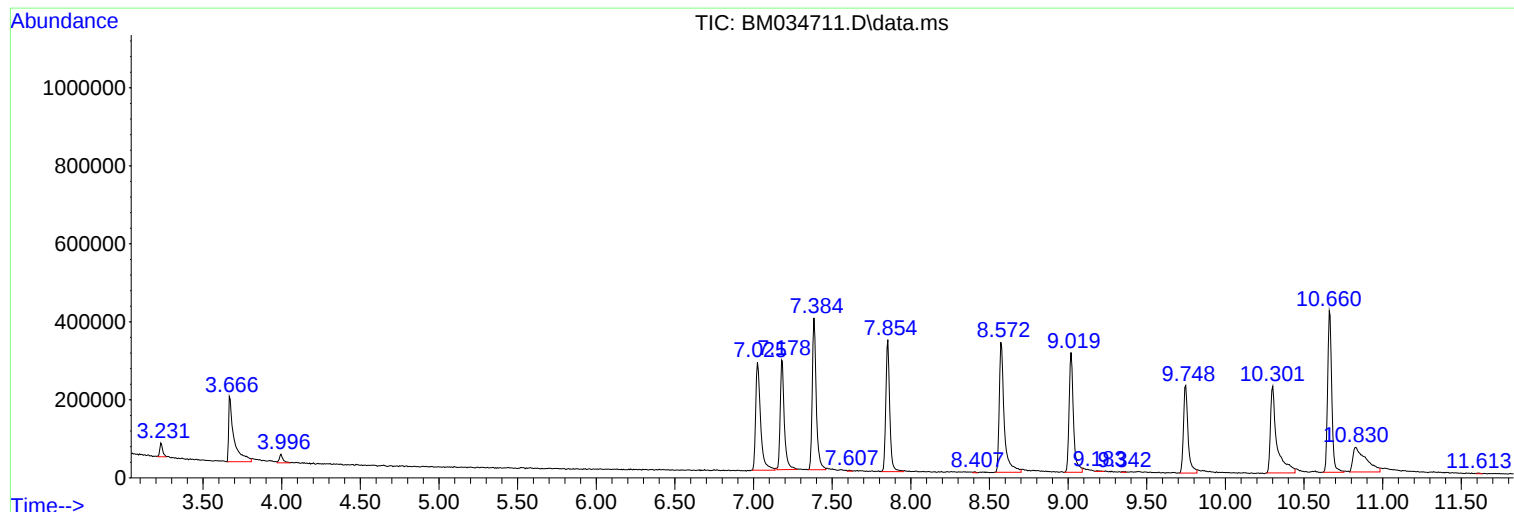

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
Data File : BM034711.D
Acq On : 15 Apr 2022 20:39
Operator : CG/JU
Sample : PB144121BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041522\
Data File : BM034711.D
Acq On : 15 Apr 2022 20:39
Operator : CG/JU
Sample : PB144121BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040922.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc