




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045280.D
Acq On : 16 Apr 2024 14:28
Operator : MA/JU
Sample : P2032-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMF2

Manual IntegrationsAPPROVED

Quant Time: Apr 16 15:33:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 15 22:24:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/17/2024
Supervised By :mohammad ahmed 04/18/2024

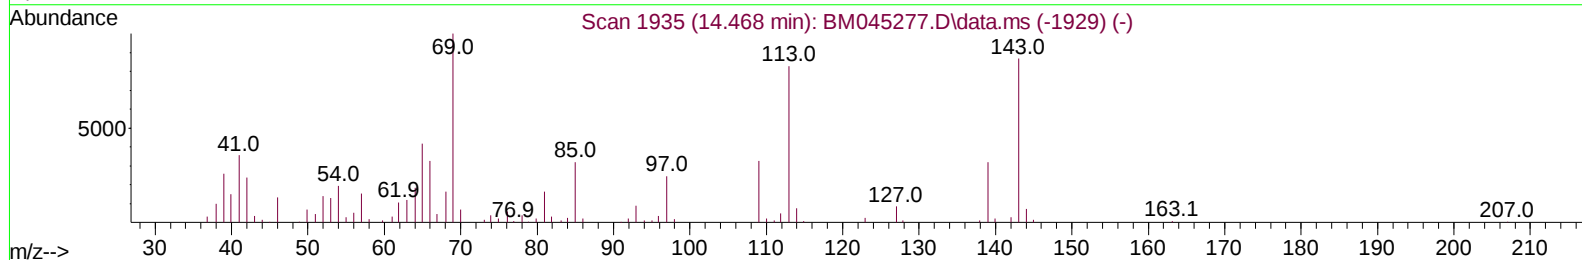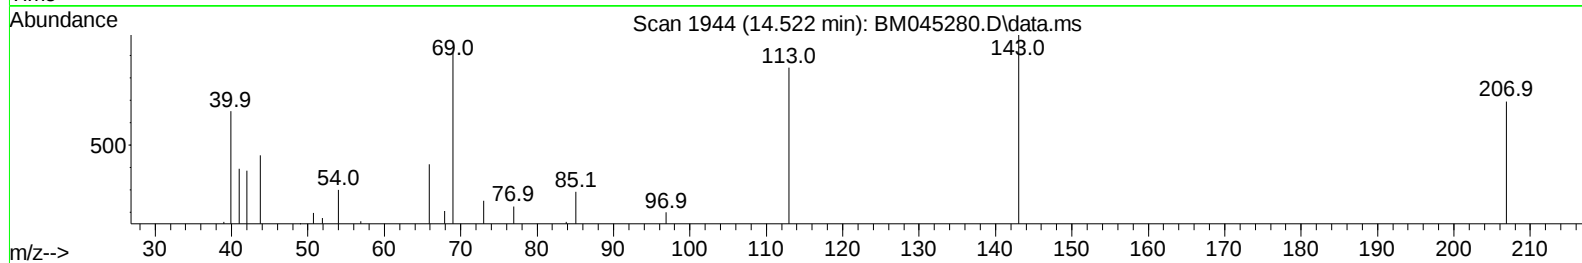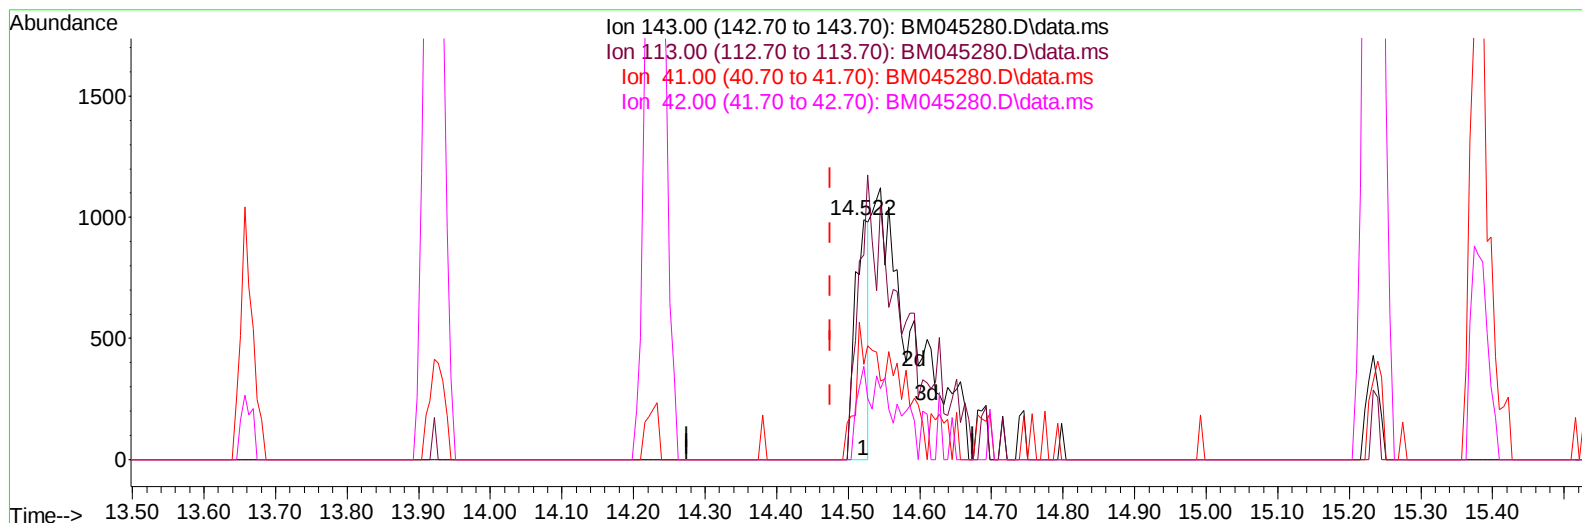

TIC: BM045280.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.522min (+ 0.047) 0.62 ng/u1

response 1347

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	85.37
41.00	36.50	39.76
42.00	23.30	38.95#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045280.D
Acq On : 16 Apr 2024 14:28
Operator : MA/JU
Sample : P2032-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MF2

Manual IntegrationsAPPROVED

Quant Time: Apr 16 15:33:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 15 22:24:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/17/2024
Supervised By :mohammad ahmed 04/18/2024

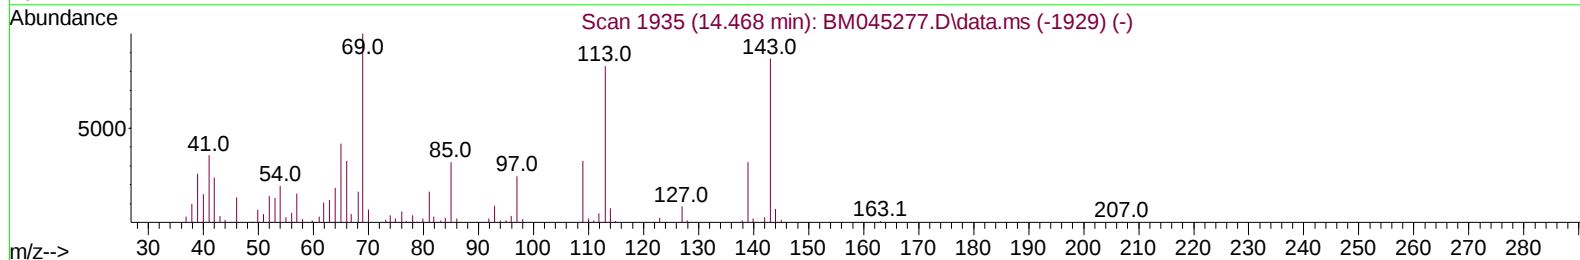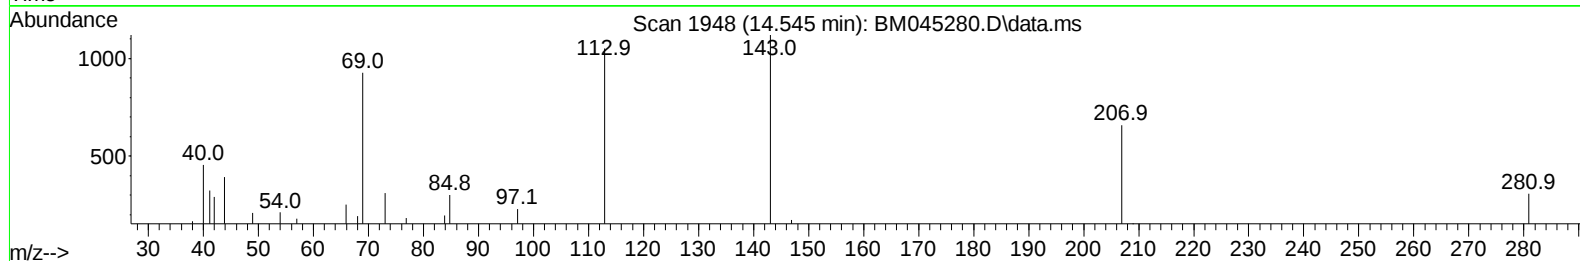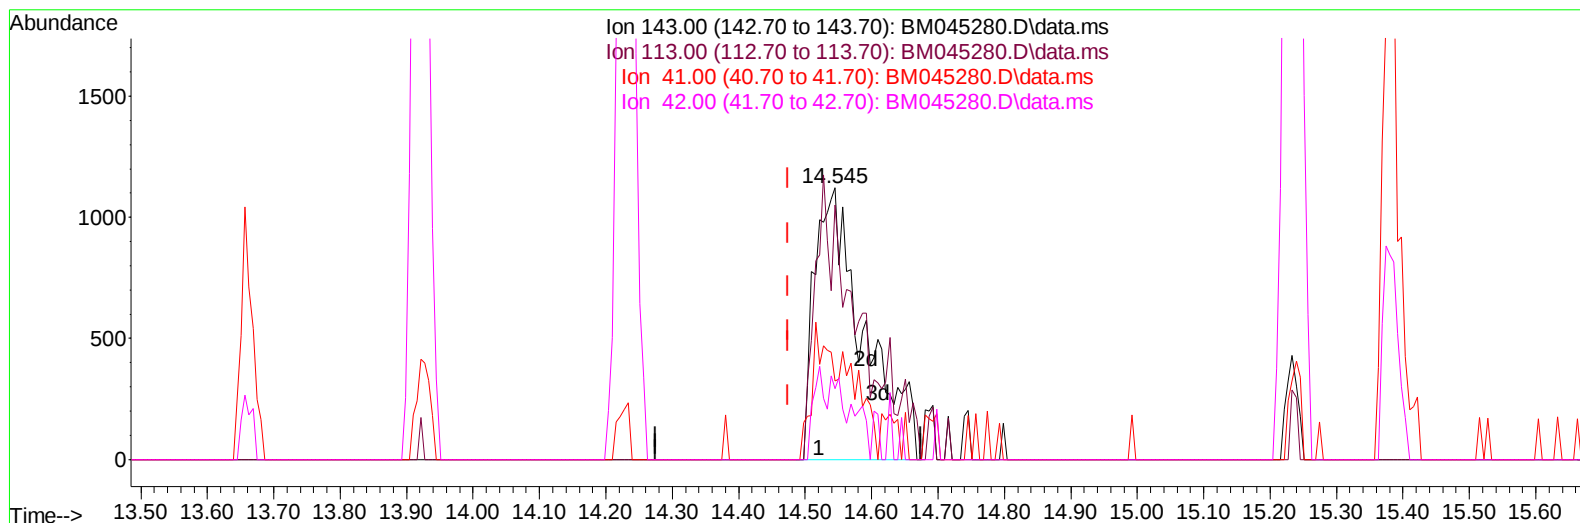

TIC: BM045280.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.545min (+ 0.071) 2.65 ng/ul m

response 5786

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.80	93.84
41.00	36.50	28.99#
42.00	23.30	26.05

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045280.D
 Acq On : 16 Apr 2024 14:28
 Operator : MA/JU
 Sample : P2032-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0MF2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/17/2024
 Supervised By :mohammad ahmed 04/18/2024

Quant Time: Apr 16 15:34:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 15 22:24:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	63537	20.000	ng/ul	0.00
20) Naphthalene-d8	10.351	136	252970	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.233	164	150269	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.992	188	310487	20.000	ng/ul	0.00
79) Chrysene-d12	21.203	240	342685	20.000	ng/ul	0.00
88) Perylene-d12	23.403	264	446771	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	5450	3.203	ng/uL	0.00
4) Pyridine-d5	3.587	84	22610	4.887	ng/ul	0.00
7) Phenol-d5	6.769	99	23655	4.392	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.940	67	85373	26.603	ng/ul	0.00
11) 2-Chlorophenol-d4	7.116	132	85079	20.161	ng/ul	0.00
15) 4-Methylphenol-d8	8.293	113	47243	11.205	ng/ul	0.00
21) Nitrobenzene-d5	8.745	128	52366	26.949	ng/ul	0.00
24) 2-Nitrophenol-d4	9.457	143	53331	26.003	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.987	165	78587	20.899	ng/ul	0.00
31) 4-Chloroaniline-d4	10.516	131	108607	18.141	ng/ul	0.00
46) Dimethylphthalate-d6	13.663	166	305309	29.180	ng/ul	0.00
49) Acenaphthylene-d8	13.922	160	351190	28.412	ng/ul	0.00
54) 4-Nitrophenol-d4	14.545	143	5786m	2.650	ng/ul	0.07
60) Fluorene-d10	15.233	176	271438	29.100	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.380	200	37442	20.338	ng/ul	0.00
73) Anthracene-d10	17.092	188	437407	31.316	ng/ul	0.00
81) Pyrene-d10	19.398	212	527840	31.282	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.268	264	677245	31.074	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045280.D
Acq On : 16 Apr 2024 14:28
Operator : MA/JU
Sample : P2032-06
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MF2

Manual IntegrationsAPPROVED

Quant Time: Apr 16 15:34:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 15 22:24:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/17/2024
Supervised By :mohammad ahmed 04/18/2024

