

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045246.D
 Acq On : 15 Apr 2024 16:13
 Operator : MA/JU
 Sample : PB160235BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045246.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	22	rVB2	12825	16673	1.58%	0.168%
2	3.469	62	65	67	rBV4	1595	2049	0.19%	0.021%
3	3.540	76	77	80	rVB3	1838	1180	0.11%	0.012%
4	3.575	80	83	95	rBV	142378	239835	22.67%	2.415%
5	3.875	130	134	137	rBV4	2250	3193	0.30%	0.032%
6	3.969	147	150	154	rVB5	1009	1299	0.12%	0.013%
7	4.075	166	168	171	rVB3	1278	1122	0.11%	0.011%
8	4.122	173	176	181	rVB5	1842	2571	0.24%	0.026%
9	4.487	234	238	241	rVB5	925	1411	0.13%	0.014%
10	4.522	241	244	248	rBV5	882	1285	0.12%	0.013%
11	4.593	254	256	259	rBV3	1513	1369	0.13%	0.014%
12	4.787	287	289	293	rBV4	882	1115	0.11%	0.011%
13	4.881	304	305	307	rBV2	1073	1082	0.10%	0.011%
14	5.393	388	392	394	rBV4	857	1111	0.10%	0.011%
15	5.569	419	422	426	rVV4	911	1281	0.12%	0.013%
16	6.310	544	548	550	rBV3	970	1289	0.12%	0.013%
17	6.416	563	566	570	rVB5	820	1277	0.12%	0.013%
18	6.693	612	613	620	rVB3	1558	2263	0.21%	0.023%
19	6.769	620	626	637	rBV	176603	310318	29.33%	3.124%
20	6.940	650	655	665	rBV	146693	245184	23.17%	2.468%
21	7.122	678	686	699	rBV	200582	330897	31.27%	3.331%
22	7.345	722	724	728	rBV3	906	1177	0.11%	0.012%
23	7.587	759	765	777	rVB	133693	224846	21.25%	2.264%
24	7.663	777	778	783	rVB2	1356	1493	0.14%	0.015%
25	7.969	828	830	833	rVB3	978	1156	0.11%	0.012%
26	8.298	879	886	901	rBV	203058	362948	34.30%	3.654%
27	8.751	956	963	976	rBV	161502	292235	27.62%	2.942%
28	9.034	1009	1011	1015	rVV4	908	1118	0.11%	0.011%
29	9.463	1076	1084	1096	rBV	140743	246941	23.34%	2.486%
30	9.916	1160	1161	1164	rBV2	1065	1072	0.10%	0.011%
31	9.992	1167	1174	1183	rBV	185050	333520	31.52%	3.358%
32	10.151	1199	1201	1205	rVB4	1099	1245	0.12%	0.013%
33	10.357	1229	1236	1246	rBV	175321	286465	27.07%	2.884%
34	10.522	1257	1264	1288	rBV	143251	356485	33.69%	3.589%
35	10.716	1296	1297	1302	rVB3	968	1256	0.12%	0.013%
36	10.833	1314	1317	1321	rBV4	1128	1175	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045246.D
 Acq On : 15 Apr 2024 16:13
 Operator : MA/JU
 Sample : PB160235BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	10.875	1321	1324	1326	rBV3	820	1151	0.11%	0.012%
38	11.698	1463	1464	1467	rVB3	1178	1116	0.11%	0.011%
39	11.992	1511	1514	1515	rBV4	1439	1357	0.13%	0.014%
40	13.133	1705	1708	1713	rVB5	2371	4015	0.38%	0.040%

41	13.533	1773	1776	1780	rVB5	743	1066	0.10%	0.011%
42	13.669	1792	1799	1810	rBV	316310	487074	46.03%	4.904%
43	13.804	1821	1822	1828	rBV4	926	1587	0.15%	0.016%
44	13.927	1836	1843	1856	rBV	403661	589034	55.67%	5.930%
45	14.145	1877	1880	1884	rBV4	767	1436	0.14%	0.014%

46	14.239	1887	1896	1904	rVB	233130	345148	32.62%	3.475%
47	14.486	1931	1938	1960	rBV	65339	194514	18.38%	1.958%
48	14.651	1964	1966	1972	rVB6	1442	2476	0.23%	0.025%
49	15.239	2058	2066	2073	rBV	489379	721305	68.17%	7.262%
50	15.386	2085	2091	2105	rVV	115981	193816	18.32%	1.951%

51	15.480	2105	2107	2112	rVB3	2165	2745	0.26%	0.028%
52	15.733	2145	2150	2151	rVB2	889	1268	0.12%	0.013%
53	16.027	2198	2200	2204	rBV3	1536	1647	0.16%	0.017%
54	16.727	2314	2319	2323	rBV4	1064	2236	0.21%	0.023%
55	16.998	2359	2365	2374	rVV	288236	386093	36.49%	3.887%

56	17.098	2376	2382	2398	rVV2	501325	759906	71.82%	7.650%
57	17.210	2398	2401	2402	rVB2	1313	1173	0.11%	0.012%
58	17.286	2412	2414	2417	rVV3	977	1244	0.12%	0.013%
59	17.704	2482	2485	2487	rBV2	1306	1422	0.13%	0.014%
60	17.762	2492	2495	2497	rVB3	1311	1649	0.16%	0.017%

61	17.845	2504	2509	2512	rBV5	854	1624	0.15%	0.016%
62	17.921	2518	2522	2529	rBV5	10475	20227	1.91%	0.204%
63	18.180	2564	2566	2571	rVB3	1589	1424	0.13%	0.014%
64	18.968	2697	2700	2706	rVB4	5984	7808	0.74%	0.079%
65	19.015	2706	2708	2710	rBV2	1559	1418	0.13%	0.014%

66	19.051	2710	2714	2720	rVV3	2880	5224	0.49%	0.053%
67	19.209	2737	2741	2746	rBV5	6288	11878	1.12%	0.120%
68	19.286	2751	2754	2755	rBV2	1983	1923	0.18%	0.019%
69	19.404	2768	2774	2785	rBV	626247	878469	83.02%	8.844%
70	19.656	2815	2817	2819	rBV2	1646	1867	0.18%	0.019%

71	19.739	2828	2831	2832	rBV3	2325	2581	0.24%	0.026%
72	19.886	2854	2856	2858	rBV2	2638	2124	0.20%	0.021%
73	19.968	2868	2870	2873	rVB4	1786	1756	0.17%	0.018%
74	20.009	2875	2877	2878	rVV	1548	1059	0.10%	0.011%
75	20.398	2941	2943	2944	rBV2	3148	1596	0.15%	0.016%

76	21.215	3077	3082	3092	rBV	291965	435622	41.17%	4.386%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045246.D
Acq On : 15 Apr 2024 16:13
Operator : MA/JU
Sample : PB160235BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK235

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

77	23.274	3426	3432	3439	rBV	609856	1058120	100.00%	10.653%
78	23.421	3450	3457	3465	rBV	248136	512652	48.45%	5.161%




Sum of corrected areas: 9932786

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045246.D
Acq On : 15 Apr 2024 16:13
Operator : MA/JU
Sample : PB160235BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

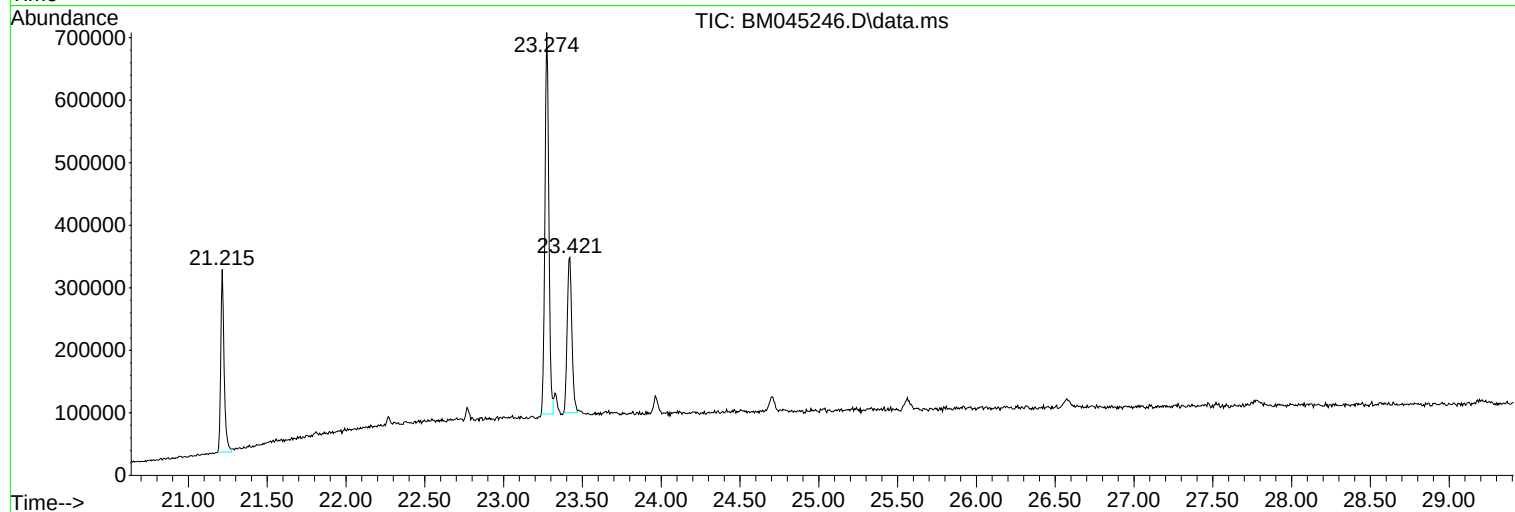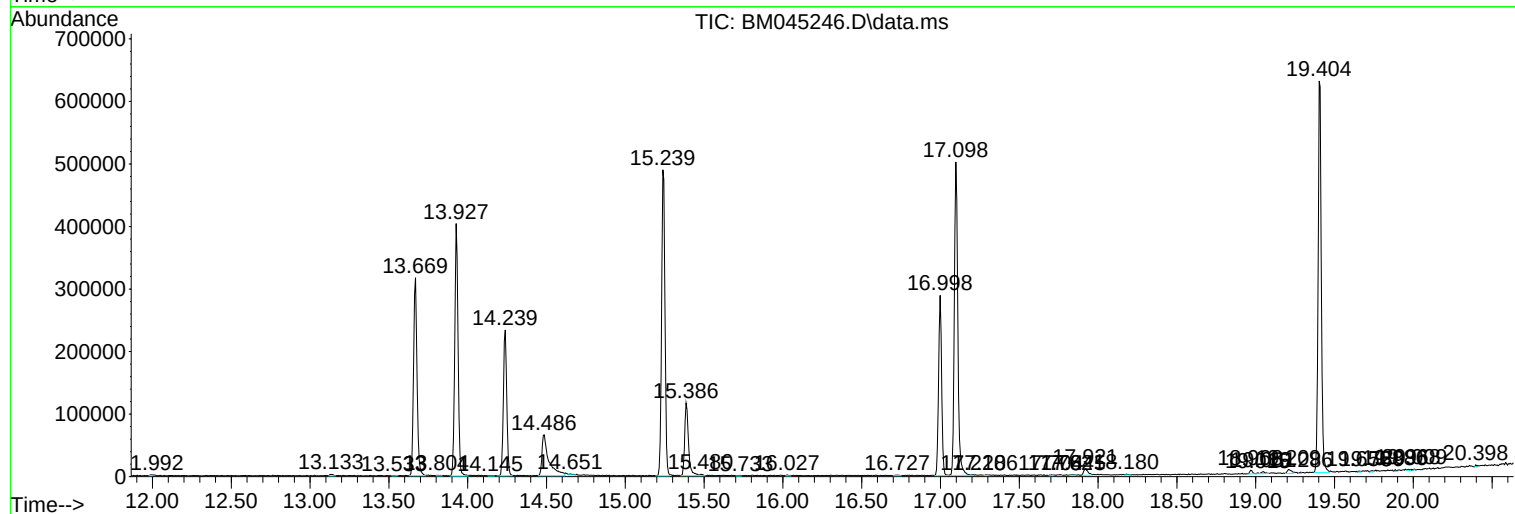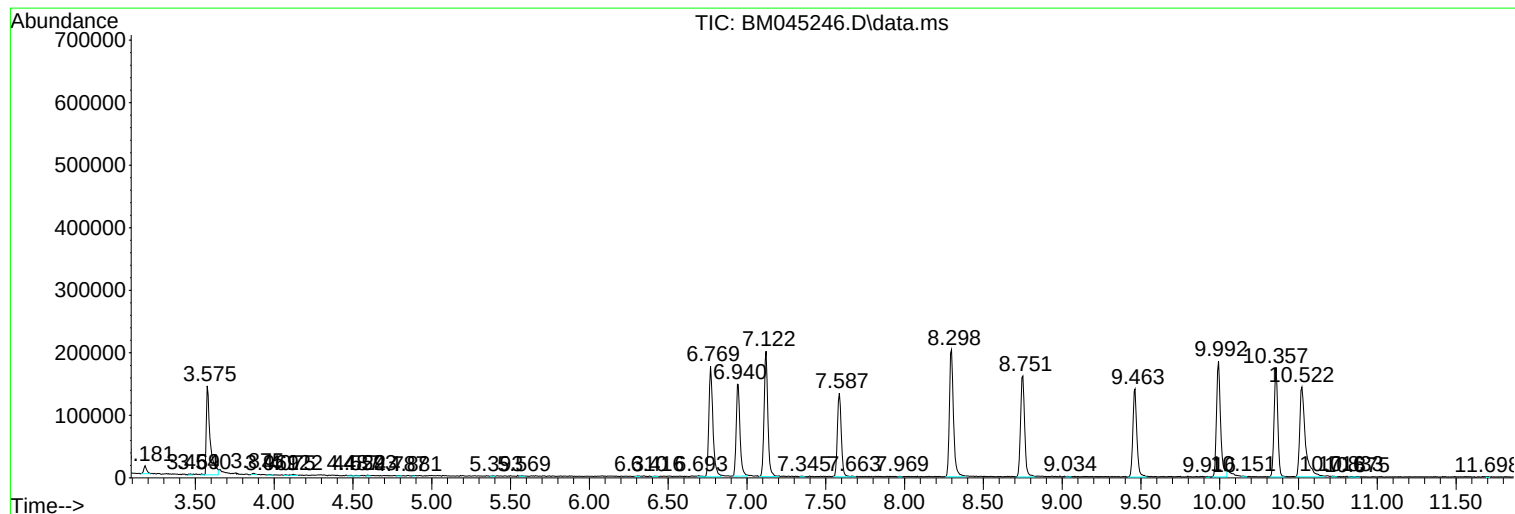

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045246.D
Acq On : 15 Apr 2024 16:13
Operator : MA/JU
Sample : PB160235BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045246.D
Acq On : 15 Apr 2024 16:13
Operator : MA/JU
Sample : PB160235BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK235

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------