

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045248.D
 Acq On : 15 Apr 2024 17:28
 Operator : MA/JU
 Sample : P2051-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CORH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	14	17	22	rVB2	8568	12015	0.83%	0.106%
2	3.404	52	54	57	rVB3	1920	1562	0.11%	0.014%
3	3.593	83	86	97	rBV	31535	62260	4.30%	0.551%
4	3.869	130	133	139	rBV4	3474	4864	0.34%	0.043%
5	4.240	192	196	199	rVB5	1380	2050	0.14%	0.018%
6	4.287	202	204	210	rVB5	2073	3720	0.26%	0.033%
7	4.487	236	238	241	rVB4	1446	1461	0.10%	0.013%
8	4.957	314	318	325	rVB6	3359	6408	0.44%	0.057%
9	5.093	339	341	344	rVB3	1570	1655	0.11%	0.015%
10	6.692	612	613	620	rBV3	1260	1865	0.13%	0.017%
11	6.775	622	627	636	rBV	24046	50909	3.52%	0.451%
12	6.945	649	656	665	rBV	158004	258063	17.84%	2.286%
13	7.122	679	686	701	rBV	144643	247750	17.13%	2.194%
14	7.475	742	746	748	rBV3	1238	1496	0.10%	0.013%
15	7.586	758	765	777	rBV	186671	312721	21.62%	2.770%
16	7.934	820	824	829	rVB5	4447	7324	0.51%	0.065%
17	8.304	880	887	900	rBV	82068	157127	10.86%	1.392%
18	8.751	956	963	976	rBV	172255	306472	21.19%	2.714%
19	9.116	1020	1025	1028	rVB5	1094	1747	0.12%	0.015%
20	9.463	1078	1084	1098	rBV	137121	240893	16.65%	2.134%
21	9.992	1167	1174	1196	rBV	165085	336663	23.27%	2.982%
22	10.357	1229	1236	1245	rVV	235663	393213	27.18%	3.483%
23	10.422	1245	1247	1252	rVB4	1405	1552	0.11%	0.014%
24	10.522	1257	1264	1285	rBV	106741	272137	18.81%	2.410%
25	10.739	1297	1301	1308	rVB5	4378	6795	0.47%	0.060%
26	11.186	1372	1377	1379	rBV2	1557	2020	0.14%	0.018%
27	11.986	1510	1513	1517	rBV3	1701	2641	0.18%	0.023%
28	13.027	1687	1690	1691	rBV2	1714	1718	0.12%	0.015%
29	13.063	1691	1696	1702	rVV7	10399	16875	1.17%	0.149%
30	13.127	1702	1707	1713	rVB3	2221	4476	0.31%	0.040%
31	13.268	1726	1731	1735	rVB2	4386	6762	0.47%	0.060%
32	13.668	1792	1799	1807	rBV	354967	549731	38.00%	4.869%
33	13.733	1807	1810	1814	rVV4	3378	5512	0.38%	0.049%
34	13.927	1836	1843	1852	rBV	442809	647798	44.78%	5.737%
35	14.015	1855	1858	1863	rVB3	1709	2297	0.16%	0.020%
36	14.233	1890	1895	1904	rBV	323239	479012	33.11%	4.242%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045248.D
Acq On : 15 Apr 2024 17:28
Operator : MA/JU
Sample : P2051-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CORH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	14.539	1938	1947	1949	rBV5	5404	10360	0.72%	0.092%
38	15.239	2060	2066	2079	rBV	561787	823664	56.94%	7.295%
39	15.386	2086	2091	2103	rBV	150483	238188	16.47%	2.110%
40	15.798	2158	2161	2164	rVB2	1411	1692	0.12%	0.015%
41	15.821	2164	2165	2168	rBV2	1620	1645	0.11%	0.015%
42	15.986	2187	2193	2197	rBV6	3047	5633	0.39%	0.050%
43	16.433	2264	2269	2270	rBV4	1734	3028	0.21%	0.027%
44	16.462	2272	2274	2277	rVB3	1629	1573	0.11%	0.014%
45	16.621	2300	2301	2304	rBV3	1722	1914	0.13%	0.017%
46	16.768	2323	2326	2327	rBV2	2375	1512	0.10%	0.013%
47	16.798	2329	2331	2332	rVV	2610	2012	0.14%	0.018%
48	16.815	2332	2334	2338	rVB5	3146	3389	0.23%	0.030%
49	16.933	2349	2354	2359	rBV4	2624	5157	0.36%	0.046%
50	16.998	2359	2365	2373	rVV	403901	554993	38.37%	4.915%
51	17.098	2376	2382	2394	rVV	659697	929990	64.29%	8.237%
52	17.239	2405	2406	2410	rVB4	2463	2830	0.20%	0.025%
53	17.286	2410	2414	2415	rBV3	1767	2304	0.16%	0.020%
54	17.304	2415	2417	2421	rBV3	1212	1680	0.12%	0.015%
55	17.415	2435	2436	2440	rVB3	2491	2281	0.16%	0.020%
56	17.456	2440	2443	2446	rBV4	1738	1811	0.13%	0.016%
57	17.592	2465	2466	2469	rBV3	1652	1794	0.12%	0.016%
58	17.680	2478	2481	2482	rBV3	2173	1758	0.12%	0.016%
59	17.780	2496	2498	2499	rBV2	1970	1474	0.10%	0.013%
60	17.909	2516	2520	2528	rBV3	29854	46008	3.18%	0.407%
61	18.062	2545	2546	2548	rBV2	2086	1525	0.11%	0.014%
62	18.209	2568	2571	2573	rVB3	1884	1760	0.12%	0.016%
63	18.239	2573	2576	2578	rBV3	1945	1998	0.14%	0.018%
64	18.262	2578	2580	2582	rVV3	2481	1568	0.11%	0.014%
65	18.345	2591	2594	2598	rVB5	2585	2935	0.20%	0.026%
66	18.462	2612	2614	2617	rVB4	1920	1795	0.12%	0.016%
67	18.527	2624	2625	2628	rVB2	2872	2385	0.16%	0.021%
68	18.650	2644	2646	2649	rBV3	2364	1805	0.12%	0.016%
69	18.674	2649	2650	2653	rVV3	2508	1788	0.12%	0.016%
70	18.774	2666	2667	2669	rBV2	2320	2333	0.16%	0.021%
71	18.968	2696	2700	2704	rBV5	8384	9632	0.67%	0.085%
72	19.045	2710	2713	2717	rVV4	6074	8449	0.58%	0.075%
73	19.086	2717	2720	2722	rVV5	3043	3754	0.26%	0.033%
74	19.109	2722	2724	2728	rVB5	2899	3154	0.22%	0.028%
75	19.209	2736	2741	2748	rBV4	18626	31672	2.19%	0.281%
76	19.356	2763	2766	2768	rBV4	3366	2791	0.19%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045248.D
Acq On : 15 Apr 2024 17:28
Operator : MA/JU
Sample : P2051-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RH8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

77	19.403	2768	2774	2784	rVV	802619	1106265	76.48%	9.798%
78	19.568	2799	2802	2803	rBV3	2353	2002	0.14%	0.018%
79	20.939	3032	3035	3039	rBV5	14533	22636	1.56%	0.200%
80	21.215	3076	3082	3091	rBV	471402	689090	47.64%	6.103%
81	22.391	3279	3282	3286	rBV3	22297	29979	2.07%	0.266%
82	23.274	3425	3432	3439	rBV	818205	1446511	100.00%	12.811%
83	23.415	3449	3456	3466	rBV	434259	856721	59.23%	7.588%




Sum of corrected areas: 11290802

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045248.D
Acq On : 15 Apr 2024 17:28
Operator : MA/JU
Sample : P2051-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

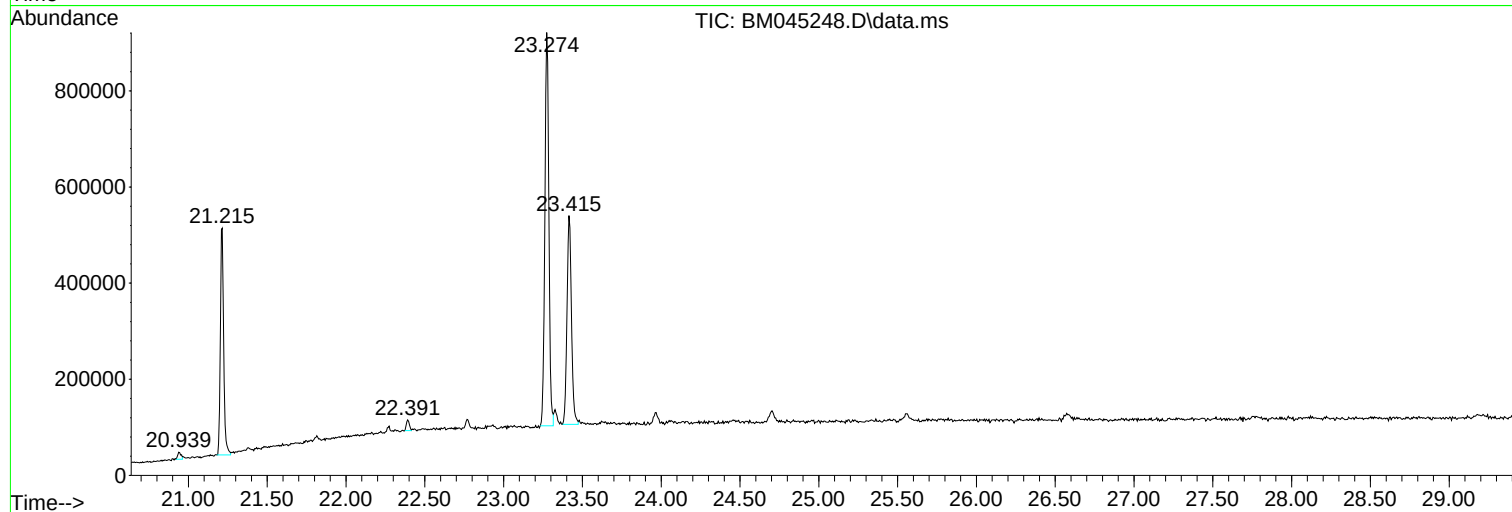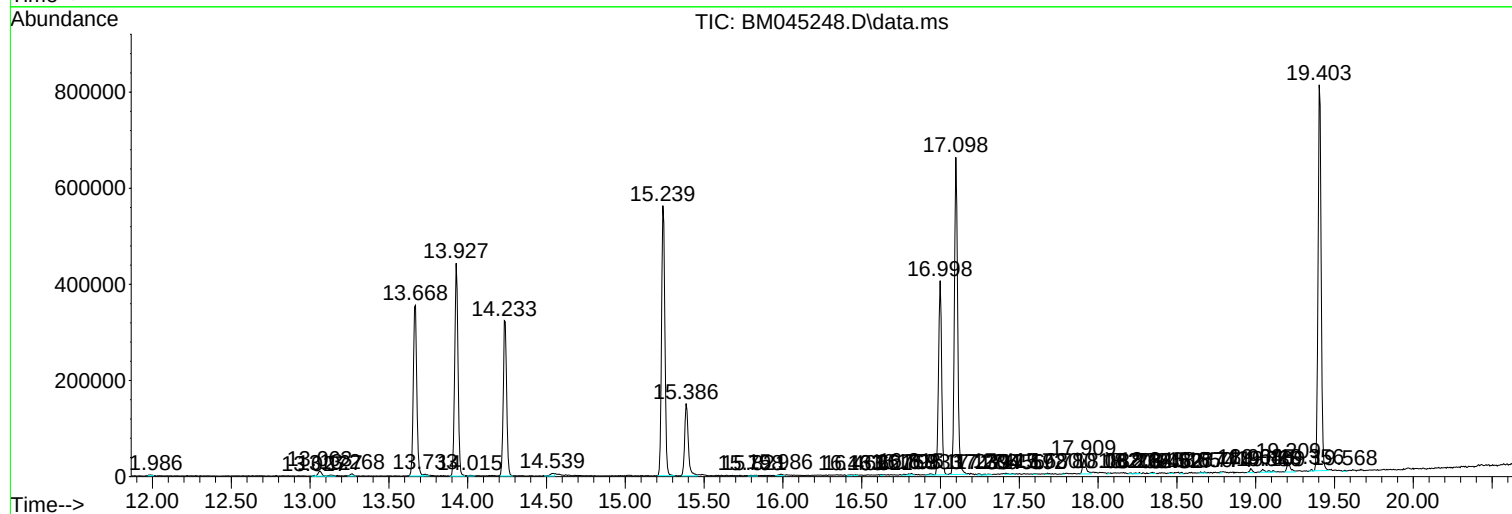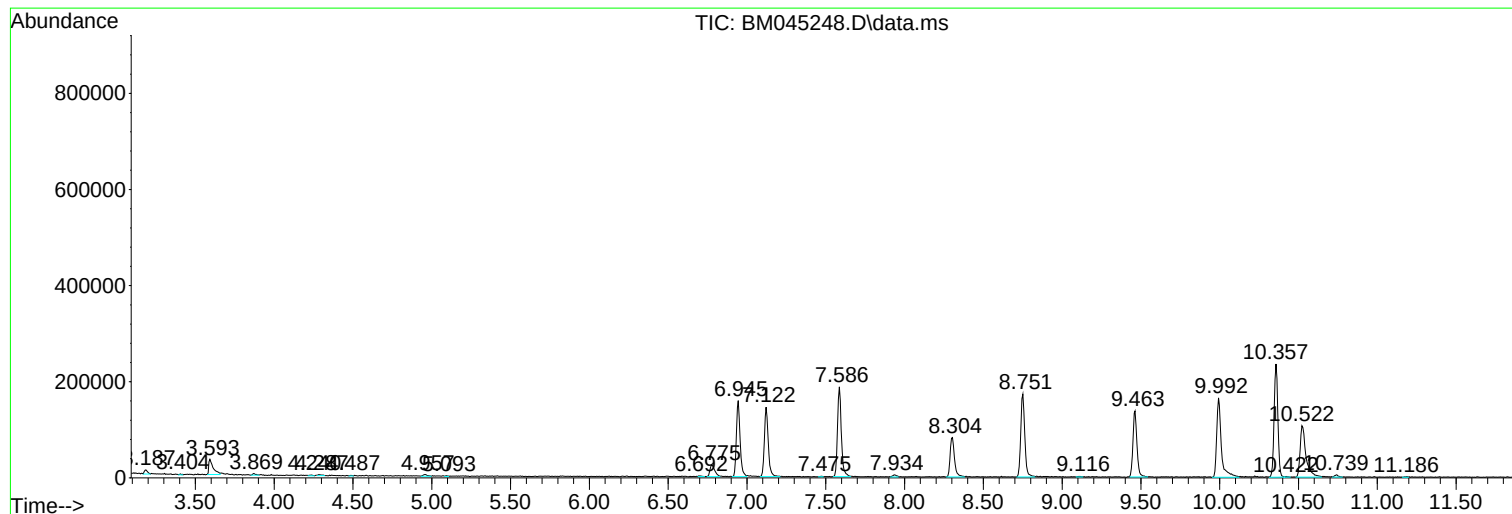

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045248.D
Acq On : 15 Apr 2024 17:28
Operator : MA/JU
Sample : P2051-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045248.D
Acq On : 15 Apr 2024 17:28
Operator : MA/JU
Sample : P2051-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RH8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------