

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045251.D
 Acq On : 15 Apr 2024 19:22
 Operator : MA/JU
 Sample : P2051-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045251.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	21	rVV2	9054	11666	0.81%	0.095%
2	3.234	23	25	29	rVB3	1938	2582	0.18%	0.021%
3	3.316	37	39	42	rVB3	2526	2431	0.17%	0.020%
4	3.599	84	87	96	rBV	14960	33428	2.33%	0.273%
5	3.693	101	103	106	rVB3	2851	2542	0.18%	0.021%
6	3.857	128	131	132	rBV3	2088	2292	0.16%	0.019%
7	3.869	132	133	139	rVB5	4162	4146	0.29%	0.034%
8	3.946	143	146	147	rBV2	2501	1788	0.12%	0.015%
9	4.322	208	210	212	rVB3	1787	1750	0.12%	0.014%
10	4.387	218	221	223	rBV2	1368	2075	0.14%	0.017%
11	5.063	334	336	342	rVB5	1021	1671	0.12%	0.014%
12	5.669	436	439	443	rBV4	1016	1468	0.10%	0.012%
13	6.693	609	613	618	rBV4	1653	1882	0.13%	0.015%
14	6.781	622	628	640	rVB2	27636	58207	4.05%	0.476%
15	6.946	649	656	667	rBV	180703	306497	21.34%	2.507%
16	7.122	680	686	696	rBV	165074	275356	19.17%	2.253%
17	7.587	757	765	776	rBV	224928	366285	25.51%	2.997%
18	7.934	821	824	829	rVB5	1599	2259	0.16%	0.018%
19	8.298	880	886	898	rBV2	101954	185858	12.94%	1.520%
20	8.751	956	963	973	rBV	203778	359655	25.04%	2.942%
21	9.063	1013	1016	1019	rBV2	1246	1605	0.11%	0.013%
22	9.104	1022	1023	1029	rVB3	1722	2128	0.15%	0.017%
23	9.216	1039	1042	1045	rVB3	1168	1523	0.11%	0.012%
24	9.463	1077	1084	1096	rBV	161485	288567	20.09%	2.361%
25	9.792	1136	1140	1141	rBV2	1240	1477	0.10%	0.012%
26	9.992	1168	1174	1183	rBV	195247	361546	25.18%	2.958%
27	10.357	1229	1236	1245	rBV	274595	464653	32.36%	3.801%
28	10.522	1256	1264	1282	rBV	122411	305233	21.26%	2.497%
29	11.986	1510	1513	1514	rBV2	2785	2724	0.19%	0.022%
30	13.133	1705	1708	1711	rBV2	1797	2165	0.15%	0.018%
31	13.669	1792	1799	1814	rVB	405257	620176	43.19%	5.074%
32	13.927	1837	1843	1853	rBV	516301	765622	53.31%	6.263%
33	14.239	1888	1896	1905	rVB	397296	583839	40.66%	4.776%
34	14.545	1942	1948	1949	rBV5	4153	7156	0.50%	0.059%
35	15.239	2060	2066	2079	rBV	638197	938962	65.39%	7.682%
36	15.386	2086	2091	2101	rBV2	158116	251681	17.53%	2.059%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045251.D
 Acq On : 15 Apr 2024 19:22
 Operator : MA/JU
 Sample : P2051-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R49

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	15.480	2105	2107	2112	rVB	2396	3193	0.22%	0.026%
38	16.939	2352	2355	2358	rVB2	1342	1490	0.10%	0.012%
39	16.998	2359	2365	2372	rVV	479493	649756	45.25%	5.316%
40	17.098	2376	2382	2397	rVV2	702536	1029288	71.68%	8.420%
41	17.910	2515	2520	2530	rBV2	26902	44877	3.13%	0.367%
42	18.780	2666	2668	2669	rBV2	1778	1669	0.12%	0.014%
43	18.968	2695	2700	2705	rVV5	6314	9778	0.68%	0.080%
44	19.045	2708	2713	2716	rBV4	5662	8414	0.59%	0.069%
45	19.092	2719	2721	2722	rBV2	2372	1662	0.12%	0.014%
46	19.209	2737	2741	2746	rBV6	14618	21173	1.47%	0.173%
47	19.404	2768	2774	2784	rBV	837873	1157381	80.60%	9.468%
48	19.927	2861	2863	2865	rVB3	2482	1523	0.11%	0.012%
49	20.945	3032	3036	3039	rBV5	11854	17034	1.19%	0.139%
50	21.209	3076	3081	3093	rBV	513993	722953	50.34%	5.914%
51	23.274	3425	3432	3439	rBV	822279	1436038	100.00%	11.748%
52	23.415	3449	3456	3467	rBV	464452	894555	62.29%	7.318%




Sum of corrected areas: 12223679

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045251.D
Acq On : 15 Apr 2024 19:22
Operator : MA/JU
Sample : P2051-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R49

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

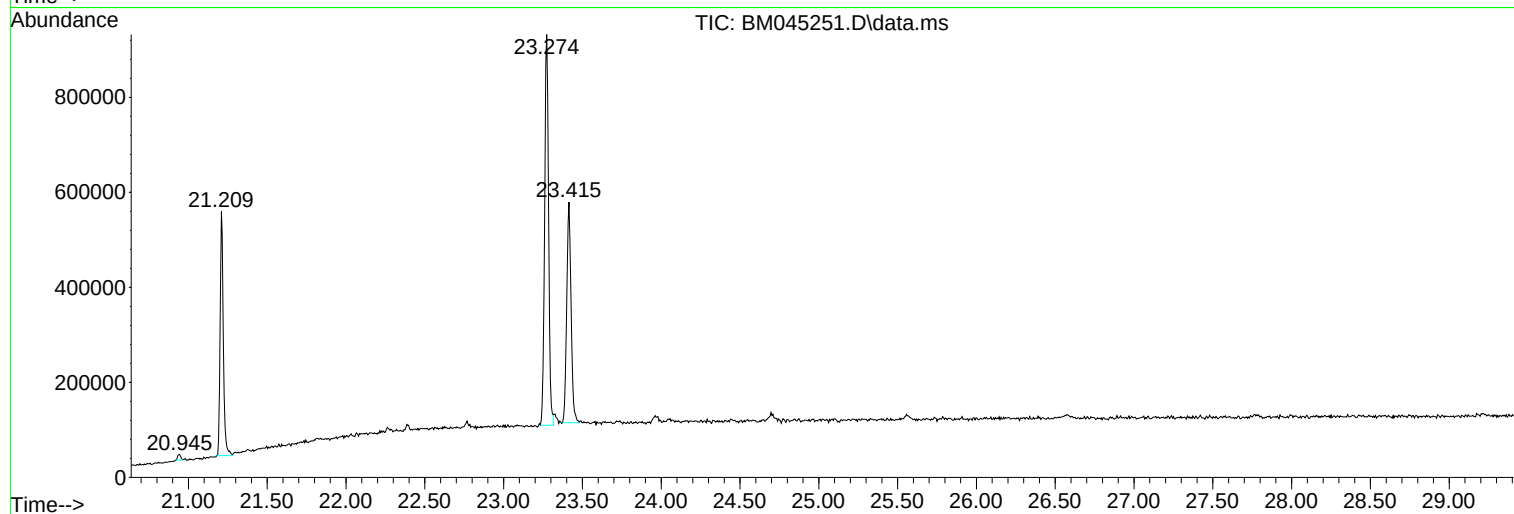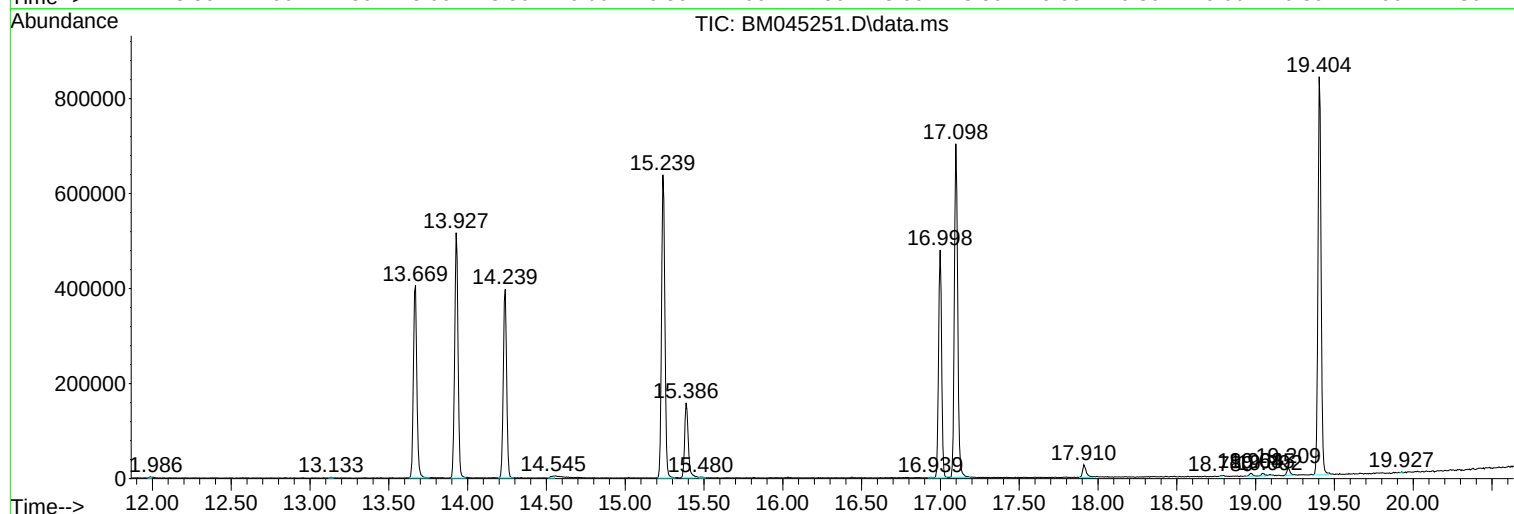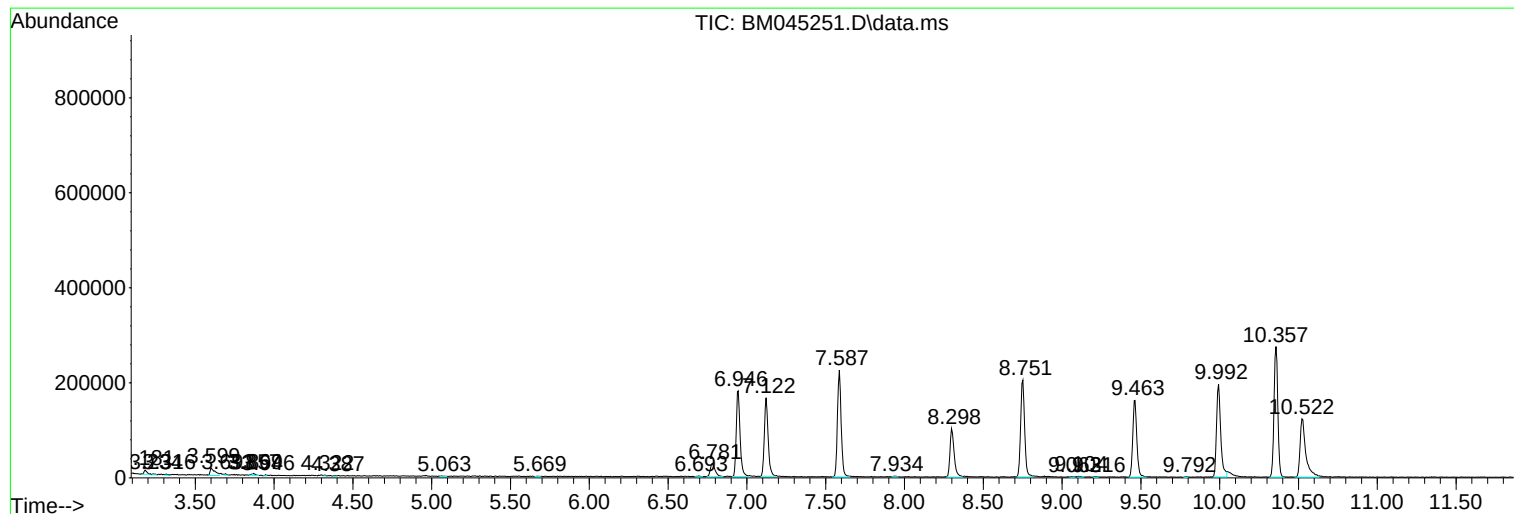

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045251.D
Acq On : 15 Apr 2024 19:22
Operator : MA/JU
Sample : P2051-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R49

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045251.D
Acq On : 15 Apr 2024 19:22
Operator : MA/JU
Sample : P2051-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R49

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc