

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045252.D
 Acq On : 15 Apr 2024 20:00
 Operator : MA/JU
 Sample : P2051-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CORH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045252.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	21	rVB3	7740	11838	0.85%	0.103%
2	3.405	50	54	55	rBV4	1611	1970	0.14%	0.017%
3	3.610	86	89	98	rBV4	9147	22500	1.62%	0.196%
4	3.869	129	133	137	rVB5	4001	5984	0.43%	0.052%
5	3.993	150	154	155	rBV4	1476	1820	0.13%	0.016%
6	4.010	155	157	160	rVV3	1512	1390	0.10%	0.012%
7	4.952	315	317	320	rVB2	1324	1592	0.11%	0.014%
8	6.781	623	628	640	rVB2	23766	53656	3.86%	0.467%
9	6.946	650	656	665	rBV	163123	263847	19.00%	2.298%
10	7.122	680	686	697	rBV	144157	248083	17.87%	2.161%
11	7.587	758	765	776	rVB	194959	319289	22.99%	2.781%
12	8.298	880	886	900	rBV	88560	161114	11.60%	1.403%
13	8.751	956	963	979	rBV	179044	314266	22.63%	2.737%
14	9.463	1075	1084	1095	rBV	145806	252158	18.16%	2.196%
15	9.992	1166	1174	1194	rBV	166452	343338	24.72%	2.990%
16	10.357	1228	1236	1245	rBV	256335	424460	30.57%	3.697%
17	10.528	1257	1265	1284	rBV2	96204	250053	18.01%	2.178%
18	11.504	1427	1431	1433	rBV2	1267	1836	0.13%	0.016%
19	11.904	1498	1499	1504	rBV4	1131	1466	0.11%	0.013%
20	11.992	1510	1514	1519	rBV4	1968	3718	0.27%	0.032%
21	12.275	1558	1562	1568	rBV4	766	1405	0.10%	0.012%
22	13.139	1705	1709	1714	rVB6	1773	2608	0.19%	0.023%
23	13.669	1792	1799	1811	rBV	379218	568471	40.94%	4.951%
24	13.927	1836	1843	1853	rBV2	476394	699654	50.38%	6.094%
25	14.233	1889	1895	1906	rVV	374340	555828	40.03%	4.841%
26	14.545	1942	1948	1949	rBV2	4769	7985	0.58%	0.070%
27	14.692	1970	1973	1977	rVB4	1603	1634	0.12%	0.014%
28	15.239	2060	2066	2077	rBV	602095	874819	63.00%	7.620%
29	15.386	2085	2091	2106	rBV	157787	248000	17.86%	2.160%
30	15.733	2147	2150	2154	rBV2	789	1574	0.11%	0.014%
31	16.998	2359	2365	2371	rBV	466526	618387	44.53%	5.386%
32	17.098	2376	2382	2397	rBV	682383	1017791	73.29%	8.865%
33	17.568	2457	2462	2463	rBV2	1073	1448	0.10%	0.013%
34	17.704	2482	2485	2487	rVB3	1299	1535	0.11%	0.013%
35	17.780	2495	2498	2501	rBV2	1142	1668	0.12%	0.015%
36	17.910	2515	2520	2527	rBV3	20848	33615	2.42%	0.293%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045252.D
 Acq On : 15 Apr 2024 20:00
 Operator : MA/JU
 Sample : P2051-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CORH6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	17.974	2529	2531	2533	rVV3	2061	1899	0.14%	0.017%
38	18.027	2537	2540	2542	rBV2	2187	1971	0.14%	0.017%
39	18.074	2546	2548	2551	rBV3	1251	1453	0.10%	0.013%
40	18.345	2591	2594	2596	rBV3	1571	1527	0.11%	0.013%
41	18.968	2696	2700	2705	rBV4	7647	9995	0.72%	0.087%
42	19.045	2709	2713	2718	rBV3	5637	8662	0.62%	0.075%
43	19.209	2736	2741	2744	rBV5	11797	17613	1.27%	0.153%
44	19.404	2768	2774	2783	rBV	834186	1136679	81.85%	9.900%
45	19.956	2867	2868	2872	rBV3	2356	3254	0.23%	0.028%
46	20.056	2883	2885	2887	rVB3	2261	1517	0.11%	0.013%
47	20.121	2894	2896	2899	rBV3	2827	3079	0.22%	0.027%
48	20.951	3031	3037	3042	rBV8	9809	25871	1.86%	0.225%
49	21.209	3076	3081	3092	rBV	482416	707096	50.92%	6.159%
50	23.274	3425	3432	3439	rBV	783903	1388650	100.00%	12.095%
51	23.415	3449	3456	3469	rVB	429146	851192	61.30%	7.414%




Sum of corrected areas: 11481258

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045252.D
Acq On : 15 Apr 2024 20:00
Operator : MA/JU
Sample : P2051-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CORH6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

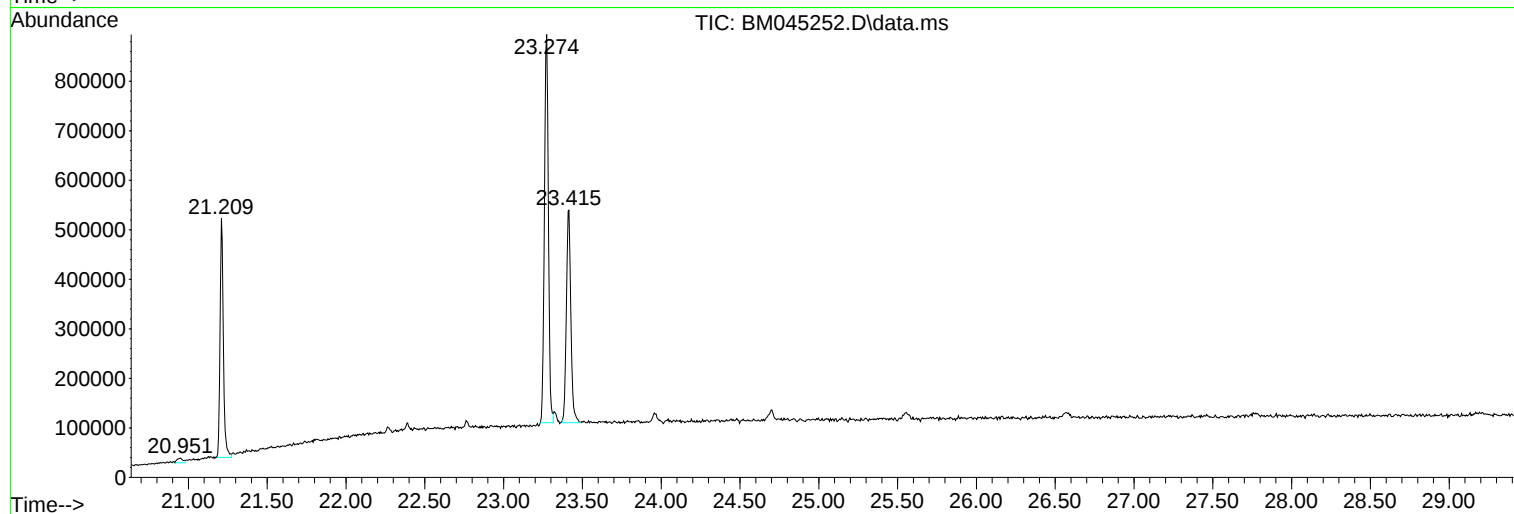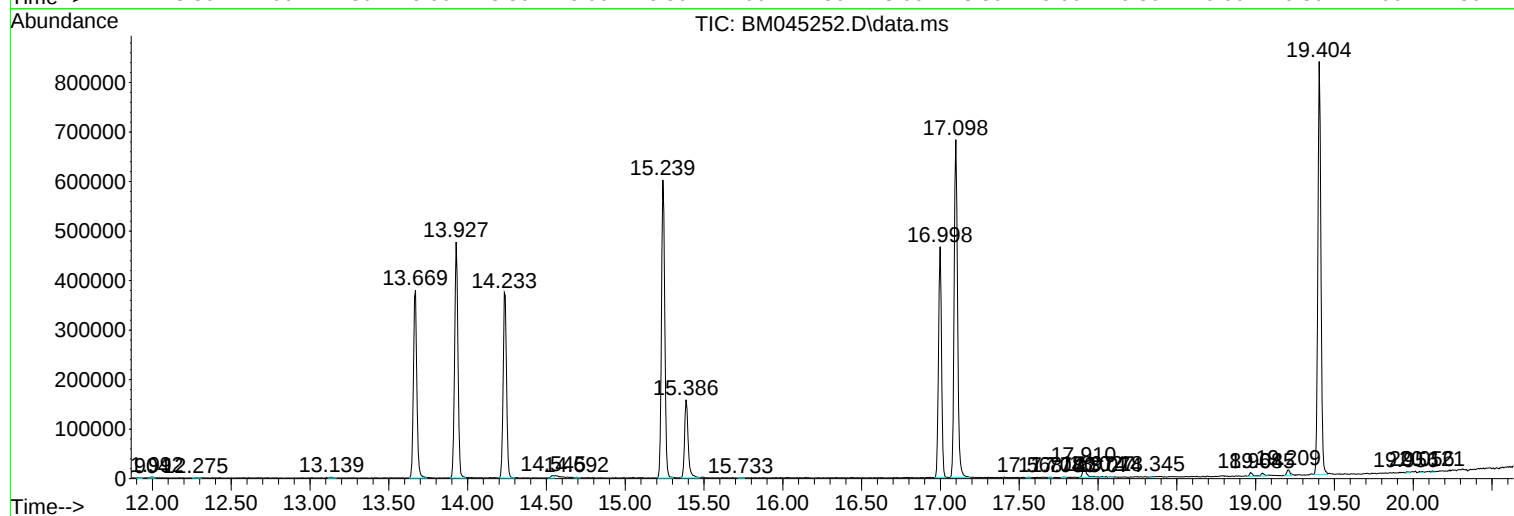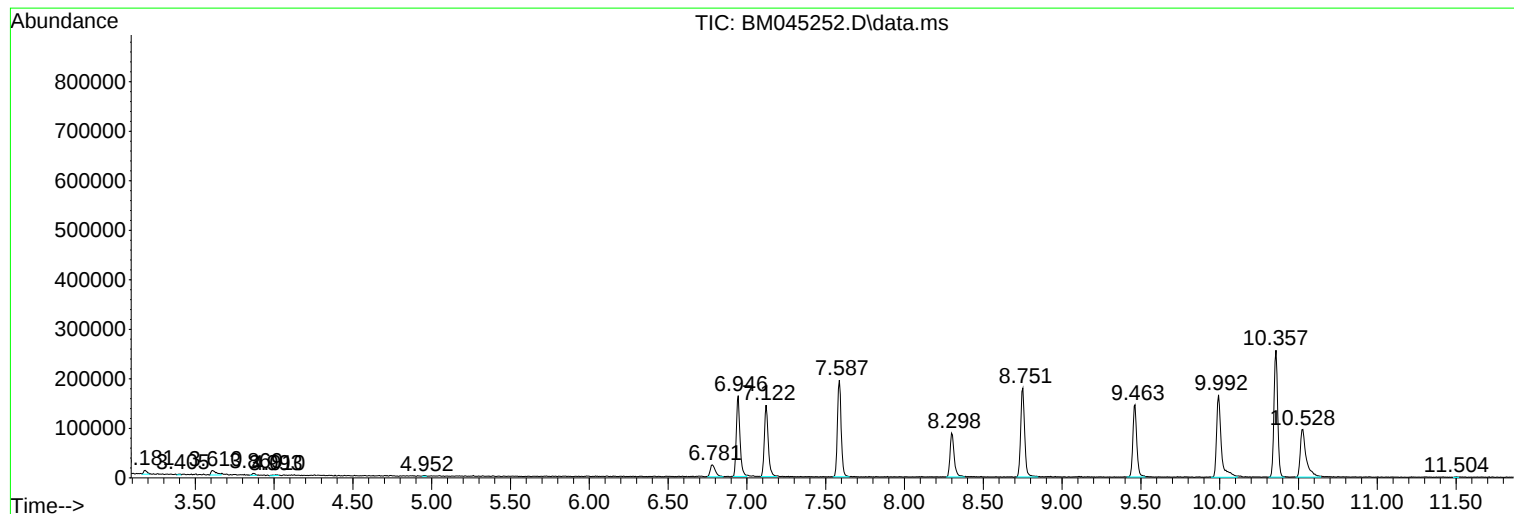

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045252.D
Acq On : 15 Apr 2024 20:00
Operator : MA/JU
Sample : P2051-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RH6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045252.D
Acq On : 15 Apr 2024 20:00
Operator : MA/JU
Sample : P2051-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0RH6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc