

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045253.D
 Acq On : 15 Apr 2024 20:38
 Operator : MA/JU
 Sample : P2036-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCSY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045253.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	6	9	14	rVV	53980	71376	4.82%	0.536%
2	3.181	14	16	19	rVV	12251	13375	0.90%	0.100%
3	3.210	19	21	26	rVB2	10114	12994	0.88%	0.098%
4	3.587	82	85	98	rBV	38649	77858	5.26%	0.585%
5	3.869	130	133	136	rVB3	3907	4295	0.29%	0.032%
6	4.081	166	169	170	rBV3	2221	1804	0.12%	0.014%
7	4.281	201	203	206	rBV2	1880	1551	0.10%	0.012%
8	4.316	206	209	211	rVV3	1281	1505	0.10%	0.011%
9	4.363	211	217	225	rVV	102798	143424	9.68%	1.077%
10	4.493	238	239	242	rBV3	1516	1540	0.10%	0.012%
11	4.763	280	285	290	rBV6	2615	4374	0.30%	0.033%
12	5.151	347	351	354	rBV5	1250	1778	0.12%	0.013%
13	5.610	428	429	433	rBV4	1344	1721	0.12%	0.013%
14	5.934	480	484	485	rBV3	1393	2146	0.14%	0.016%
15	6.134	517	518	522	rVB4	1285	1484	0.10%	0.011%
16	6.169	522	524	528	rBV2	1581	1895	0.13%	0.014%
17	6.687	606	612	613	rBV4	1003	1627	0.11%	0.012%
18	6.775	622	627	637	rBV2	31260	64501	4.35%	0.484%
19	6.945	648	656	672	rBV	171380	289179	19.52%	2.172%
20	7.122	680	686	697	rBV	178644	291860	19.70%	2.192%
21	7.587	758	765	773	rBV	226799	360786	24.36%	2.710%
22	7.692	781	783	789	rVB5	1311	2181	0.15%	0.016%
23	8.298	880	886	899	rBV	105221	188080	12.70%	1.413%
24	8.381	899	900	904	rVV3	1640	1695	0.11%	0.013%
25	8.422	904	907	910	rVB3	1364	1659	0.11%	0.012%
26	8.751	956	963	976	rBV	193028	335822	22.67%	2.522%
27	9.110	1021	1024	1027	rVB4	1839	2326	0.16%	0.017%
28	9.457	1076	1083	1094	rBV	159273	274073	18.50%	2.058%
29	9.992	1167	1174	1188	rBV	191875	372634	25.16%	2.799%
30	10.080	1188	1189	1198	rVB7	5486	5644	0.38%	0.042%
31	10.357	1229	1236	1245	rVB	294694	478993	32.34%	3.597%
32	10.522	1257	1264	1280	rVV	148640	353642	23.87%	2.656%
33	10.627	1280	1282	1284	rVV3	2675	2868	0.19%	0.022%
34	10.657	1284	1287	1291	rVB4	1595	2359	0.16%	0.018%
35	11.822	1477	1485	1487	rBV2	795	1660	0.11%	0.012%
36	11.986	1507	1513	1517	rBV4	2850	4547	0.31%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045253.D
 Acq On : 15 Apr 2024 20:38
 Operator : MA/JU
 Sample : P2036-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCSY4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	13.133	1703	1708	1713	rBV4	3205	5643	0.38%	0.042%
38	13.668	1792	1799	1812	rVB	414450	624891	42.19%	4.693%
39	13.927	1835	1843	1854	rBV2	514771	758442	51.20%	5.696%
40	14.233	1889	1895	1903	rBV	414242	630484	42.56%	4.735%
41	14.527	1938	1945	1951	rBV6	8071	24123	1.63%	0.181%
42	14.610	1957	1959	1962	rVB3	2356	2301	0.16%	0.017%
43	14.692	1969	1973	1981	rVB4	3607	7204	0.49%	0.054%
44	15.239	2060	2066	2078	rVB	662490	963676	65.06%	7.238%
45	15.386	2084	2091	2099	rBV	183926	276359	18.66%	2.076%
46	15.439	2099	2100	2106	rVV3	4066	5659	0.38%	0.043%
47	15.492	2106	2109	2112	rVB3	2206	2790	0.19%	0.021%
48	16.262	2235	2240	2244	rBV4	1122	2290	0.15%	0.017%
49	16.427	2266	2268	2271	rVV3	1192	1498	0.10%	0.011%
50	16.945	2352	2356	2358	rVB4	1305	1880	0.13%	0.014%
51	16.998	2358	2365	2373	rBV	537754	724011	48.88%	5.438%
52	17.098	2376	2382	2397	rVV	721937	1059158	71.50%	7.955%
53	17.404	2432	2434	2437	rBV4	1839	1626	0.11%	0.012%
54	17.456	2440	2443	2447	rVB2	1113	1501	0.10%	0.011%
55	17.909	2516	2520	2529	rVV3	32089	48657	3.28%	0.365%
56	18.203	2567	2570	2574	rBV4	1126	1552	0.10%	0.012%
57	18.792	2667	2670	2672	rBV4	1874	2349	0.16%	0.018%
58	18.845	2677	2679	2683	rVB3	1721	2053	0.14%	0.015%
59	18.968	2697	2700	2704	rVB3	7293	8201	0.55%	0.062%
60	19.045	2709	2713	2717	rBV3	5280	8244	0.56%	0.062%
61	19.203	2734	2740	2746	rBV6	20523	32889	2.22%	0.247%
62	19.403	2768	2774	2787	rBV	942062	1246269	84.14%	9.360%
63	19.921	2860	2862	2864	rBV3	1950	1765	0.12%	0.013%
64	19.945	2864	2866	2868	rBV3	1956	1991	0.13%	0.015%
65	20.145	2897	2900	2903	rBV5	2737	4199	0.28%	0.032%
66	20.380	2937	2940	2941	rBV2	4521	4818	0.33%	0.036%
67	20.433	2945	2949	2954	rVV2	21232	27636	1.87%	0.208%
68	20.939	3032	3035	3040	rBV6	13746	19657	1.33%	0.148%
69	21.209	3076	3081	3093	rBV	593294	832138	56.18%	6.250%
70	21.750	3170	3173	3177	rBV3	30224	39135	2.64%	0.294%
71	22.309	3265	3268	3272	rVB2	38277	49883	3.37%	0.375%
72	22.921	3369	3372	3378	rVB3	37417	60949	4.11%	0.458%
73	23.274	3425	3432	3440	rBV	821064	1481245	100.00%	11.125%
74	23.409	3449	3455	3468	rVB	502545	968451	65.38%	7.273%

Sum of corrected areas: 13314873

Instrument :

BNA_M

ClientSampleId :




YCSY4

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045253.D
Acq On : 15 Apr 2024 20:38
Operator : MA/JU
Sample : P2036-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSY4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

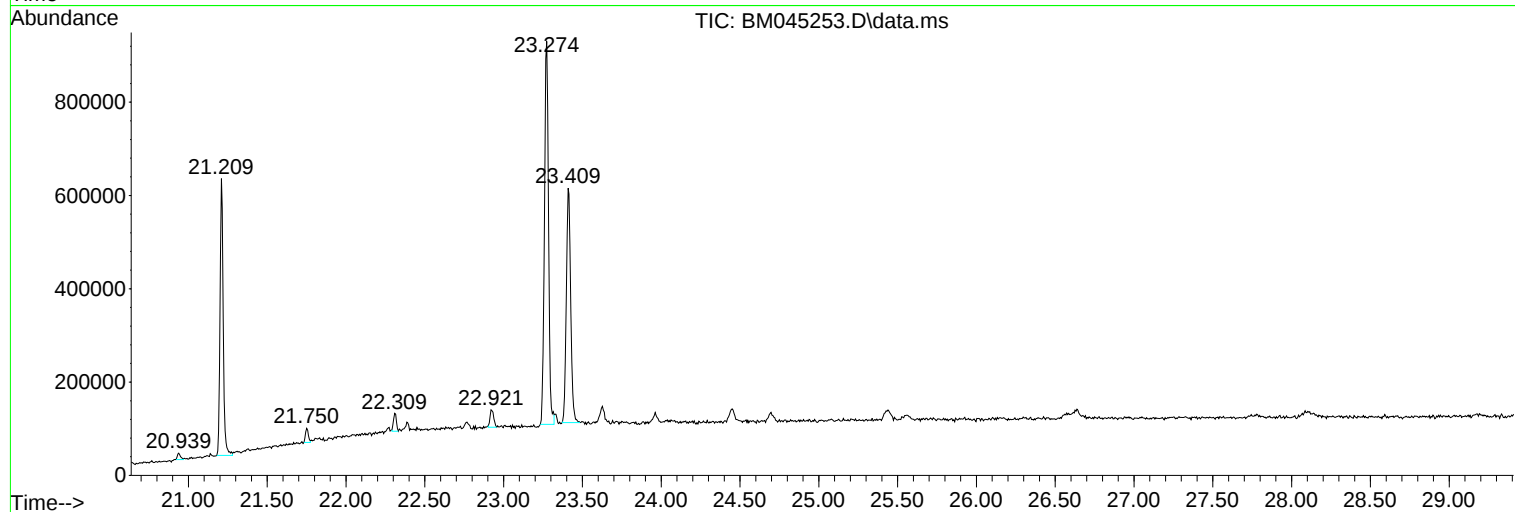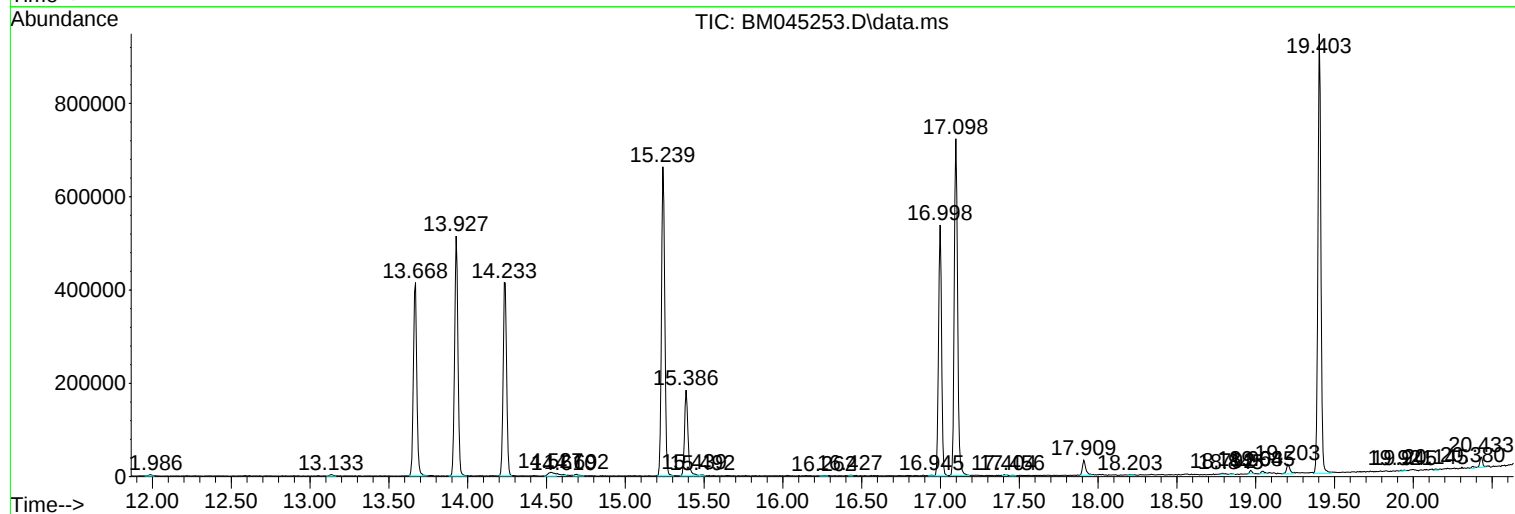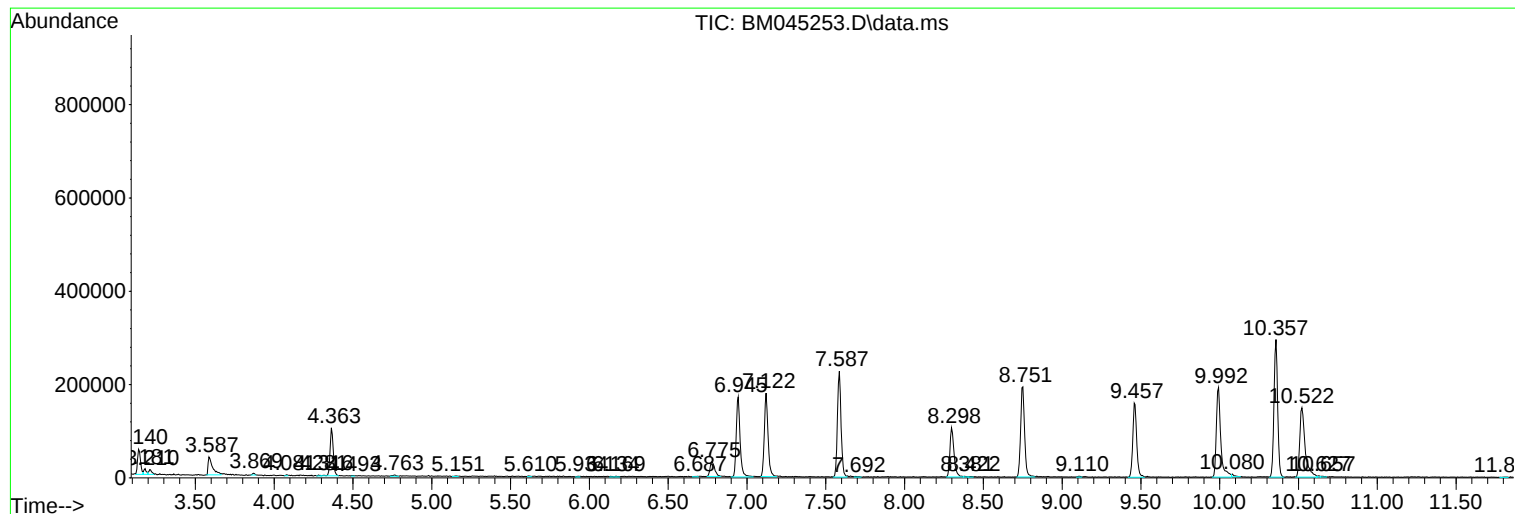

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045253.D
Acq On : 15 Apr 2024 20:38
Operator : MA/JU
Sample : P2036-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSY4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.363	7.95 ng/ul	143424	1,4-Dichlorobenzene-d4	7.587

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	96
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	25

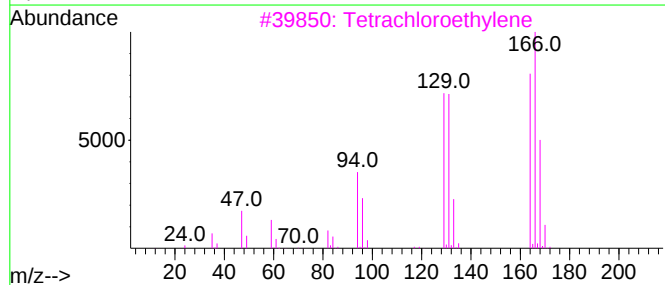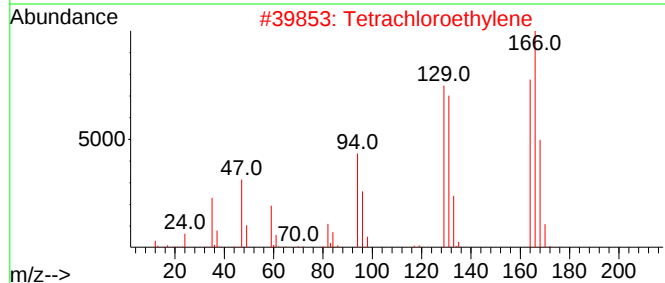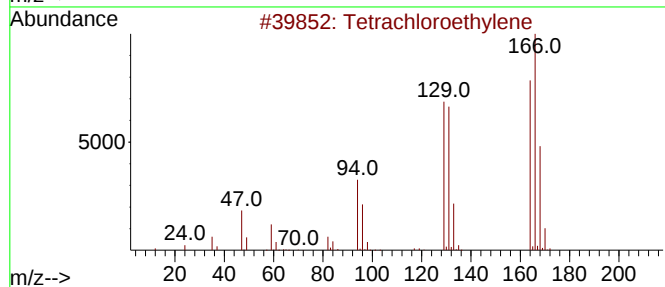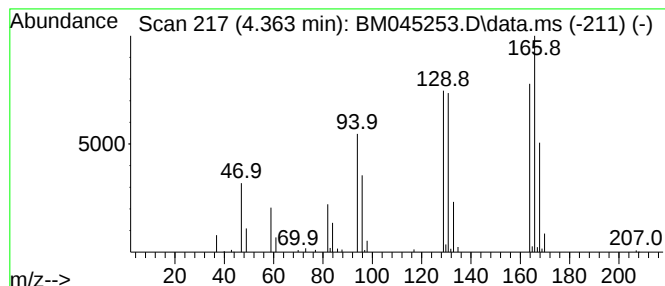

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045253.D
Acq On : 15 Apr 2024 20:38
Operator : MA/JU
Sample : P2036-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCSY4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.363	8.0	ng/ul	143424	1	7.587	360786	20.0