

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045256.D
 Acq On : 15 Apr 2024 22:31
 Operator : MA/JU
 Sample : PB160238BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK238

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045256.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	22	rBV	13411	19618	1.57%	0.156%
2	3.446	59	61	64	rVB3	1641	1812	0.15%	0.014%
3	3.575	80	83	99	rBV	150413	252806	20.25%	2.010%
4	3.869	130	133	135	rBV4	3299	3251	0.26%	0.026%
5	4.075	167	168	171	rBV2	1707	1903	0.15%	0.015%
6	4.146	178	180	183	rVB3	1520	1545	0.12%	0.012%
7	4.269	198	201	202	rBV3	1317	1258	0.10%	0.010%
8	4.293	202	205	207	rBV3	1296	1573	0.13%	0.013%
9	4.657	265	267	271	rVV4	1281	1786	0.14%	0.014%
10	4.710	274	276	280	rVB3	2074	2261	0.18%	0.018%
11	4.793	287	290	292	rBV3	1201	1517	0.12%	0.012%
12	5.099	341	342	347	rVB4	1484	1360	0.11%	0.011%
13	5.340	380	383	385	rBV3	1149	1631	0.13%	0.013%
14	5.363	385	387	391	rVB4	1724	1971	0.16%	0.016%
15	5.404	391	394	395	rBV2	1275	1286	0.10%	0.010%
16	5.516	410	413	416	rVV5	1427	1817	0.15%	0.014%
17	5.751	451	453	456	rVB3	1565	1257	0.10%	0.010%
18	6.698	613	614	619	rVB5	2406	2648	0.21%	0.021%
19	6.769	619	626	637	rBV	183554	335099	26.84%	2.664%
20	6.940	649	655	666	rVV	165929	275651	22.08%	2.191%
21	7.116	677	685	701	rBV	208513	355202	28.45%	2.824%
22	7.469	742	745	746	rBV3	1013	1252	0.10%	0.010%
23	7.587	758	765	773	rBV	191145	312939	25.07%	2.488%
24	7.663	775	778	779	rVB3	1589	1271	0.10%	0.010%
25	7.793	799	800	805	rVB4	1086	1278	0.10%	0.010%
26	7.857	810	811	817	rVB3	807	1366	0.11%	0.011%
27	8.151	858	861	865	rVV4	893	1343	0.11%	0.011%
28	8.204	867	870	873	rBV3	981	1307	0.10%	0.010%
29	8.292	878	885	900	rBV	221730	404062	32.36%	3.212%
30	8.516	920	923	924	rBV3	1258	1258	0.10%	0.010%
31	8.745	956	962	973	rBV	188498	333457	26.71%	2.651%
32	8.816	973	974	977	rVV2	2871	2464	0.20%	0.020%
33	8.875	983	984	987	rBV3	1826	1827	0.15%	0.015%
34	9.304	1054	1057	1058	rBV3	1200	1256	0.10%	0.010%
35	9.457	1077	1083	1094	rBV	158342	280130	22.44%	2.227%
36	9.992	1167	1174	1183	rBV	206277	385442	30.87%	3.064%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045256.D
 Acq On : 15 Apr 2024 22:31
 Operator : MA/JU
 Sample : PB160238BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK238

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	10.357	1228	1236	1246	rBV	251370	430196	34.46%	3.420%
38	10.516	1256	1263	1281	rBV	166163	419685	33.62%	3.336%
39	11.992	1509	1514	1517	rBV3	2314	3591	0.29%	0.029%
40	13.133	1705	1708	1711	rVB3	1181	1668	0.13%	0.013%
41	13.663	1792	1798	1812	rBV	398490	616714	49.40%	4.902%
42	13.927	1836	1843	1851	rBV	490435	730727	58.53%	5.809%
43	14.233	1890	1895	1903	rVV	372819	564953	45.25%	4.491%
44	14.480	1930	1937	1961	rBV	88313	246858	19.77%	1.962%
45	15.010	2023	2027	2030	rBV3	693	1250	0.10%	0.010%
46	15.239	2059	2066	2076	rBV	623872	903612	72.38%	7.183%
47	15.386	2086	2091	2101	rBV	149473	237268	19.00%	1.886%
48	15.451	2101	2102	2106	rVV3	2259	2421	0.19%	0.019%
49	16.786	2326	2329	2334	rVB4	1919	1871	0.15%	0.015%
50	16.998	2358	2365	2373	rBV	478145	640463	51.30%	5.091%
51	17.098	2375	2382	2398	rVV	621524	946663	75.82%	7.525%
52	17.339	2418	2423	2426	rBV4	943	1654	0.13%	0.013%
53	17.610	2466	2469	2471	rBV2	1461	1423	0.11%	0.011%
54	17.739	2488	2491	2492	rBV	1482	1296	0.10%	0.010%
55	17.886	2514	2516	2519	rVB2	1409	1283	0.10%	0.010%
56	17.927	2519	2523	2527	rBV4	4249	6731	0.54%	0.054%
57	18.486	2616	2618	2620	rVB2	2244	1322	0.11%	0.011%
58	18.968	2697	2700	2707	rVB4	6492	8371	0.67%	0.067%
59	19.039	2707	2712	2718	rBV4	5729	9211	0.74%	0.073%
60	19.215	2739	2742	2747	rVV5	2238	3535	0.28%	0.028%
61	19.404	2768	2774	2784	rBV	784921	1059359	84.85%	8.421%
62	19.609	2807	2809	2812	rBV4	2009	1725	0.14%	0.014%
63	19.892	2856	2857	2858	rBV	2313	1295	0.10%	0.010%
64	21.209	3075	3081	3090	rBV	473658	693154	55.52%	5.510%
65	23.268	3424	3431	3437	rBV2	710400	1248505	100.00%	9.925%
66	23.409	3448	3455	3465	rVB	390426	795059	63.68%	6.320%




Sum of corrected areas: 12579767

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045256.D
Acq On : 15 Apr 2024 22:31
Operator : MA/JU
Sample : PB160238BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK238

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

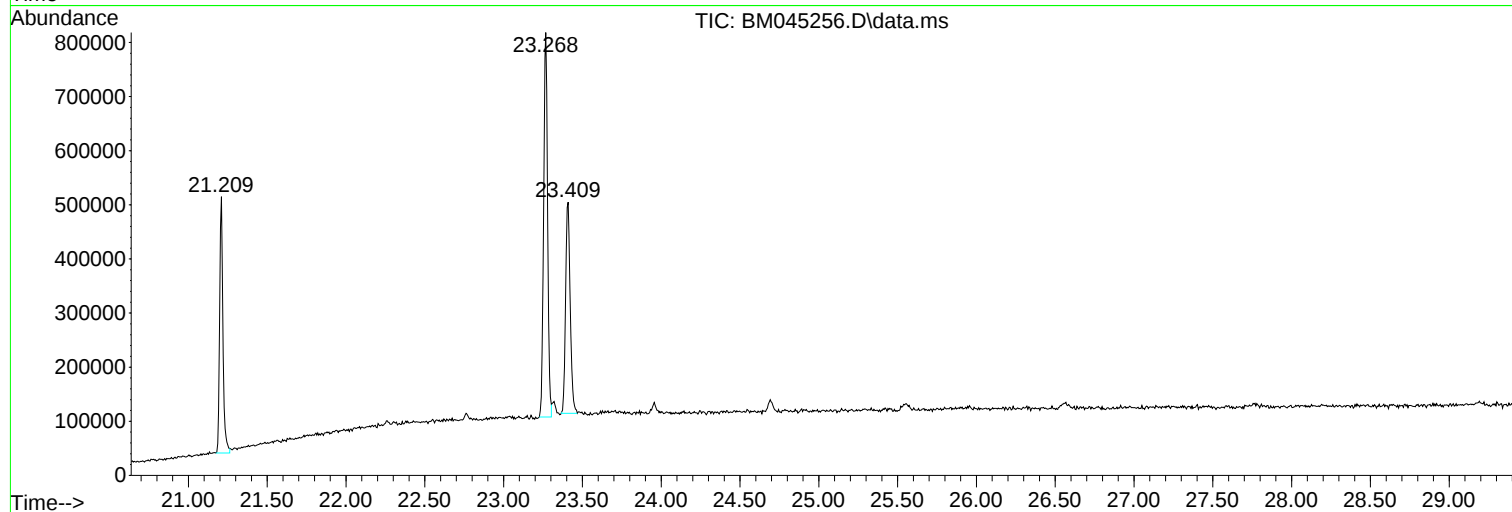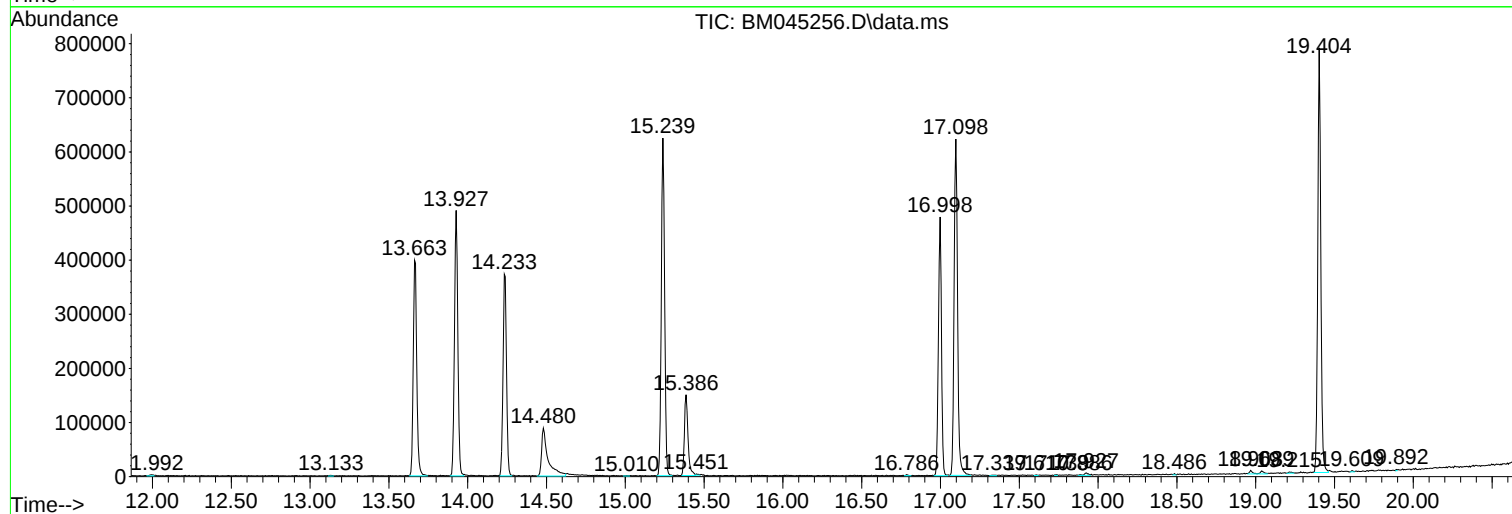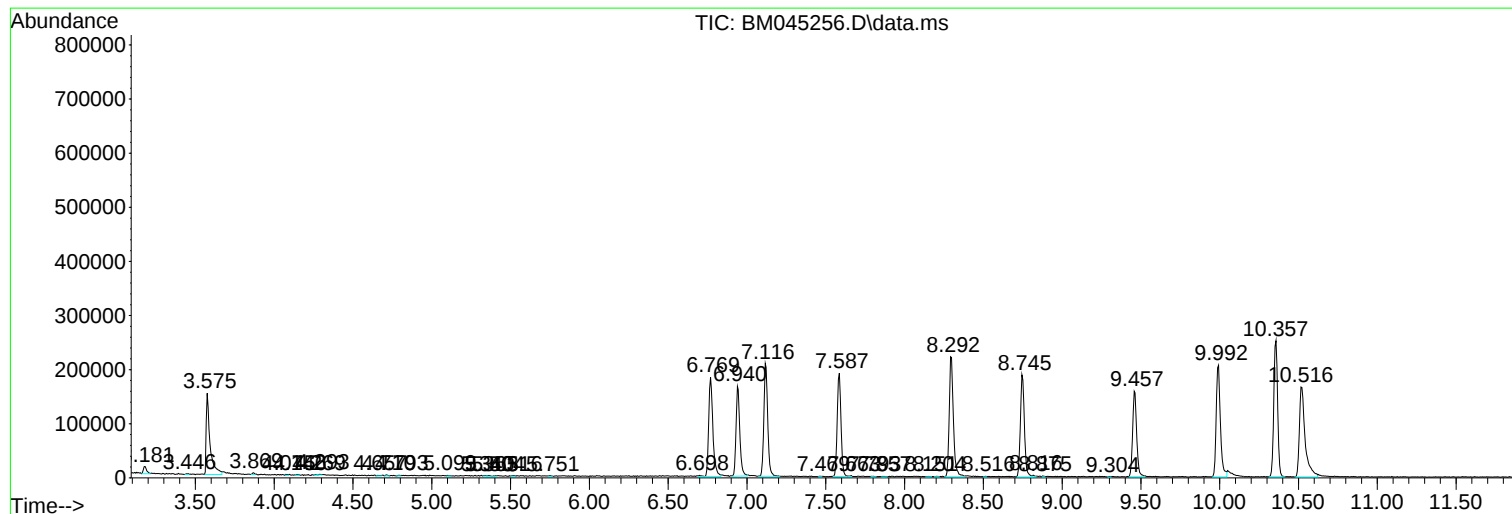

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045256.D
Acq On : 15 Apr 2024 22:31
Operator : MA/JU
Sample : PB160238BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK238

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045256.D
Acq On : 15 Apr 2024 22:31
Operator : MA/JU
Sample : PB160238BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK238

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc