

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045261.D
 Acq On : 16 Apr 2024 02:15
 Operator : MA/JU
 Sample : PB160227BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045261.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	13	15	22	rVB2	14203	18534	1.36%	0.135%
2	3.434	57	59	63	rVB5	1929	2161	0.16%	0.016%
3	3.575	80	83	104	rBV	158826	285120	20.91%	2.078%
4	3.869	128	133	136	rBV5	4372	5899	0.43%	0.043%
5	4.069	165	167	170	rBV3	1629	1403	0.10%	0.010%
6	4.164	181	183	188	rBV5	1582	1625	0.12%	0.012%
7	4.199	188	189	192	rVB3	1792	1448	0.11%	0.011%
8	4.293	203	205	210	rVB5	2691	2671	0.20%	0.019%
9	4.658	266	267	269	rBV2	1833	1414	0.10%	0.010%
10	4.705	272	275	277	rBV4	1576	1534	0.11%	0.011%
11	4.887	301	306	307	rBV4	1926	2639	0.19%	0.019%
12	4.911	307	310	312	rVV3	1681	1602	0.12%	0.012%
13	5.522	412	414	417	rVB4	1585	1580	0.12%	0.012%
14	5.558	417	420	424	rBV5	1280	1909	0.14%	0.014%
15	5.646	431	435	437	rBV5	1616	1432	0.11%	0.010%
16	5.922	480	482	485	rVB4	1129	1441	0.11%	0.011%
17	6.058	503	505	509	rBV5	1433	1614	0.12%	0.012%
18	6.093	509	511	514	rVV2	1762	1676	0.12%	0.012%
19	6.393	559	562	566	rBV5	1620	1890	0.14%	0.014%
20	6.705	609	615	618	rBV7	1680	3429	0.25%	0.025%
21	6.769	618	626	636	rBV	201540	362408	26.57%	2.641%
22	6.940	648	655	675	rVB	183031	311523	22.84%	2.270%
23	7.069	675	677	679	rBV2	1938	1781	0.13%	0.013%
24	7.116	679	685	695	rBV	231912	384554	28.20%	2.802%
25	7.181	695	696	698	rVB2	3358	1632	0.12%	0.012%
26	7.581	758	764	774	rVV	203215	339755	24.91%	2.476%
27	7.716	783	787	790	rVB4	1342	1518	0.11%	0.011%
28	8.293	879	885	896	rBV	248854	437180	32.06%	3.186%
29	8.452	909	912	914	rBV3	1751	1829	0.13%	0.013%
30	8.551	927	929	933	rVV3	1505	1920	0.14%	0.014%
31	8.746	952	962	971	rBV	209021	357515	26.21%	2.605%
32	8.916	989	991	994	rVB3	1548	1384	0.10%	0.010%
33	9.099	1018	1022	1024	rBV3	1429	1810	0.13%	0.013%
34	9.457	1075	1083	1095	rBV	178782	312051	22.88%	2.274%
35	9.987	1167	1173	1193	rBV	224333	437914	32.11%	3.191%
36	10.351	1228	1235	1244	rBV	267009	458150	33.59%	3.339%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045261.D
 Acq On : 16 Apr 2024 02:15
 Operator : MA/JU
 Sample : PB160227BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	10.516	1256	1263	1282	rBV	185561	464069	34.03%	3.382%
38	10.669	1286	1289	1293	rVV5	2474	4014	0.29%	0.029%
39	10.710	1293	1296	1299	rVB3	1466	1733	0.13%	0.013%
40	10.857	1317	1321	1323	rVB3	1638	1814	0.13%	0.013%
41	10.893	1323	1327	1330	rBV4	1192	2164	0.16%	0.016%
42	11.304	1395	1397	1402	rVB6	856	1487	0.11%	0.011%
43	11.904	1497	1499	1505	rVB3	1220	1970	0.14%	0.014%
44	11.981	1508	1512	1514	rBV4	2595	3257	0.24%	0.024%
45	12.145	1537	1540	1547	rVV4	1053	1914	0.14%	0.014%
46	12.487	1594	1598	1601	rBV3	1219	1828	0.13%	0.013%
47	12.845	1656	1659	1662	rBV2	1154	1509	0.11%	0.011%
48	13.116	1701	1705	1706	rBV3	1600	1952	0.14%	0.014%
49	13.128	1706	1707	1712	rVB3	2854	2727	0.20%	0.020%
50	13.610	1783	1789	1790	rBV5	1217	1999	0.15%	0.015%
51	13.663	1792	1798	1808	rVV	440500	675665	49.54%	4.924%
52	13.798	1820	1821	1827	rVB3	1211	1839	0.13%	0.013%
53	13.922	1836	1842	1853	rBV	533402	814360	59.71%	5.934%
54	14.233	1889	1895	1906	rVB	406312	605389	44.39%	4.411%
55	14.375	1918	1919	1923	rBV3	1062	1638	0.12%	0.012%
56	14.481	1930	1937	1952	rBV2	92741	253253	18.57%	1.845%
57	14.628	1961	1962	1968	rVB6	2364	2647	0.19%	0.019%
58	15.116	2042	2045	2050	rVB4	1278	1644	0.12%	0.012%
59	15.239	2059	2066	2075	rVV	657046	988590	72.49%	7.204%
60	15.380	2085	2090	2100	rBV	163789	263303	19.31%	1.919%
61	15.475	2105	2106	2107	rBV	2497	1430	0.10%	0.010%
62	15.569	2120	2122	2126	rBV3	1038	1381	0.10%	0.010%
63	15.933	2181	2184	2187	rBV4	1295	1744	0.13%	0.013%
64	16.027	2197	2200	2203	rBV4	2294	3614	0.26%	0.026%
65	16.292	2242	2245	2250	rVB5	1828	2164	0.16%	0.016%
66	16.492	2277	2279	2283	rBV4	1446	2113	0.15%	0.015%
67	16.680	2308	2311	2314	rVB3	1258	1378	0.10%	0.010%
68	16.992	2358	2364	2372	rBV	490079	680668	49.91%	4.960%
69	17.092	2375	2381	2398	rBV	661160	1024363	75.11%	7.464%
70	17.310	2414	2418	2422	rBV4	1518	1885	0.14%	0.014%
71	17.486	2443	2448	2449	rBV4	1255	1685	0.12%	0.012%
72	17.527	2452	2455	2459	rVV5	1545	1764	0.13%	0.013%
73	17.833	2506	2507	2512	rVB4	1615	1946	0.14%	0.014%
74	17.921	2517	2522	2524	rBV3	4978	6535	0.48%	0.048%
75	18.304	2585	2587	2593	rBV2	1066	1928	0.14%	0.014%
76	18.486	2612	2618	2619	rVV5	1289	2225	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045261.D
Acq On : 16 Apr 2024 02:15
Operator : MA/JU
Sample : PB160227BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

77	18.651	2642	2646	2647	rBV2	1406	1504	0.11%	0.011%
78	18.821	2672	2675	2676	rBV3	1552	1913	0.14%	0.014%
79	18.968	2696	2700	2704	rVB4	6840	9175	0.67%	0.067%
80	19.039	2708	2712	2716	rBV2	5792	8579	0.63%	0.063%
81	19.168	2732	2734	2737	rBV3	1780	1969	0.14%	0.014%
82	19.204	2738	2740	2745	rVB5	3960	5999	0.44%	0.044%
83	19.351	2764	2765	2768	rVB3	1854	1592	0.12%	0.012%
84	19.404	2768	2774	2785	rBV	814778	1142001	83.74%	8.322%
85	19.951	2865	2867	2868	rBV2	1753	1673	0.12%	0.012%
86	21.209	3075	3081	3094	rBV	487933	741746	54.39%	5.405%
87	23.262	3424	3430	3437	rBV2	743944	1363788	100.00%	9.938%
88	23.403	3448	3454	3465	rVB	445253	851734	62.45%	6.207%




Sum of corrected areas: 13723206

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045261.D
Acq On : 16 Apr 2024 02:15
Operator : MA/JU
Sample : PB160227BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK227

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

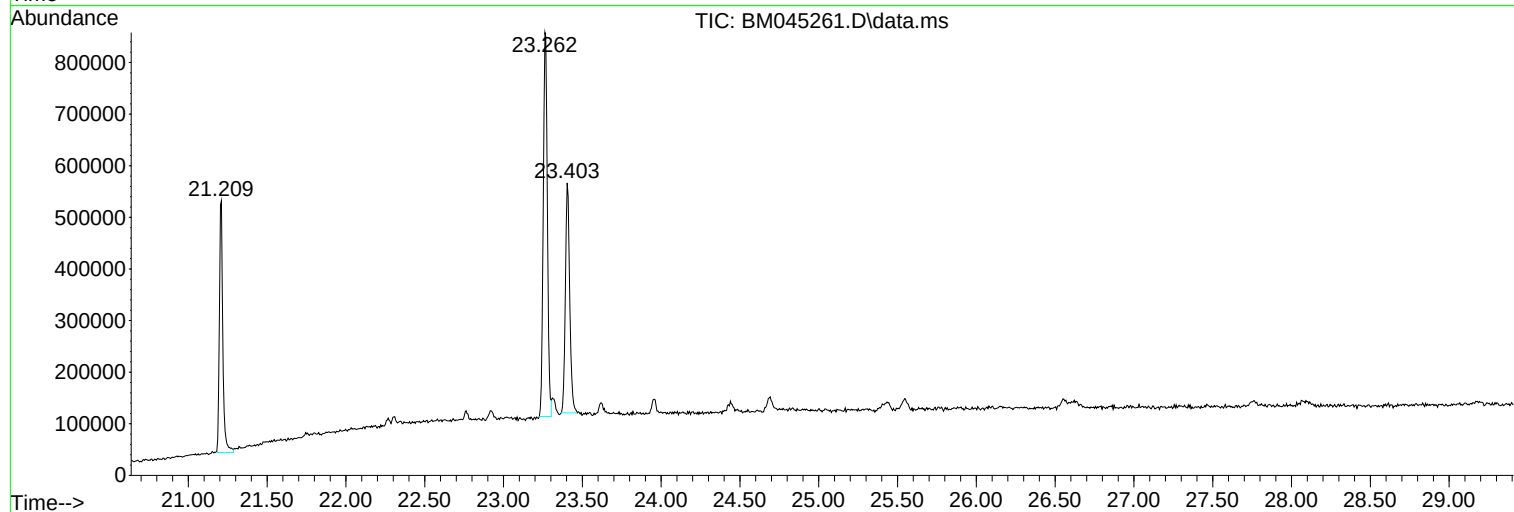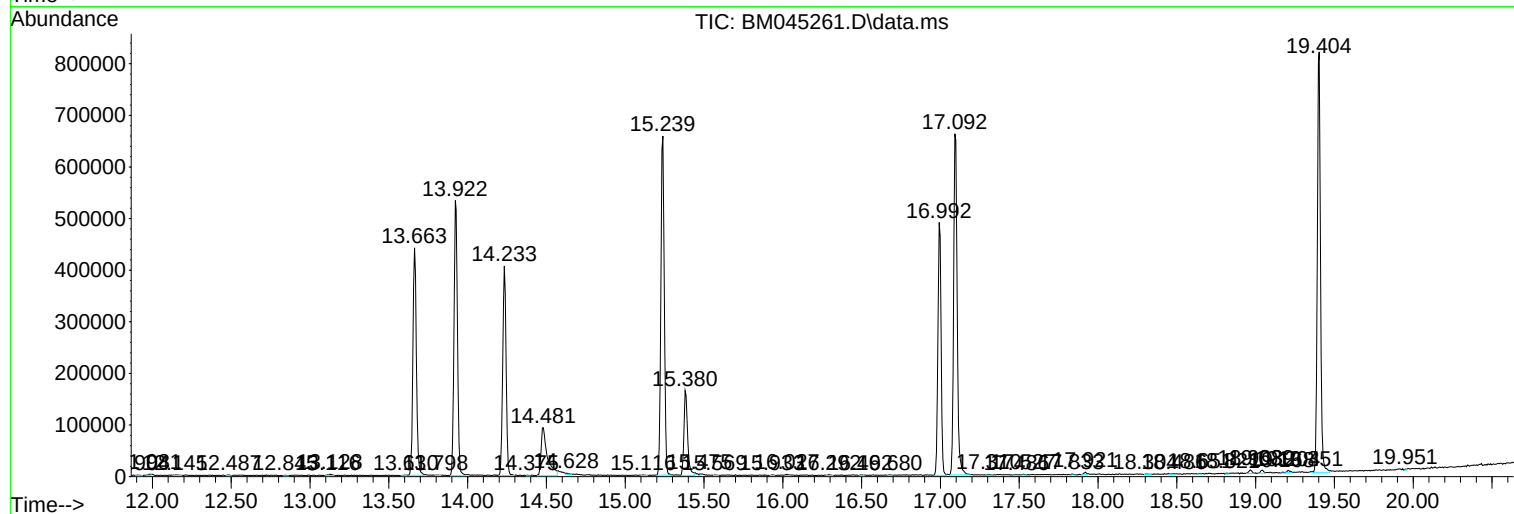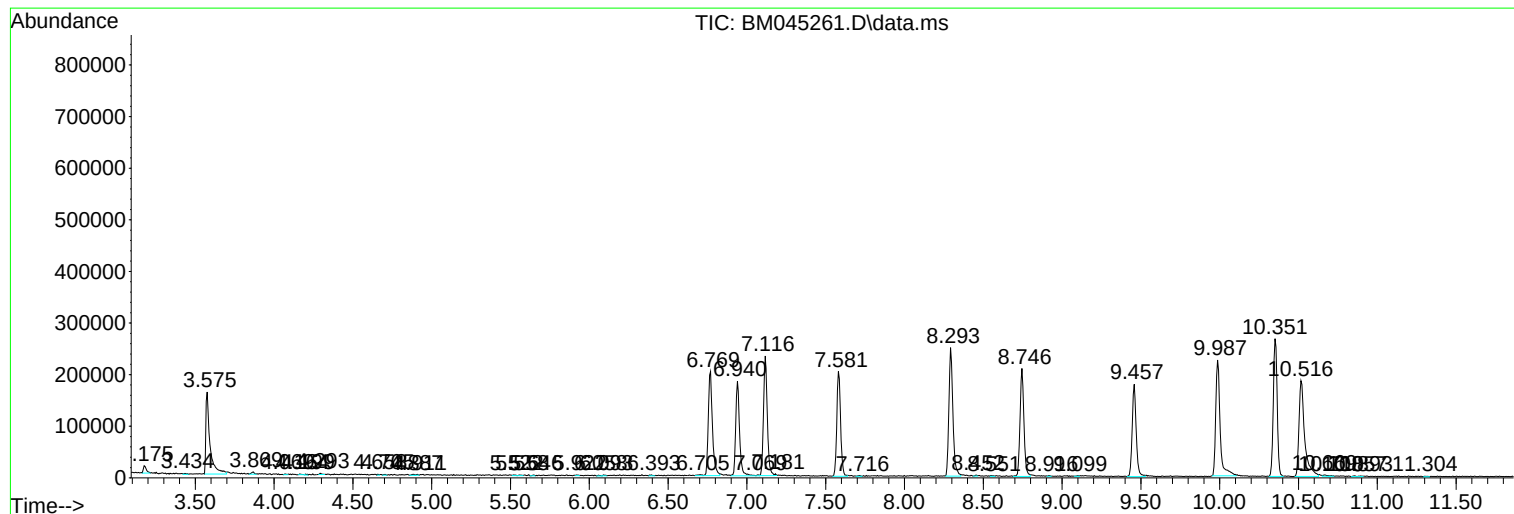

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045261.D
Acq On : 16 Apr 2024 02:15
Operator : MA/JU
Sample : PB160227BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK227

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045261.D
Acq On : 16 Apr 2024 02:15
Operator : MA/JU
Sample : PB160227BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK227

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------