

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045262.D
 Acq On : 16 Apr 2024 02:52
 Operator : MA/JU
 Sample : PB160228BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK228

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM045262.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	23	rBV	14696	21271	1.55%	0.151%
2	3.416	54	56	60	rVB5	1763	2047	0.15%	0.015%
3	3.575	79	83	103	rBV	157533	283773	20.71%	2.016%
4	3.863	129	132	137	rVB6	3988	5996	0.44%	0.043%
5	3.922	141	142	145	rBV3	2046	1587	0.12%	0.011%
6	4.063	161	166	169	rVB6	1776	2986	0.22%	0.021%
7	4.087	169	170	173	rBV3	2339	1691	0.12%	0.012%
8	4.222	192	193	196	rVB3	1853	1395	0.10%	0.010%
9	4.252	196	198	201	rBV2	1786	1739	0.13%	0.012%
10	4.310	201	208	215	rBV4	7093	18507	1.35%	0.131%
11	4.993	321	324	326	rVB3	1088	1383	0.10%	0.010%
12	5.569	419	422	423	rBV2	1666	1490	0.11%	0.011%
13	5.628	431	432	436	rVB3	1581	1521	0.11%	0.011%
14	5.657	436	437	440	rBV3	1490	1370	0.10%	0.010%
15	6.004	495	496	498	rBV	1656	1550	0.11%	0.011%
16	6.287	541	544	547	rVB3	1761	2330	0.17%	0.017%
17	6.493	574	579	584	rVV6	2360	5200	0.38%	0.037%
18	6.698	610	614	620	rVB3	5273	9501	0.69%	0.067%
19	6.763	620	625	637	rBV	197004	364897	26.64%	2.592%
20	6.940	649	655	667	rBV	190267	306679	22.39%	2.179%
21	7.063	673	676	678	rBV4	1429	1475	0.11%	0.010%
22	7.116	678	685	698	rVV	231845	390018	28.47%	2.771%
23	7.581	757	764	774	rVV	226978	368562	26.90%	2.618%
24	7.669	777	779	782	rVB2	1955	1805	0.13%	0.013%
25	8.081	848	849	855	rVB4	2162	1893	0.14%	0.013%
26	8.292	879	885	902	rBV2	256604	444451	32.44%	3.157%
27	8.457	911	913	918	rVV3	2487	3515	0.26%	0.025%
28	8.557	927	930	932	rBV2	1418	1452	0.11%	0.010%
29	8.745	955	962	972	rBV	206332	352983	25.77%	2.508%
30	8.869	980	983	988	rVB4	1388	2700	0.20%	0.019%
31	9.045	1011	1013	1016	rBV3	1513	1524	0.11%	0.011%
32	9.104	1019	1023	1028	rBV5	2364	4448	0.32%	0.032%
33	9.328	1058	1061	1063	rBV3	1090	1411	0.10%	0.010%
34	9.457	1074	1083	1095	rBV	176235	311215	22.72%	2.211%
35	9.987	1166	1173	1180	rBV	232782	416774	30.42%	2.961%
36	10.139	1196	1199	1201	rVB2	1768	1555	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
 Data File : BM045262.D
 Acq On : 16 Apr 2024 02:52
 Operator : MA/JU
 Sample : PB160228BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK228

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	10.292	1220	1225	1226	rBV4	1477	1860	0.14%	0.013%
38	10.351	1228	1235	1243	rVV	300723	496158	36.22%	3.525%
39	10.516	1254	1263	1283	rBV	196407	463575	33.84%	3.293%
40	11.098	1358	1362	1365	rBV4	1238	2340	0.17%	0.017%
41	11.539	1431	1437	1440	rVV3	2158	3927	0.29%	0.028%
42	11.581	1443	1444	1449	rVV2	1867	2296	0.17%	0.016%
43	11.628	1449	1452	1455	rVB3	1015	1402	0.10%	0.010%
44	11.998	1509	1515	1517	rBV4	2759	4629	0.34%	0.033%
45	12.557	1608	1610	1612	rBV2	1730	1661	0.12%	0.012%
46	13.133	1704	1708	1714	rVB8	3888	5251	0.38%	0.037%
47	13.663	1791	1798	1810	rVV	466968	677889	49.48%	4.816%
48	13.922	1836	1842	1854	rBV	532367	807230	58.93%	5.734%
49	14.233	1888	1895	1903	rBV	455283	653753	47.72%	4.644%
50	14.474	1931	1936	1956	rBV	95323	262951	19.19%	1.868%
51	14.721	1977	1978	1983	rVB4	1430	1670	0.12%	0.012%
52	14.827	1993	1996	1999	rVB3	1327	1370	0.10%	0.010%
53	14.980	2020	2022	2025	rBV3	1396	1589	0.12%	0.011%
54	15.033	2028	2031	2034	rVV3	1906	3135	0.23%	0.022%
55	15.239	2059	2066	2074	rBV	660254	999915	72.99%	7.103%
56	15.292	2074	2075	2079	rVB3	1732	2152	0.16%	0.015%
57	15.380	2084	2090	2103	rBV	160131	261971	19.12%	1.861%
58	15.657	2134	2137	2140	rVB4	2055	2389	0.17%	0.017%
59	15.898	2174	2178	2182	rBV2	1261	1949	0.14%	0.014%
60	16.033	2196	2201	2204	rBV4	2206	2948	0.22%	0.021%
61	16.774	2322	2327	2328	rBV2	1129	1374	0.10%	0.010%
62	16.845	2336	2339	2345	rVB4	1473	1811	0.13%	0.013%
63	16.992	2358	2364	2374	rBV	553214	734155	53.59%	5.215%
64	17.092	2375	2381	2396	rVB2	692099	1032618	75.38%	7.336%
65	17.639	2471	2474	2476	rVB	1314	1419	0.10%	0.010%
66	17.698	2481	2484	2487	rVV3	1449	1747	0.13%	0.012%
67	17.833	2504	2507	2510	rVB3	1173	1409	0.10%	0.010%
68	17.921	2517	2522	2528	rVV6	3721	6549	0.48%	0.047%
69	18.492	2617	2619	2622	rVB4	1458	1411	0.10%	0.010%
70	18.780	2662	2668	2673	rBV6	1354	3171	0.23%	0.023%
71	18.968	2695	2700	2705	rBV6	7801	11060	0.81%	0.079%
72	19.039	2708	2712	2716	rVV3	5899	7373	0.54%	0.052%
73	19.215	2738	2742	2744	rBV5	3002	3920	0.29%	0.028%
74	19.404	2767	2774	2786	rBV	813429	1141984	83.36%	8.112%
75	19.915	2858	2861	2864	rBV4	2614	3472	0.25%	0.025%
76	20.427	2945	2948	2952	rBV4	16421	22183	1.62%	0.158%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045262.D
Acq On : 16 Apr 2024 02:52
Operator : MA/JU
Sample : PB160228BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK228

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

77	20.551	2967	2969	2970	rBV2	4131	3074	0.22%	0.022%
78	21.209	3076	3081	3091	rBV	564363	787451	57.48%	5.594%
79	23.268	3424	3431	3437	rBV2	770375	1369919	100.00%	9.732%
80	23.403	3448	3454	3465	rBV	472249	934142	68.19%	6.636%




Sum of corrected areas: 14076946

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045262.D
Acq On : 16 Apr 2024 02:52
Operator : MA/JU
Sample : PB160228BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK228

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

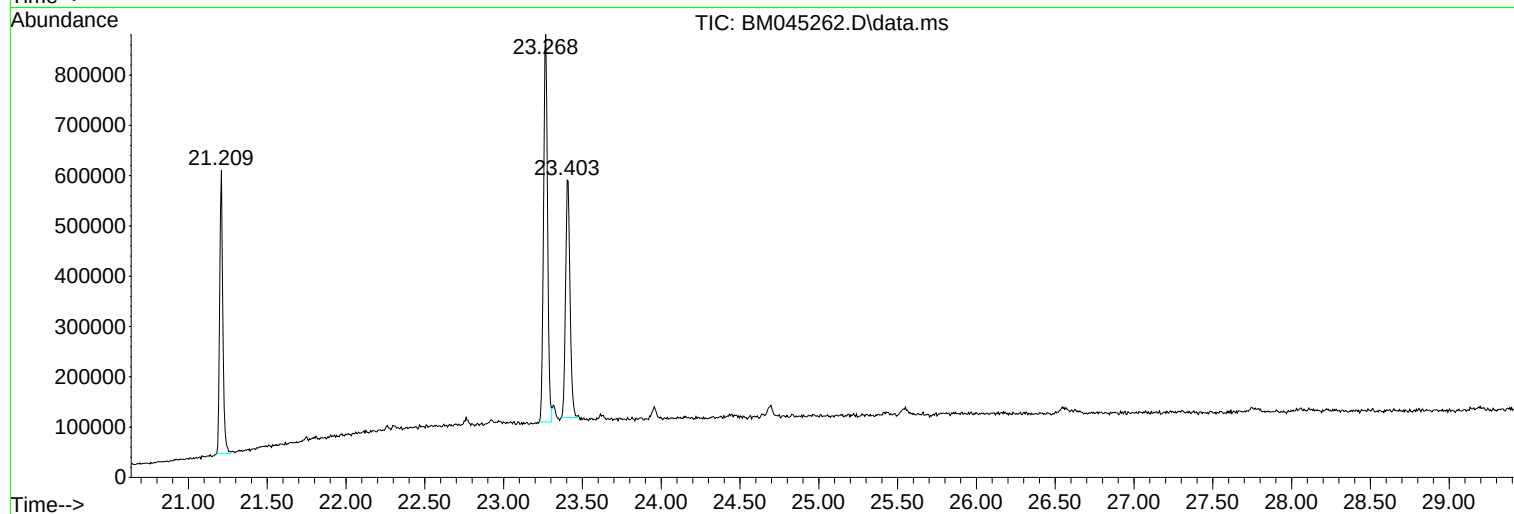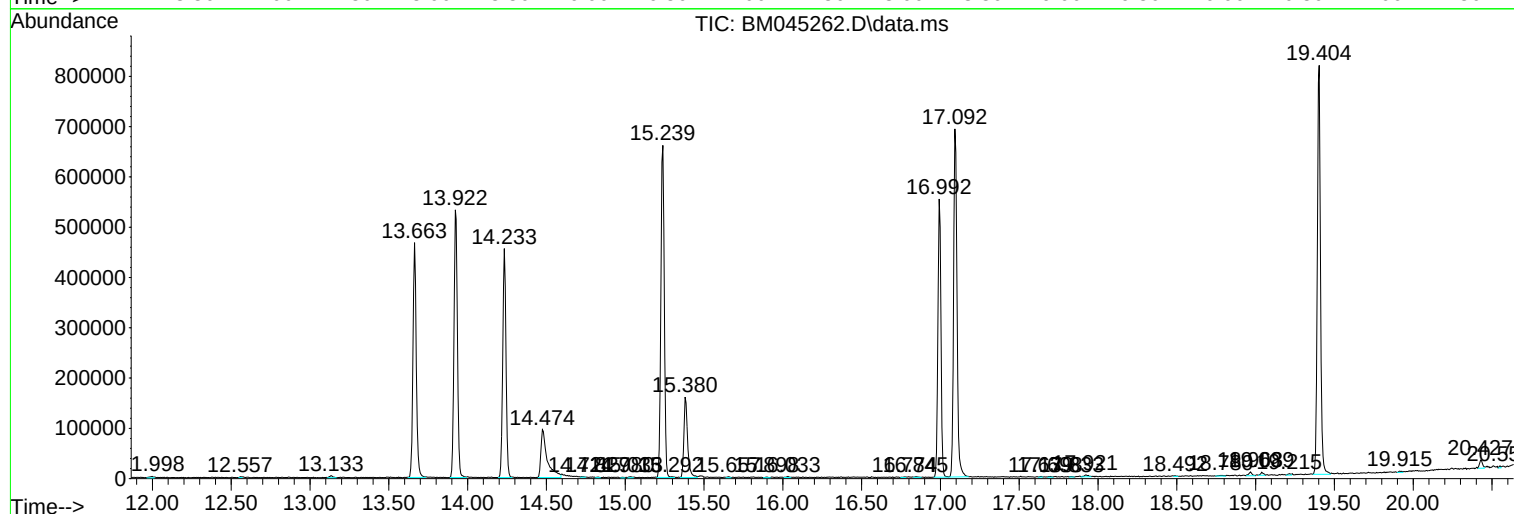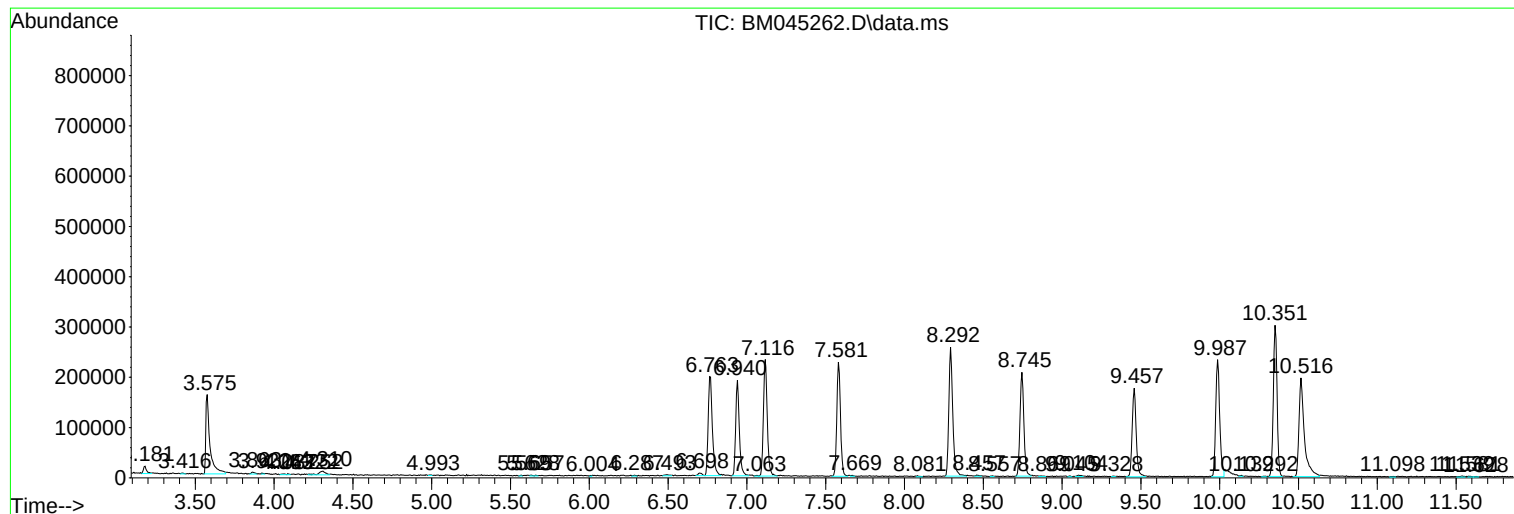

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045262.D
Acq On : 16 Apr 2024 02:52
Operator : MA/JU
Sample : PB160228BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK228

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041524\
Data File : BM045262.D
Acq On : 16 Apr 2024 02:52
Operator : MA/JU
Sample : PB160228BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK228

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc